

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061120\
Data File : FB024446.D
Signal(s) : FID2B.CH
Acq On : 11 Jun 2020 11:02
Operator : DD/AJ
Sample : L2970-01
Misc : 5.05gm/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 12 01:49:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	395438	16.344 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.413	1330	0.040 ng/ml
4) t Benzene	7.901	5811	0.144 ng/ml
6) t Toluene	10.632	60219	1.532 ng/ml
7) t Ethylbenzene	13.080	2289	0.065 ng/ml
8) t m-Xylene	13.200	3039	0.089 ng/ml
9) t O-Xylene	13.890	1296	0.039 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061120\
Data File : FB024446.D
Signal(s) : FID2B.CH
Acq On : 11 Jun 2020 11:02
Operator : DD/AJ
Sample : L2970-01
Misc : 5.05gm/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 12 01:49:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

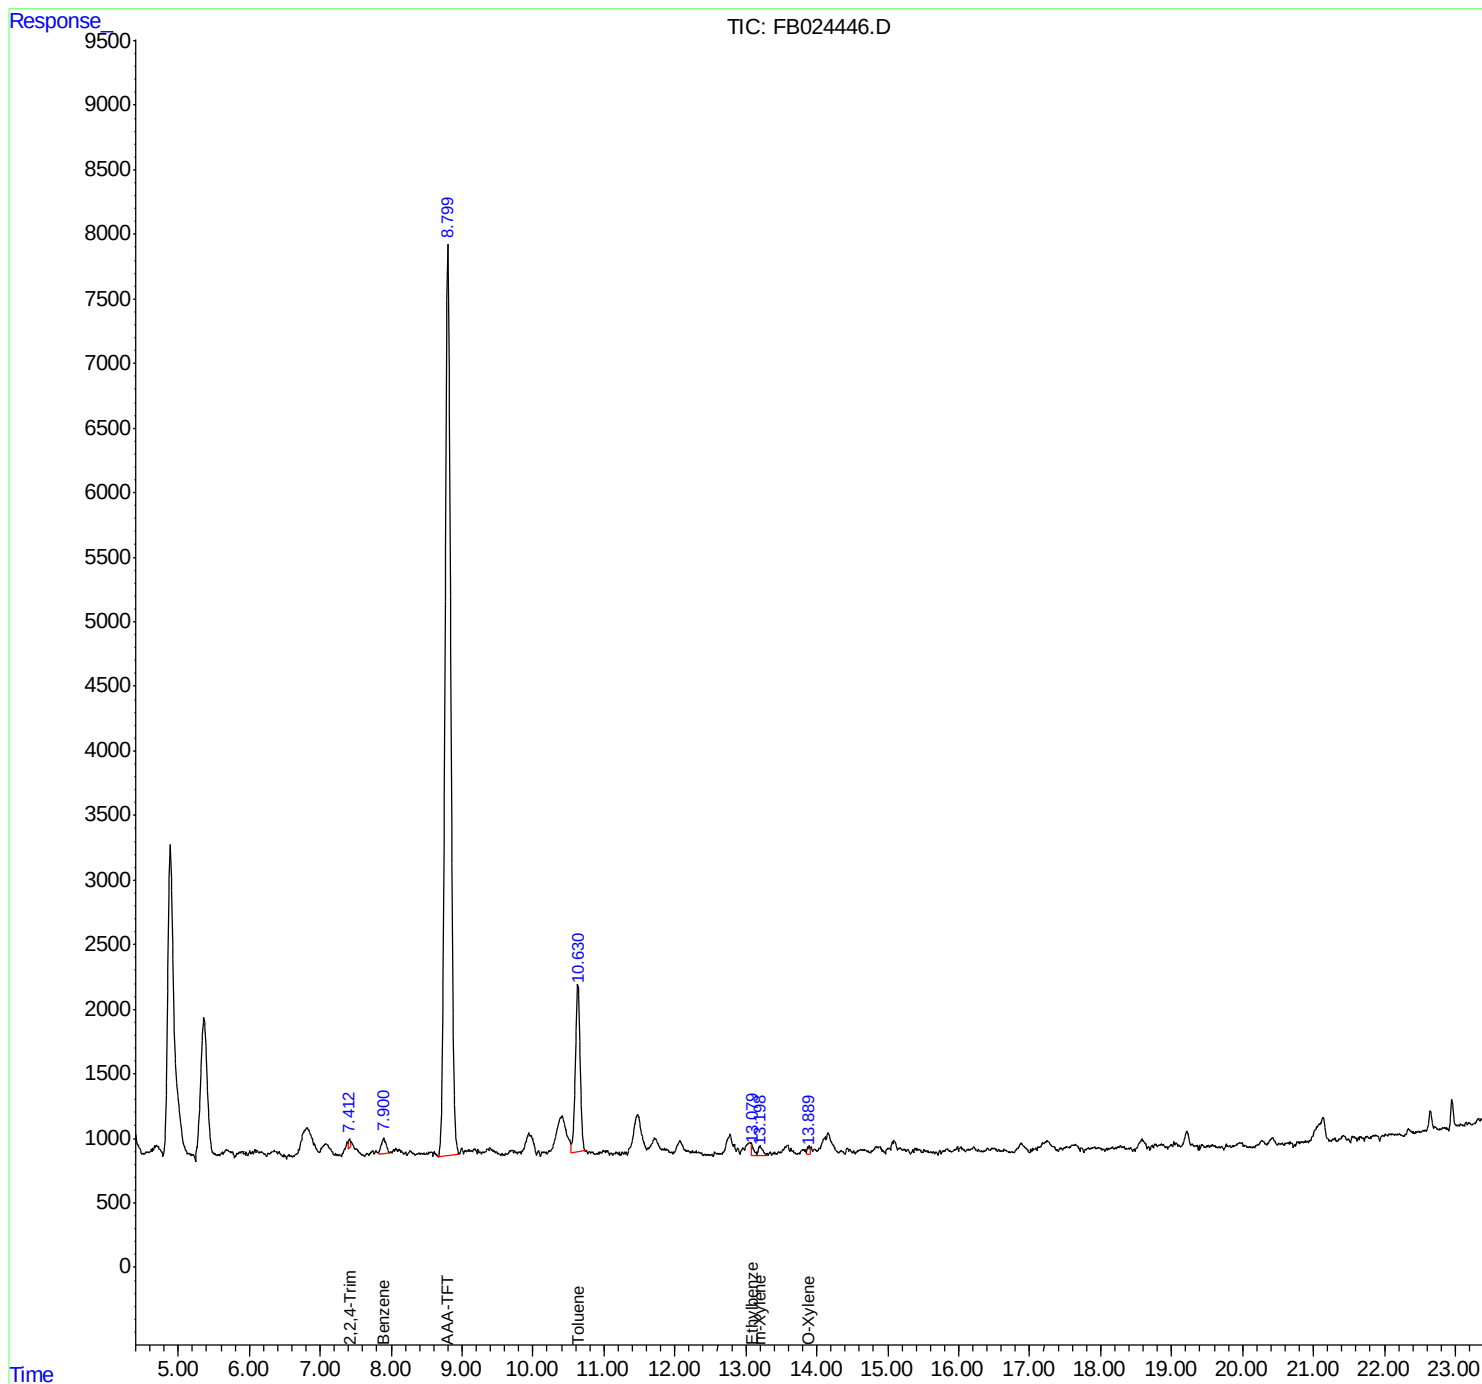

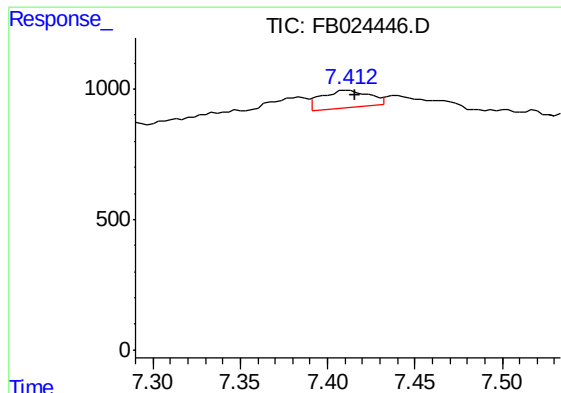


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.003 min
Response: 1330
Conc: 0.04 ng/ml

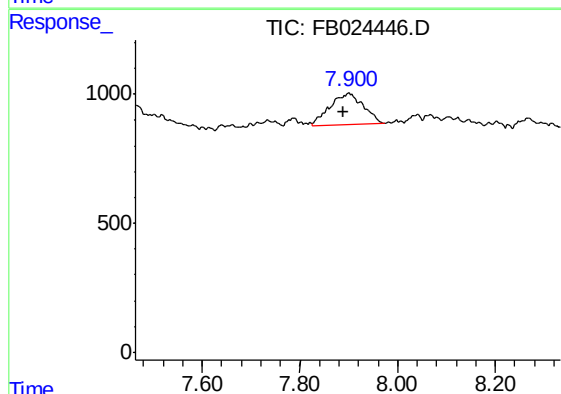


#4 Benzene

R.T.: 7.901 min
Delta R.T.: 0.011 min
Response: 5811
Conc: 0.14 ng/ml

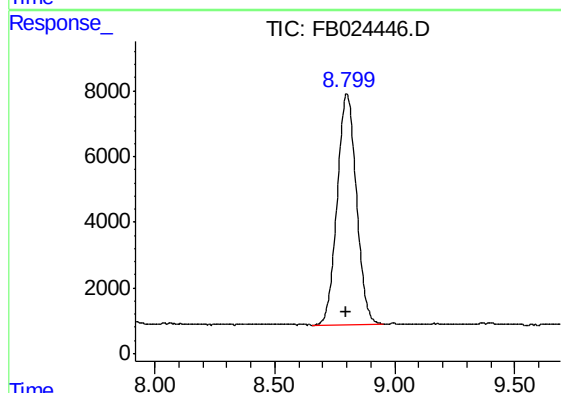


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.004 min
Response: 395438
Conc: 16.34 ng/ml

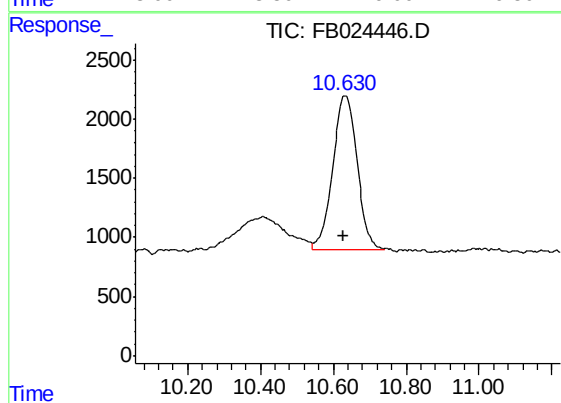


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.004 min
Response: 60219
Conc: 1.53 ng/ml

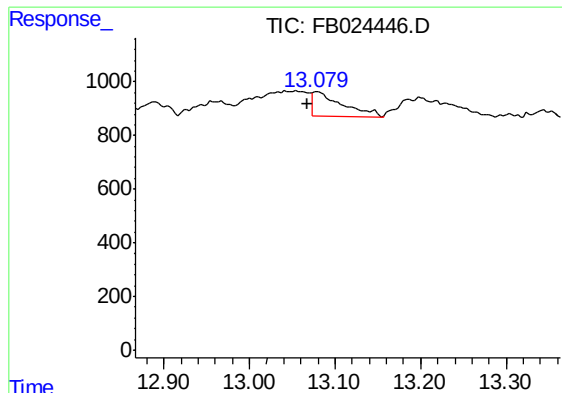


#7 Ethylbenzene

R.T.: 13.080 min
Delta R.T.: 0.012 min
Response: 2289
Conc: 0.07 ng/ml

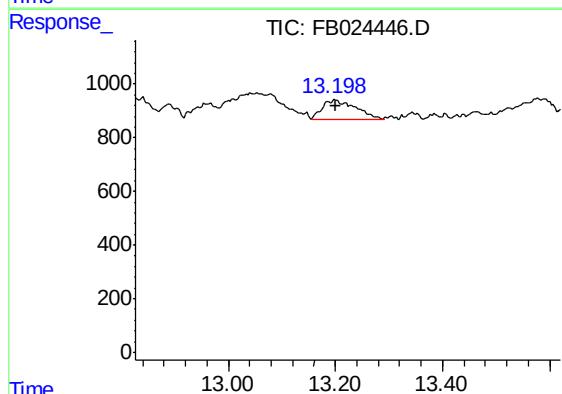

#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.001 min
Response: 3039
Conc: 0.09 ng/ml

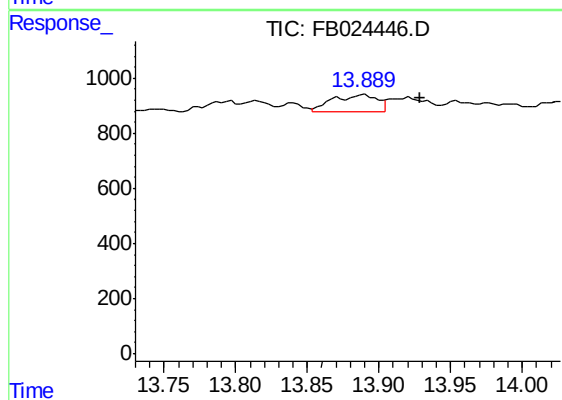

#9 O-Xylene

R.T.: 13.890 min
Delta R.T.: -0.039 min
Response: 1296
Conc: 0.04 ng/ml