

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061120\
 Data File : FB024444.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jun 2020 10:01
 Operator : DD/AJ
 Sample : BSF0611S1
 Misc : 5.00gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 12 01:49:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	389098	16.082 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	849608	26.581 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	902647	26.925 ng/ml
3) t n-Heptane	7.759	296821	8.777 ng/ml
4) t Benzene	7.893	353384	8.742 ng/ml
6) t Toluene	10.631	1080227	27.488 ng/ml
7) t Ethylbenzene	13.071	310518	8.849 ng/ml
8) t m-Xylene	13.204	604746	17.659 ng/ml
9) t O-Xylene	13.932	591657	17.647 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	497691	17.925 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061120\
Data File : FB024444.D
Signal(s) : FID2B.CH
Acq On : 11 Jun 2020 10:01
Operator : DD/AJ
Sample : BSF0611S1
Misc : 5.00gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 12 01:49:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

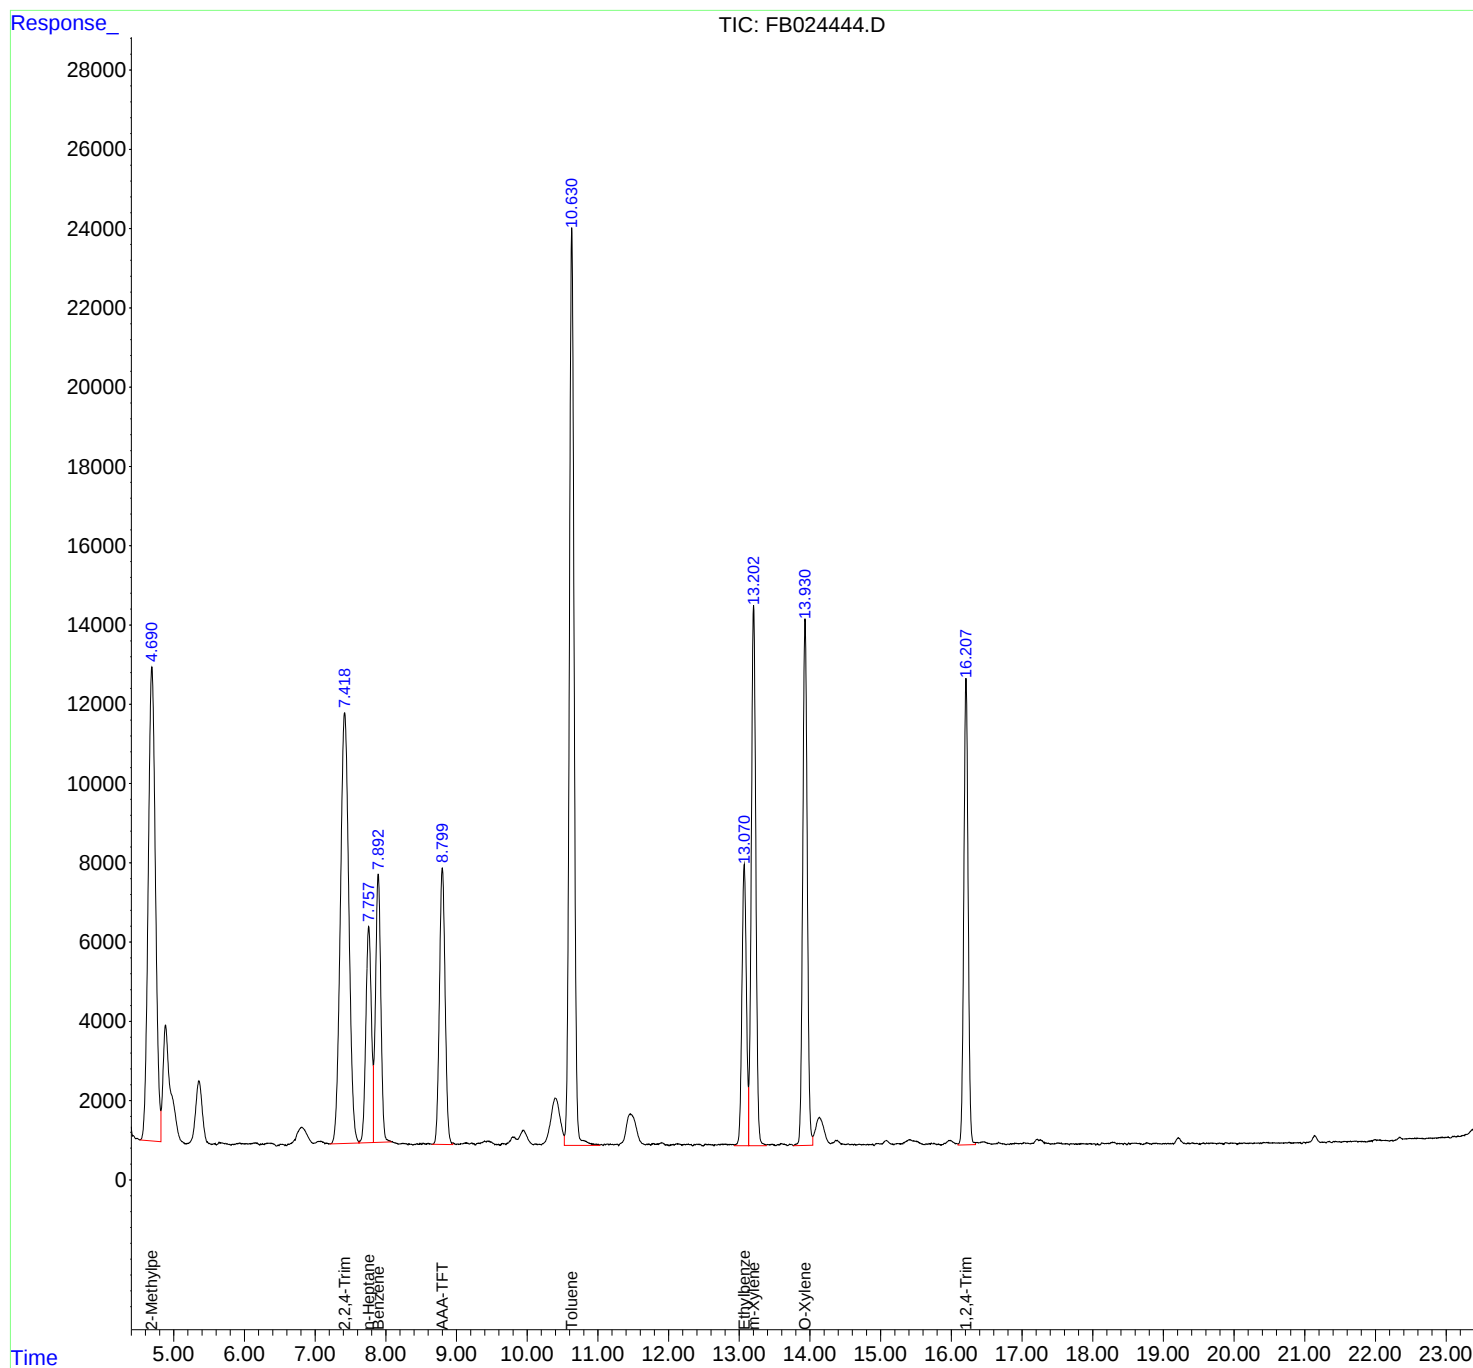

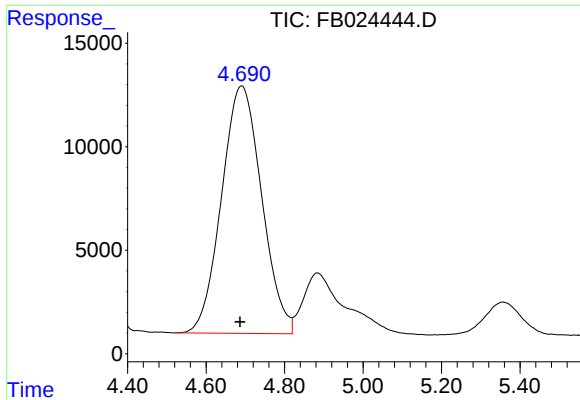


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.004 min
Response: 849608
Conc: 26.58 ng/ml

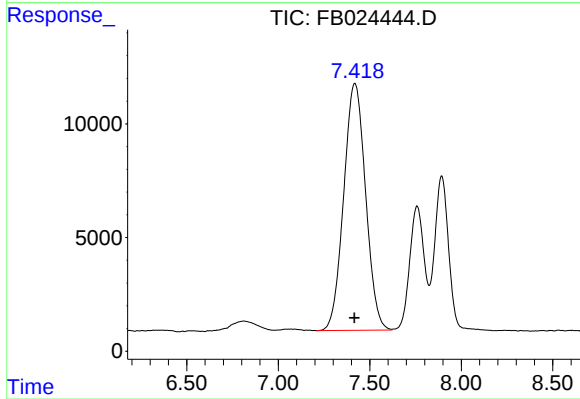


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 902647
Conc: 26.93 ng/ml

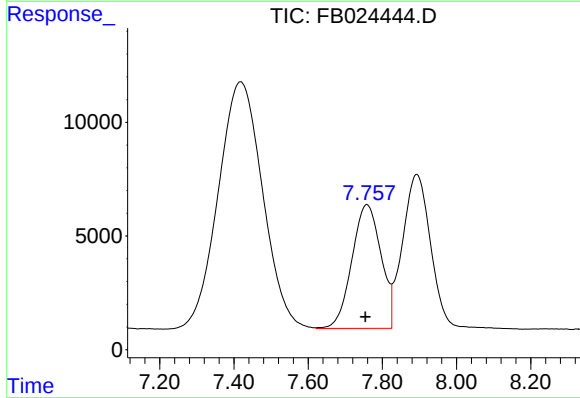


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 296821
Conc: 8.78 ng/ml

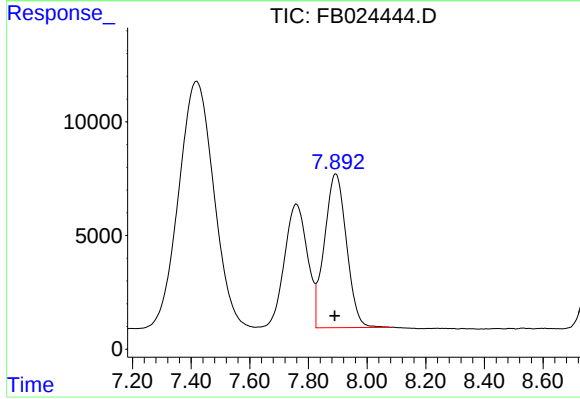


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.003 min
Response: 353384
Conc: 8.74 ng/ml

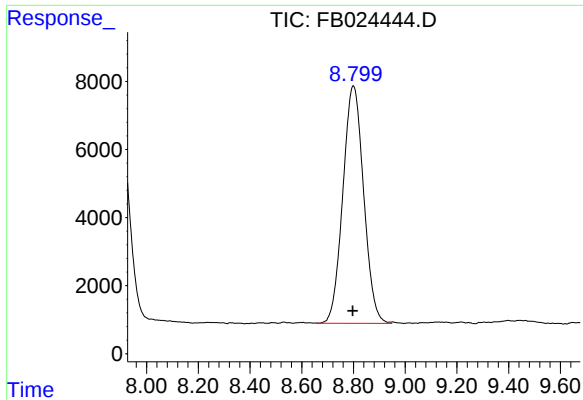


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 389098
Conc: 16.08 ng/ml

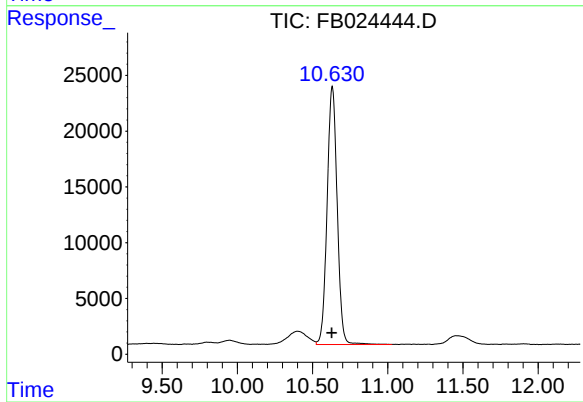


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.003 min
Response: 1080227
Conc: 27.49 ng/ml

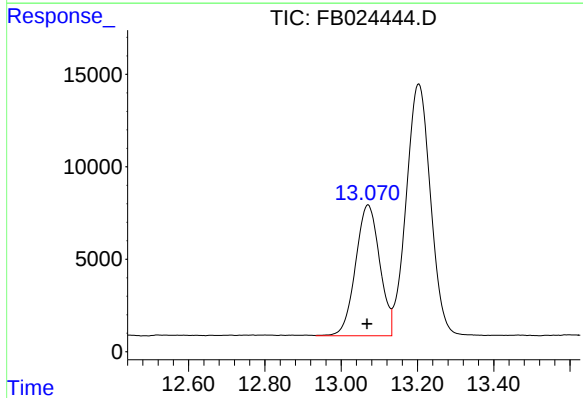


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.003 min
Response: 310518
Conc: 8.85 ng/ml

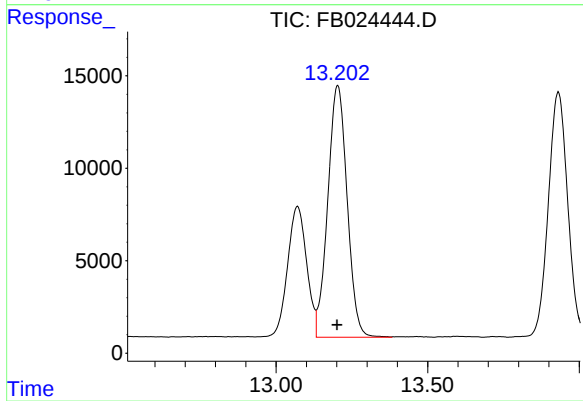


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 604746
Conc: 17.66 ng/ml

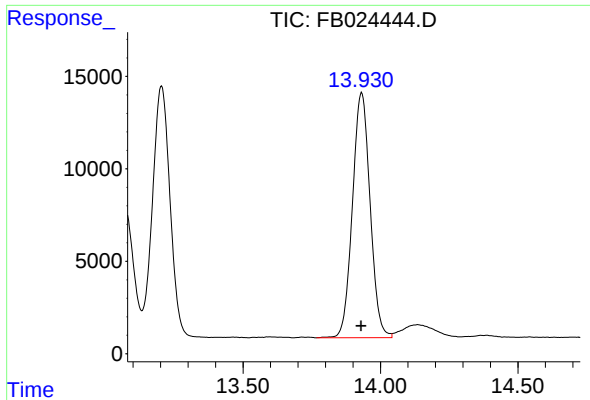

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.003 min
Response: 591657
Conc: 17.65 ng/ml

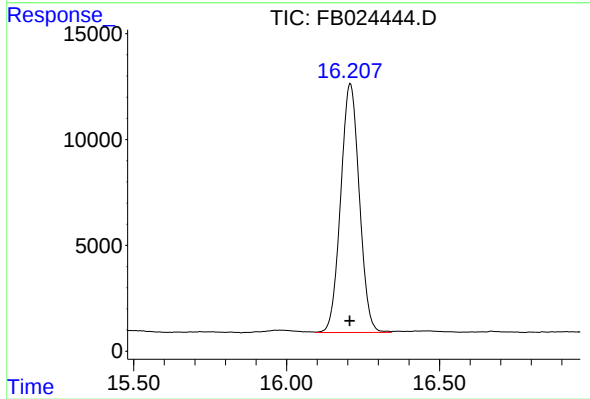

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.002 min
Response: 497691
Conc: 17.92 ng/ml