

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061219\
 Data File : FB021364.D
 Signal(s) : FID2B.CH
 Acq On : 12 Jun 2019 9:34
 Operator : MJ/SJ
 Sample : BSF0612S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 13 01:55:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	297686	20.190 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	955799	25.425 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	1045011	30.600 ng/ml
3) t n-Heptane	7.947	328101	10.064 ng/ml
4) t Benzene	8.086	314245	9.104 ng/ml
6) t Toluene	10.837	747542	31.539 ng/ml
7) t Ethylbenzene	13.287	254406	10.887 ng/ml
8) t m-Xylene	13.420	540530	21.656 ng/ml
9) t O-Xylene	14.151	560047	21.469 ng/ml
10) t 1,2,4-Trimethylbenzene	16.436	566091	21.079 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061219\
Data File : FB021364.D
Signal(s) : FID2B.CH
Acq On : 12 Jun 2019 9:34
Operator : MJ/SJ
Sample : BSF0612S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 13 01:55:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

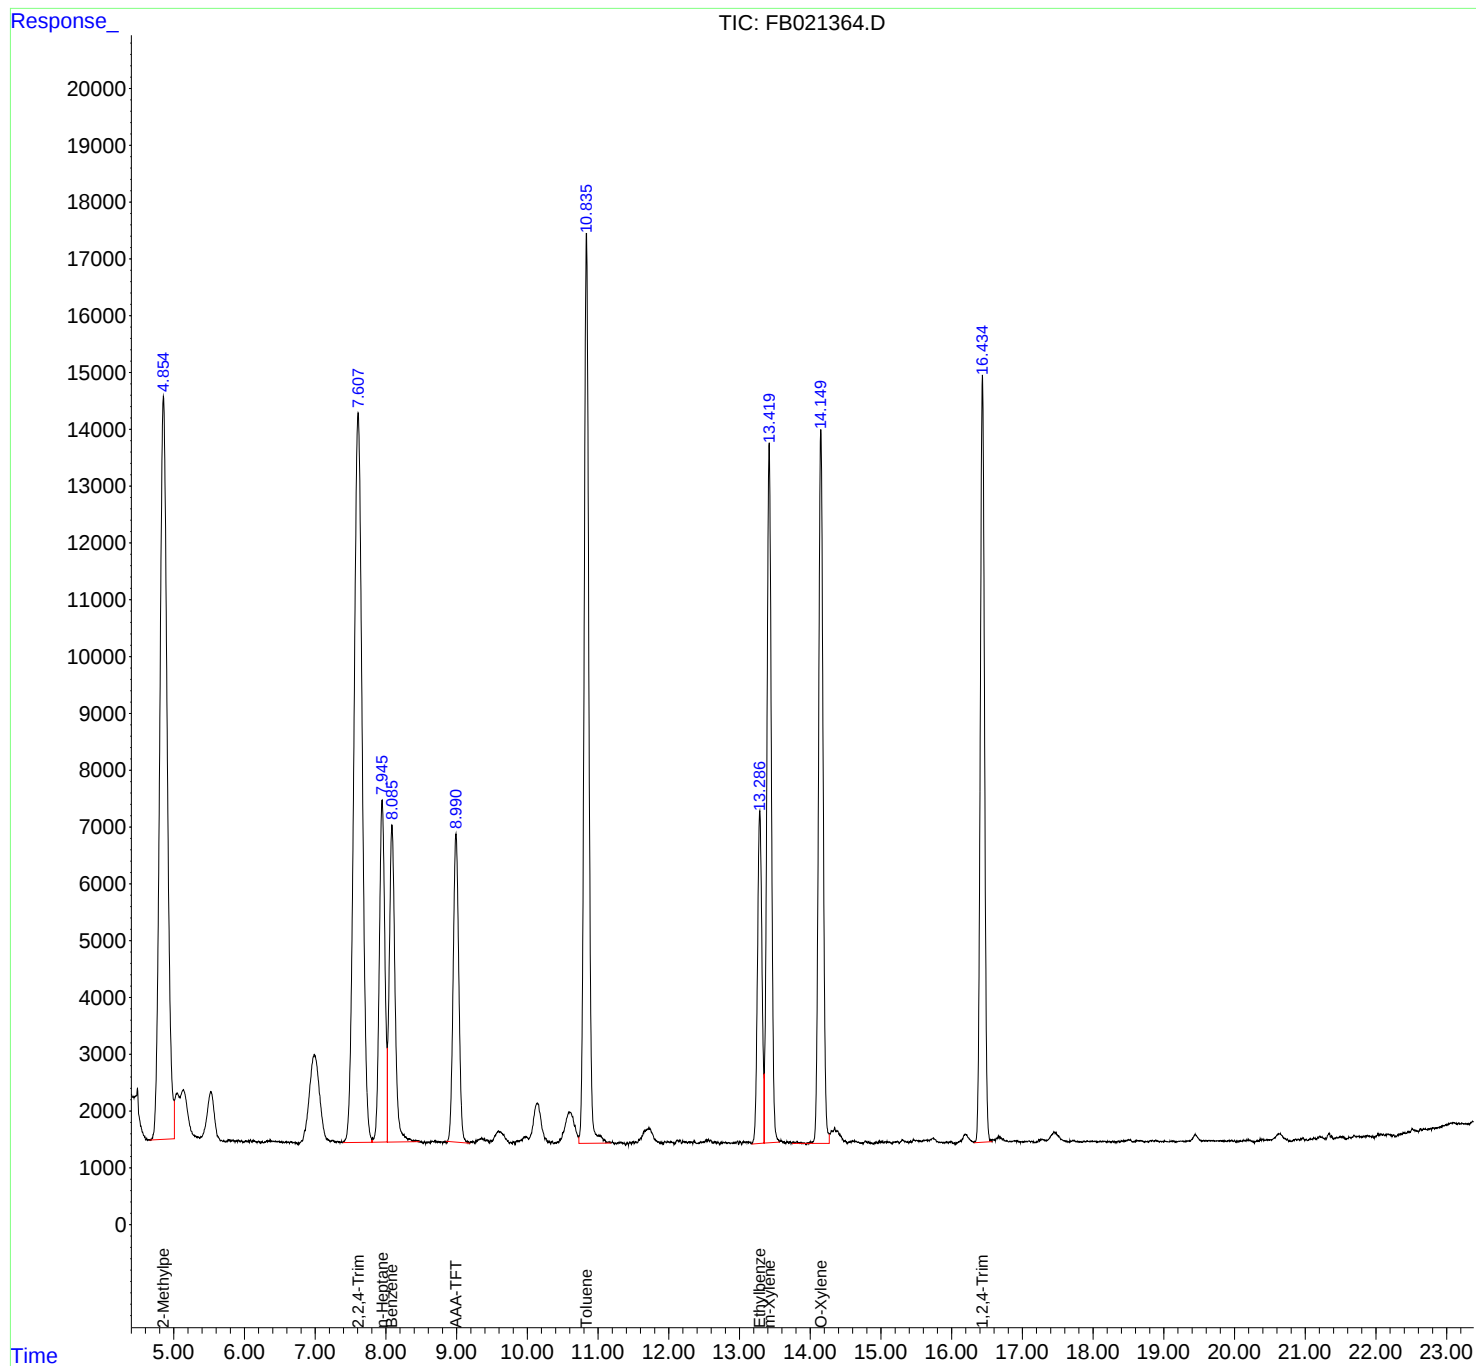

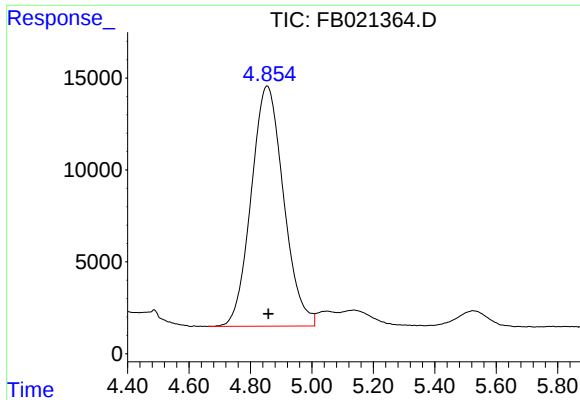


#1 2-Methylpentane

R.T.: 4.855 min
Delta R.T.: -0.003 min
Response: 955799
Conc: 25.42 ng/ml

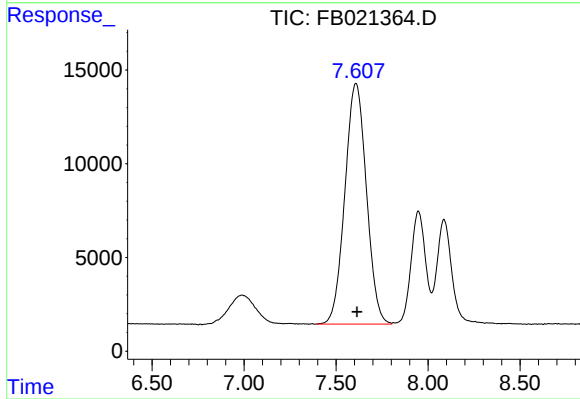


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: -0.006 min
Response: 1045011
Conc: 30.60 ng/ml

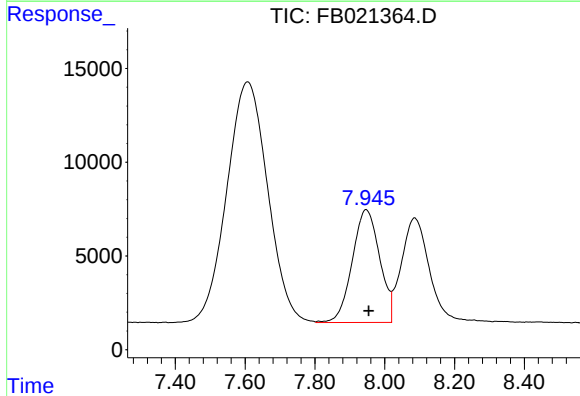


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: -0.007 min
Response: 328101
Conc: 10.06 ng/ml

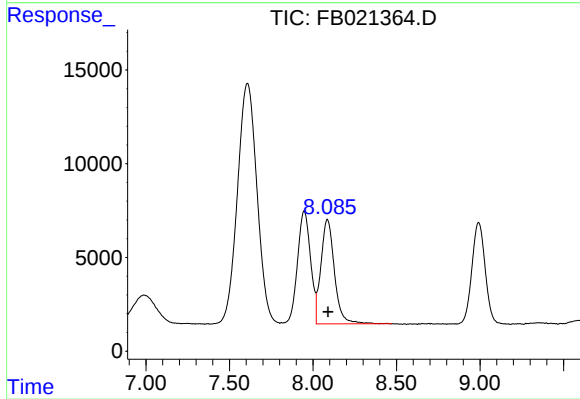


#4 Benzene

R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 314245
Conc: 9.10 ng/ml

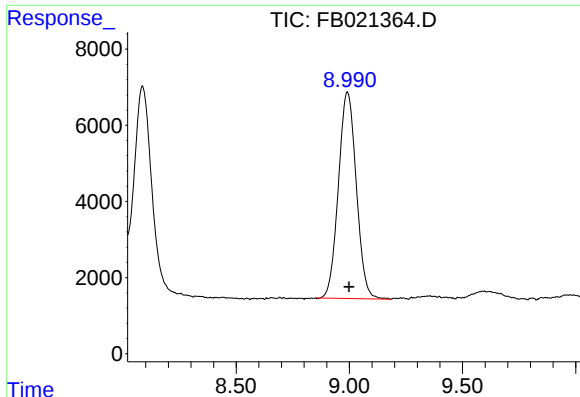


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: -0.007 min
Response: 297686
Conc: 20.19 ng/ml

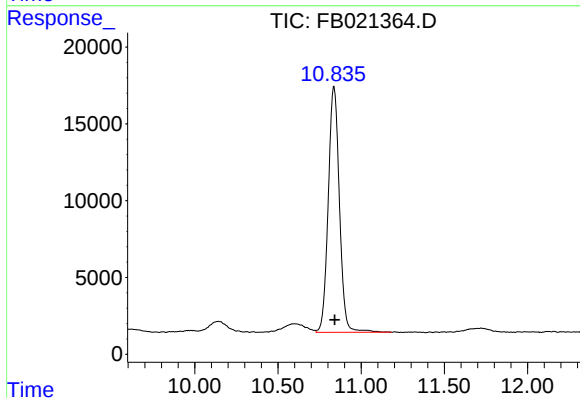


#6 Toluene

R.T.: 10.837 min
Delta R.T.: -0.006 min
Response: 747542
Conc: 31.54 ng/ml

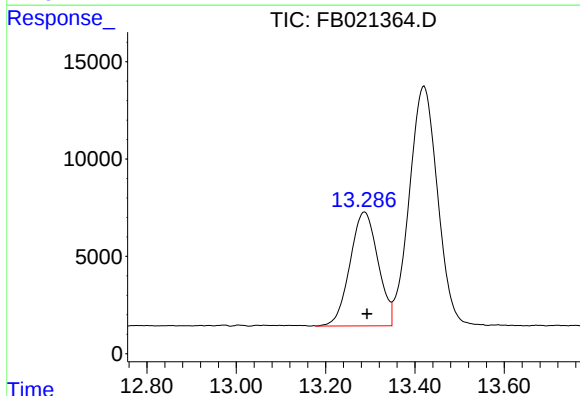


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: -0.006 min
Response: 254406
Conc: 10.89 ng/ml

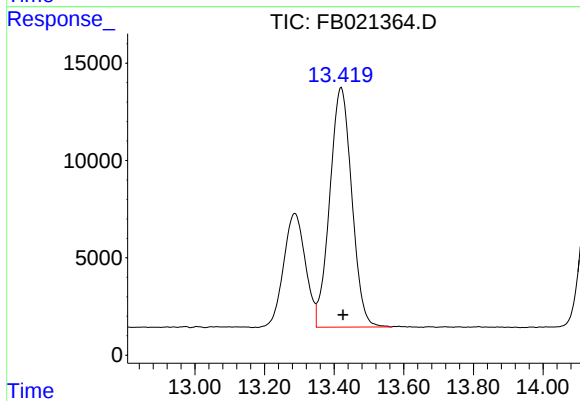

#8 m-Xylene

R.T.: 13.420 min
Delta R.T.: -0.005 min
Response: 540530
Conc: 21.66 ng/ml

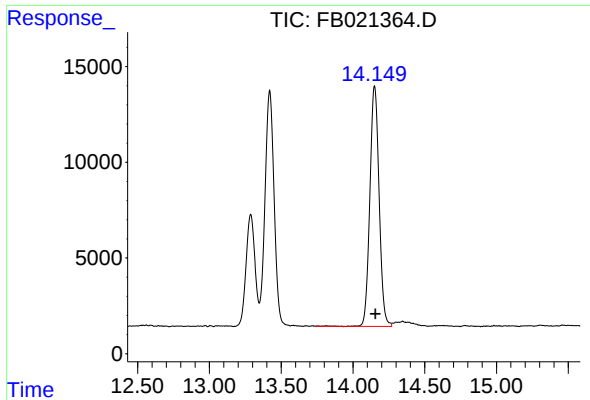


#9 O-Xylene

R.T.: 14.151 min

Delta R.T.: -0.006 min

Response: 560047

Conc: 21.47 ng/ml

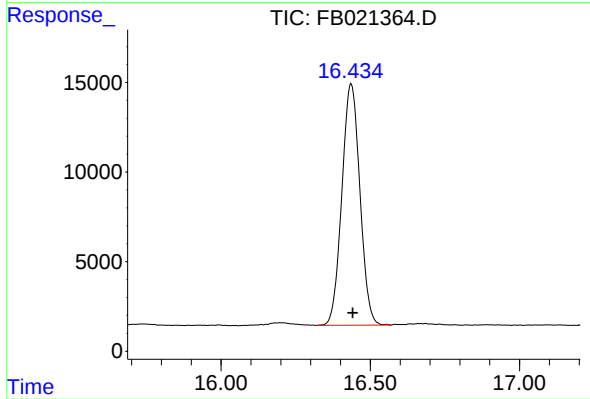

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min

Delta R.T.: -0.005 min

Response: 566091

Conc: 21.08 ng/ml