

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061219\
 Data File : FB021369.D
 Signal(s) : FID2B.CH
 Acq On : 12 Jun 2019 13:05
 Operator : MJ/SJ
 Sample : K3159-03MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 13 01:56:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	284197	19.275 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.857	704031	18.727 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	554486	16.237 ng/ml
3) t n-Heptane	7.950	108007	3.313 ng/ml
4) t Benzene	8.090	286758	8.308 ng/ml
6) t Toluene	10.840	661446	27.906 ng/ml
7) t Ethylbenzene	13.290	194654	8.330 ng/ml
8) t m-Xylene	13.423	387555	15.527 ng/ml
9) t O-Xylene	14.154	427514	16.388 ng/ml
10) t 1,2,4-Trimethylbenzene	16.439	249077	9.275 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061219\
Data File : FB021369.D
Signal(s) : FID2B.CH
Acq On : 12 Jun 2019 13:05
Operator : MJ/SJ
Sample : K3159-03MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 13 01:56:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

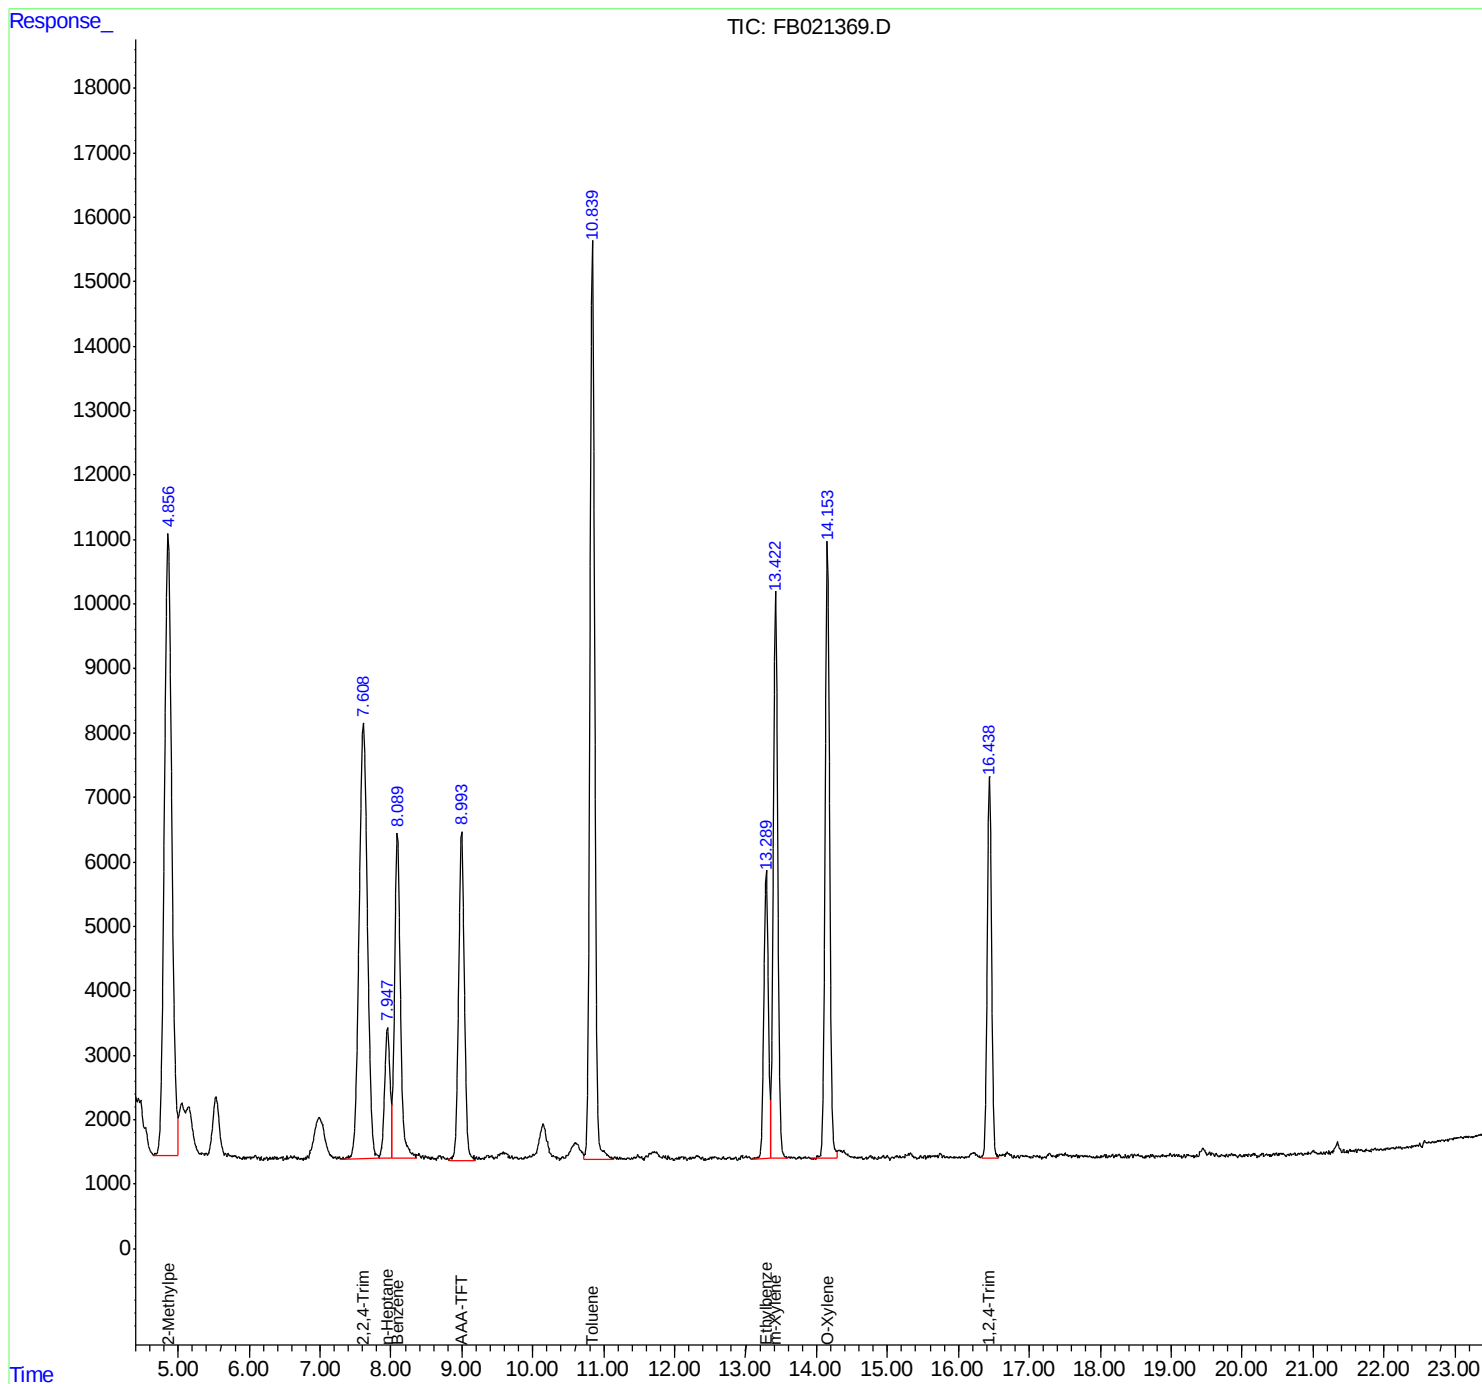

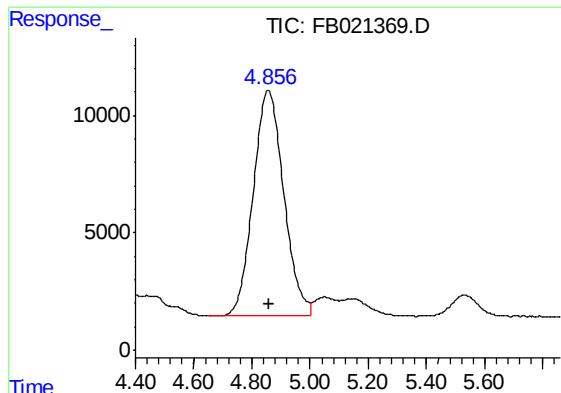


#1 2-Methylpentane

R.T.: 4.857 min
Delta R.T.: -0.001 min
Response: 704031
Conc: 18.73 ng/ml

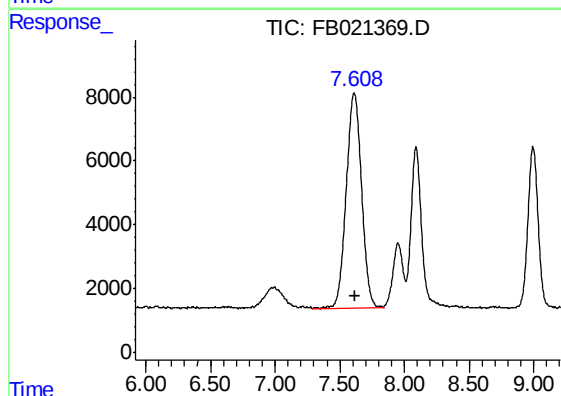


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.003 min
Response: 554486
Conc: 16.24 ng/ml

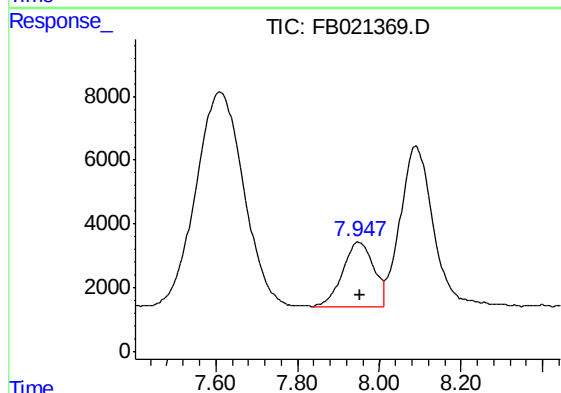


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 108007
Conc: 3.31 ng/ml

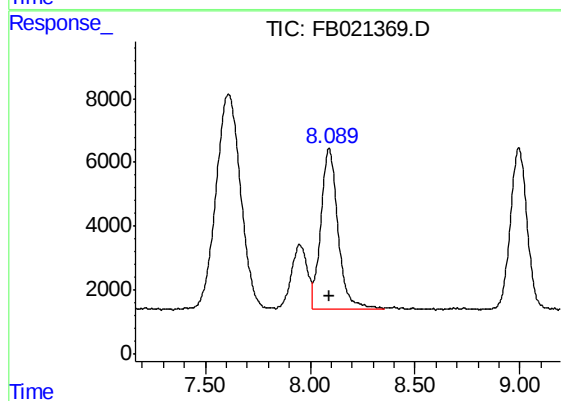


#4 Benzene

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 286758
Conc: 8.31 ng/ml

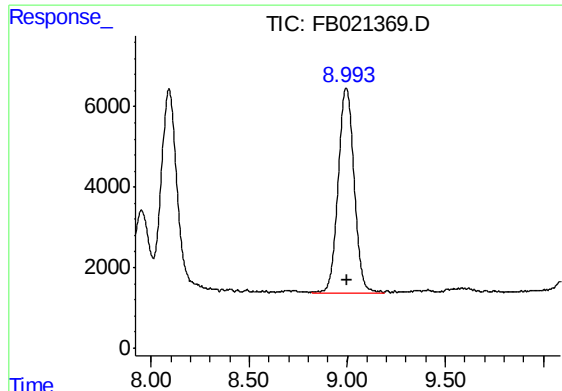


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 284197
Conc: 19.28 ng/ml

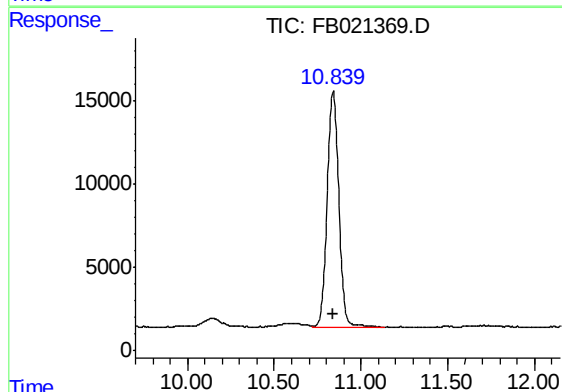


#6 Toluene

R.T.: 10.840 min
Delta R.T.: -0.003 min
Response: 661446
Conc: 27.91 ng/ml

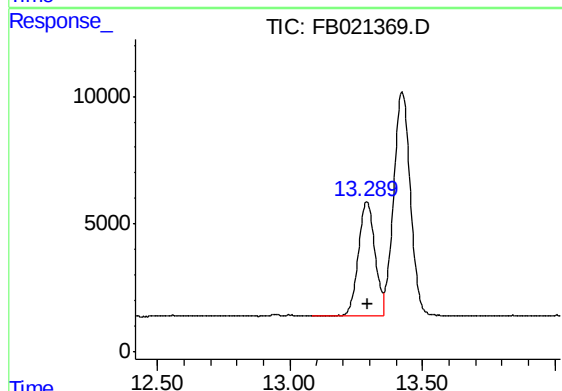


#7 Ethylbenzene

R.T.: 13.290 min
Delta R.T.: -0.003 min
Response: 194654
Conc: 8.33 ng/ml

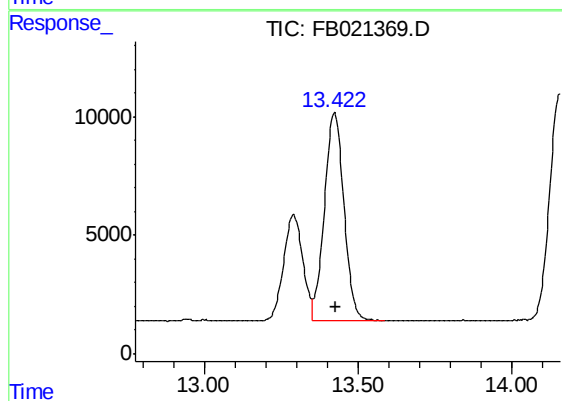


#8 m-Xylene

R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 387555
Conc: 15.53 ng/ml

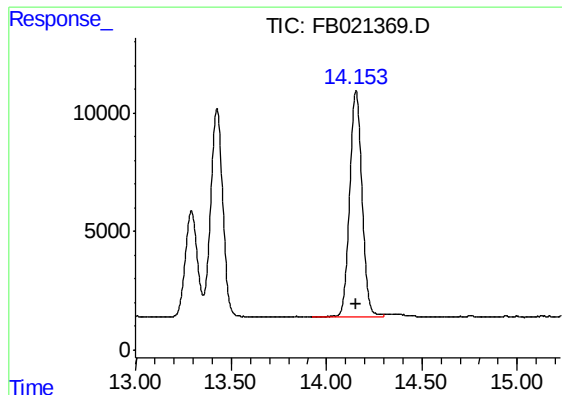

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: -0.003 min
Response: 427514
Conc: 16.39 ng/ml

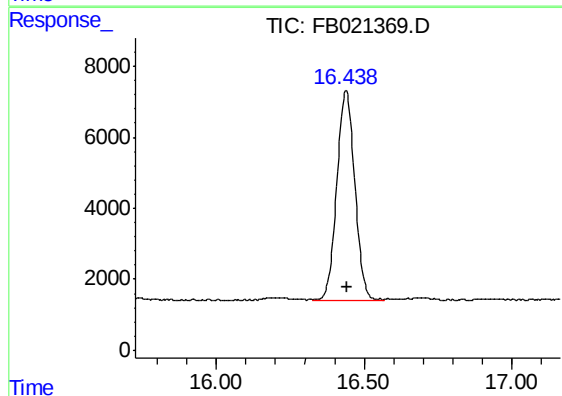

#10 1,2,4-Trimethylbenzene

R.T.: 16.439 min
Delta R.T.: -0.002 min
Response: 249077
Conc: 9.27 ng/ml