

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061319\
 Data File : FB021376.D
 Signal(s) : FID2B.CH
 Acq On : 13 Jun 2019 11:08
 Operator : MJ/SJ
 Sample : K3156-03MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 14 00:35:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	285326	19.352 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.859	749439	19.935 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	763367	22.353 ng/ml
3) t n-Heptane	7.952	237594	7.288 ng/ml
4) t Benzene	8.092	287298	8.323 ng/ml
6) t Toluene	10.841	673479	28.414 ng/ml
7) t Ethylbenzene	13.292	206858	8.853 ng/ml
8) t m-Xylene	13.425	437110	17.512 ng/ml
9) t O-Xylene	14.156	462801	17.741 ng/ml
10) t 1,2,4-Trimethylbenzene	16.441	446999	16.645 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061319\
Data File : FB021376.D
Signal(s) : FID2B.CH
Acq On : 13 Jun 2019 11:08
Operator : MJ/SJ
Sample : K3156-03MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 14 00:35:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

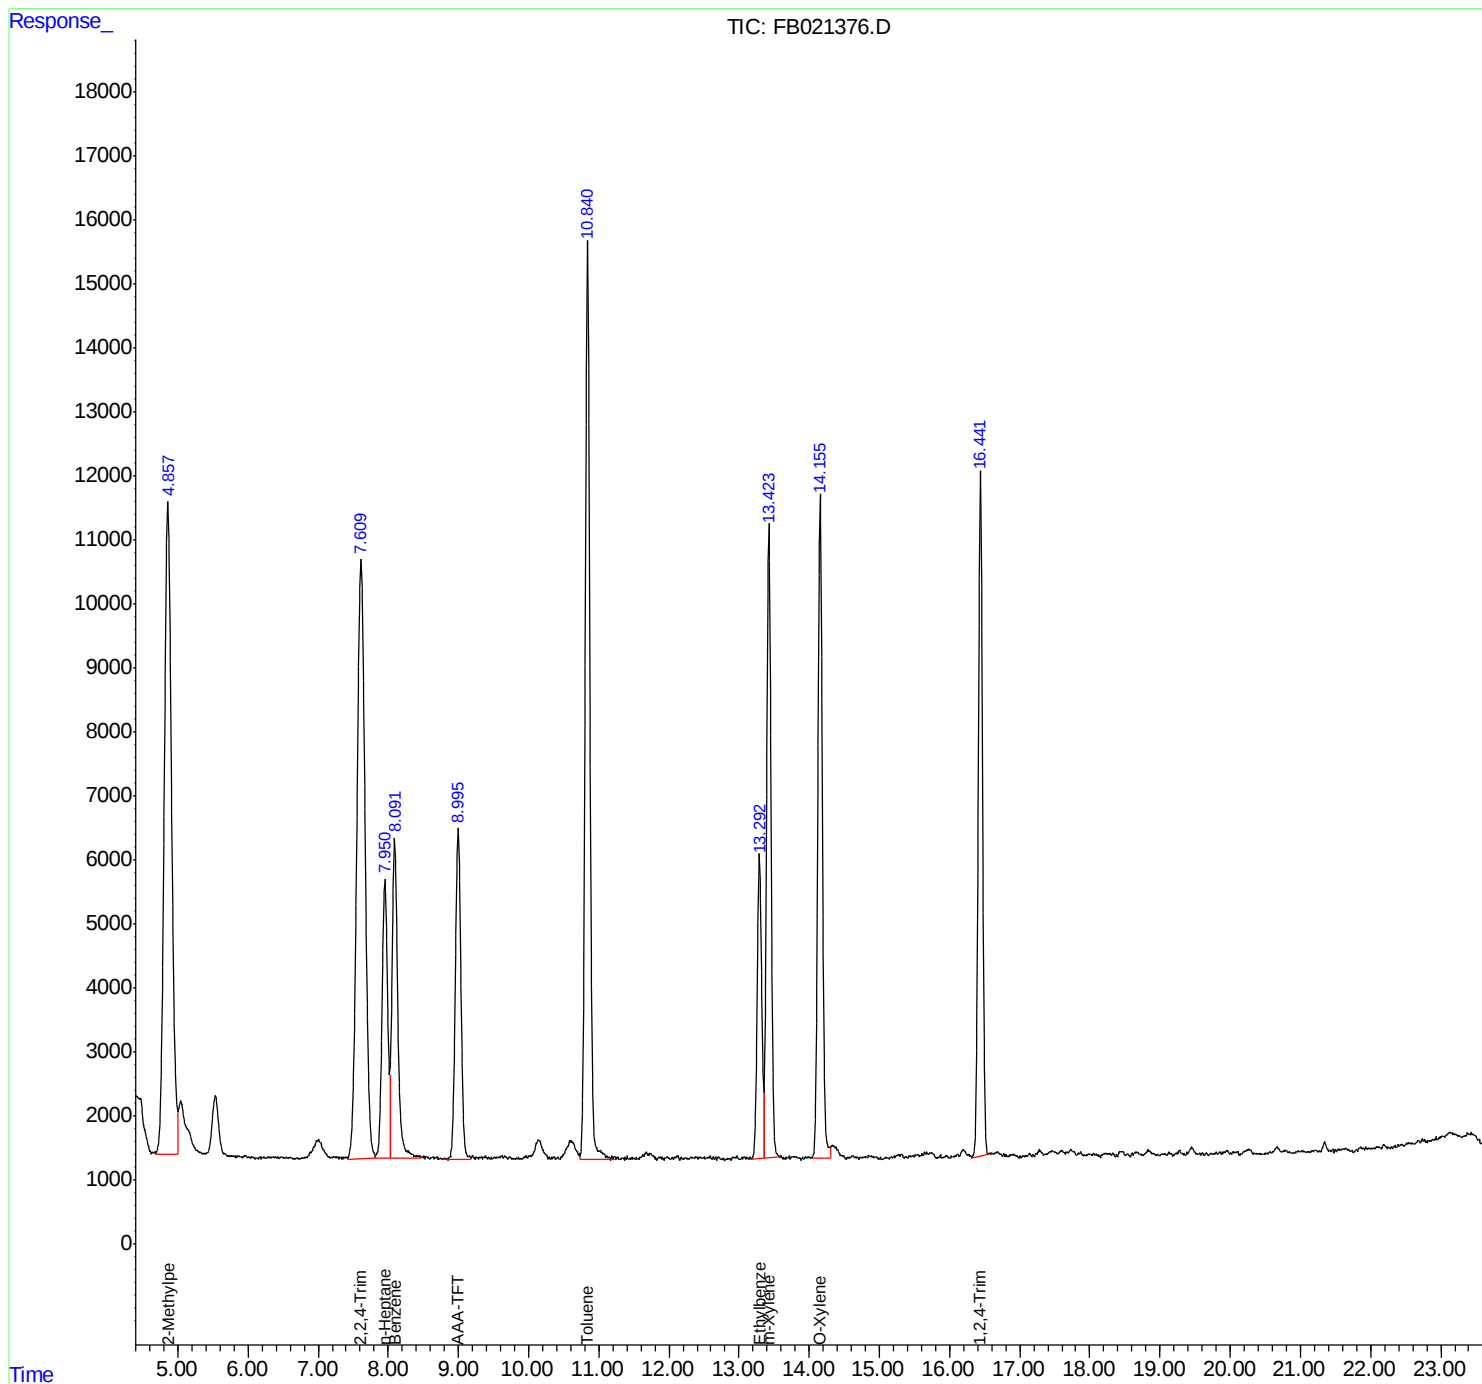

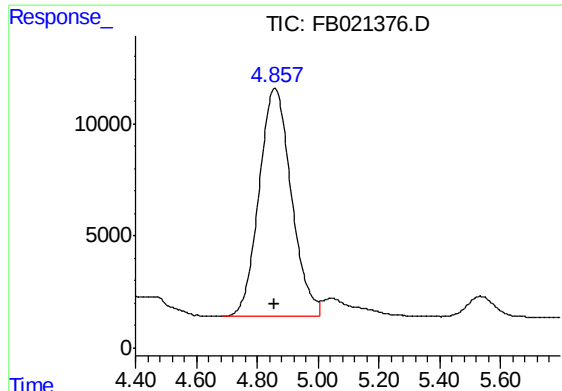


#1 2-Methylpentane

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 749439
Conc: 19.94 ng/ml

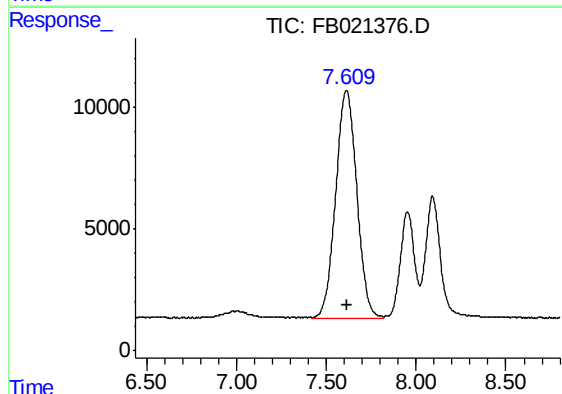


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 763367
Conc: 22.35 ng/ml

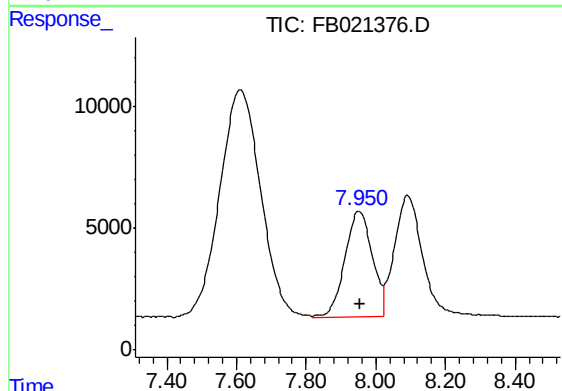


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: -0.002 min
Response: 237594
Conc: 7.29 ng/ml

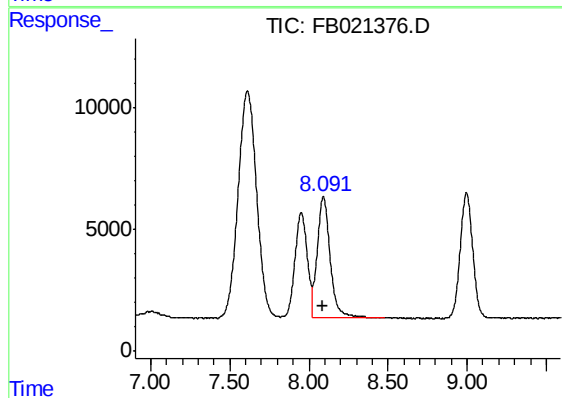


#4 Benzene

R.T.: 8.092 min
Delta R.T.: 0.002 min
Response: 287298
Conc: 8.32 ng/ml

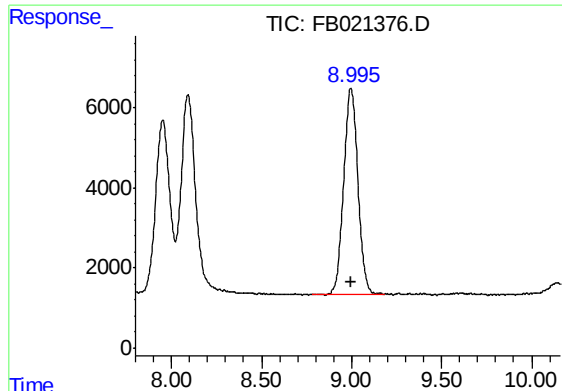


#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: -0.002 min
Response: 285326
Conc: 19.35 ng/ml

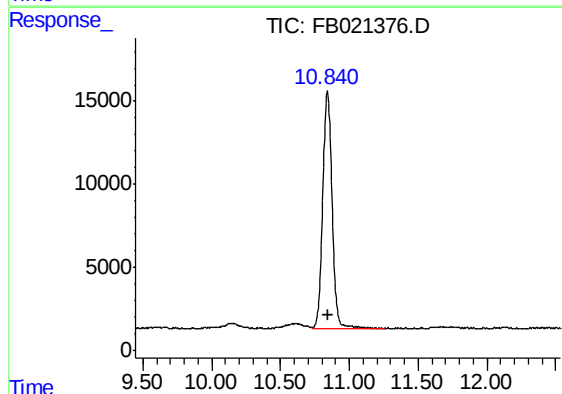


#6 Toluene

R.T.: 10.841 min
Delta R.T.: -0.001 min
Response: 673479
Conc: 28.41 ng/ml

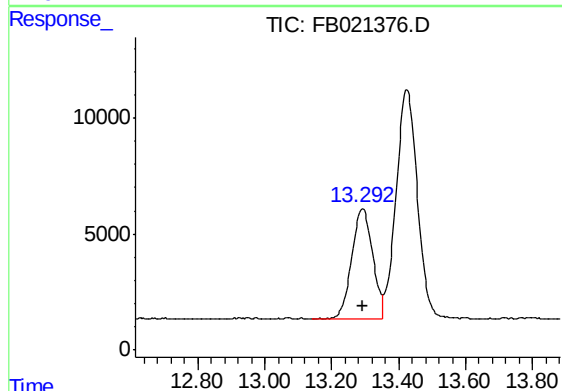


#7 Ethylbenzene

R.T.: 13.292 min
Delta R.T.: 0.000 min
Response: 206858
Conc: 8.85 ng/ml

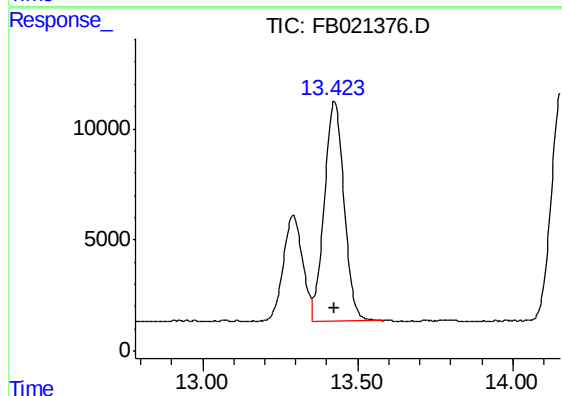


#8 m-Xylene

R.T.: 13.425 min
Delta R.T.: -0.001 min
Response: 437110
Conc: 17.51 ng/ml

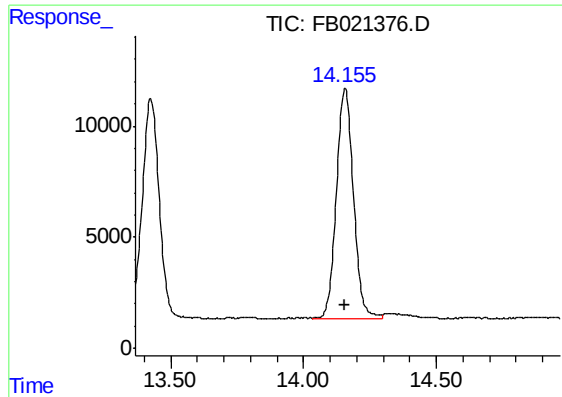

#9 O-Xylene

R.T.: 14.156 min
Delta R.T.: 0.000 min
Response: 462801
Conc: 17.74 ng/ml

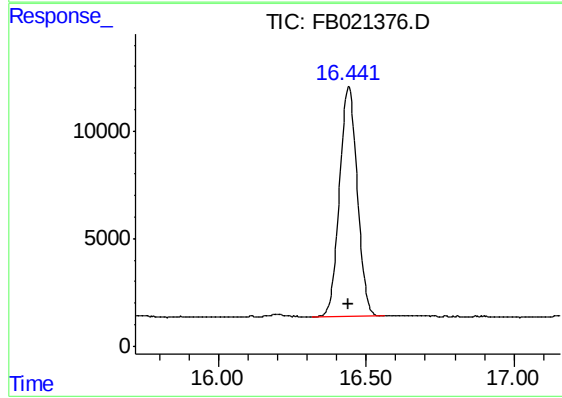

#10 1,2,4-Trimethylbenzene

R.T.: 16.441 min
Delta R.T.: 0.000 min
Response: 446999
Conc: 16.64 ng/ml