

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061322\
 Data File : FB027411.D
 Signal(s) : FID2B.CH
 Acq On : 13 Jun 2022 21:39
 Operator : AJ/MA
 Sample : N3304-06
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 14 03:06:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.859	471305	42.018 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	5010	0.297 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	86262	4.913 ng/ml
3) t n-Heptane	7.819	110787	6.324 ng/ml
4) t Benzene	7.819	110787	5.433 ng/ml
7) t Ethylbenzene	13.020	3252529	179.604 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061322\
Data File : FB027411.D
Signal(s) : FID2B.CH
Acq On : 13 Jun 2022 21:39
Operator : AJ/MA
Sample : N3304-06
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 14 03:06:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

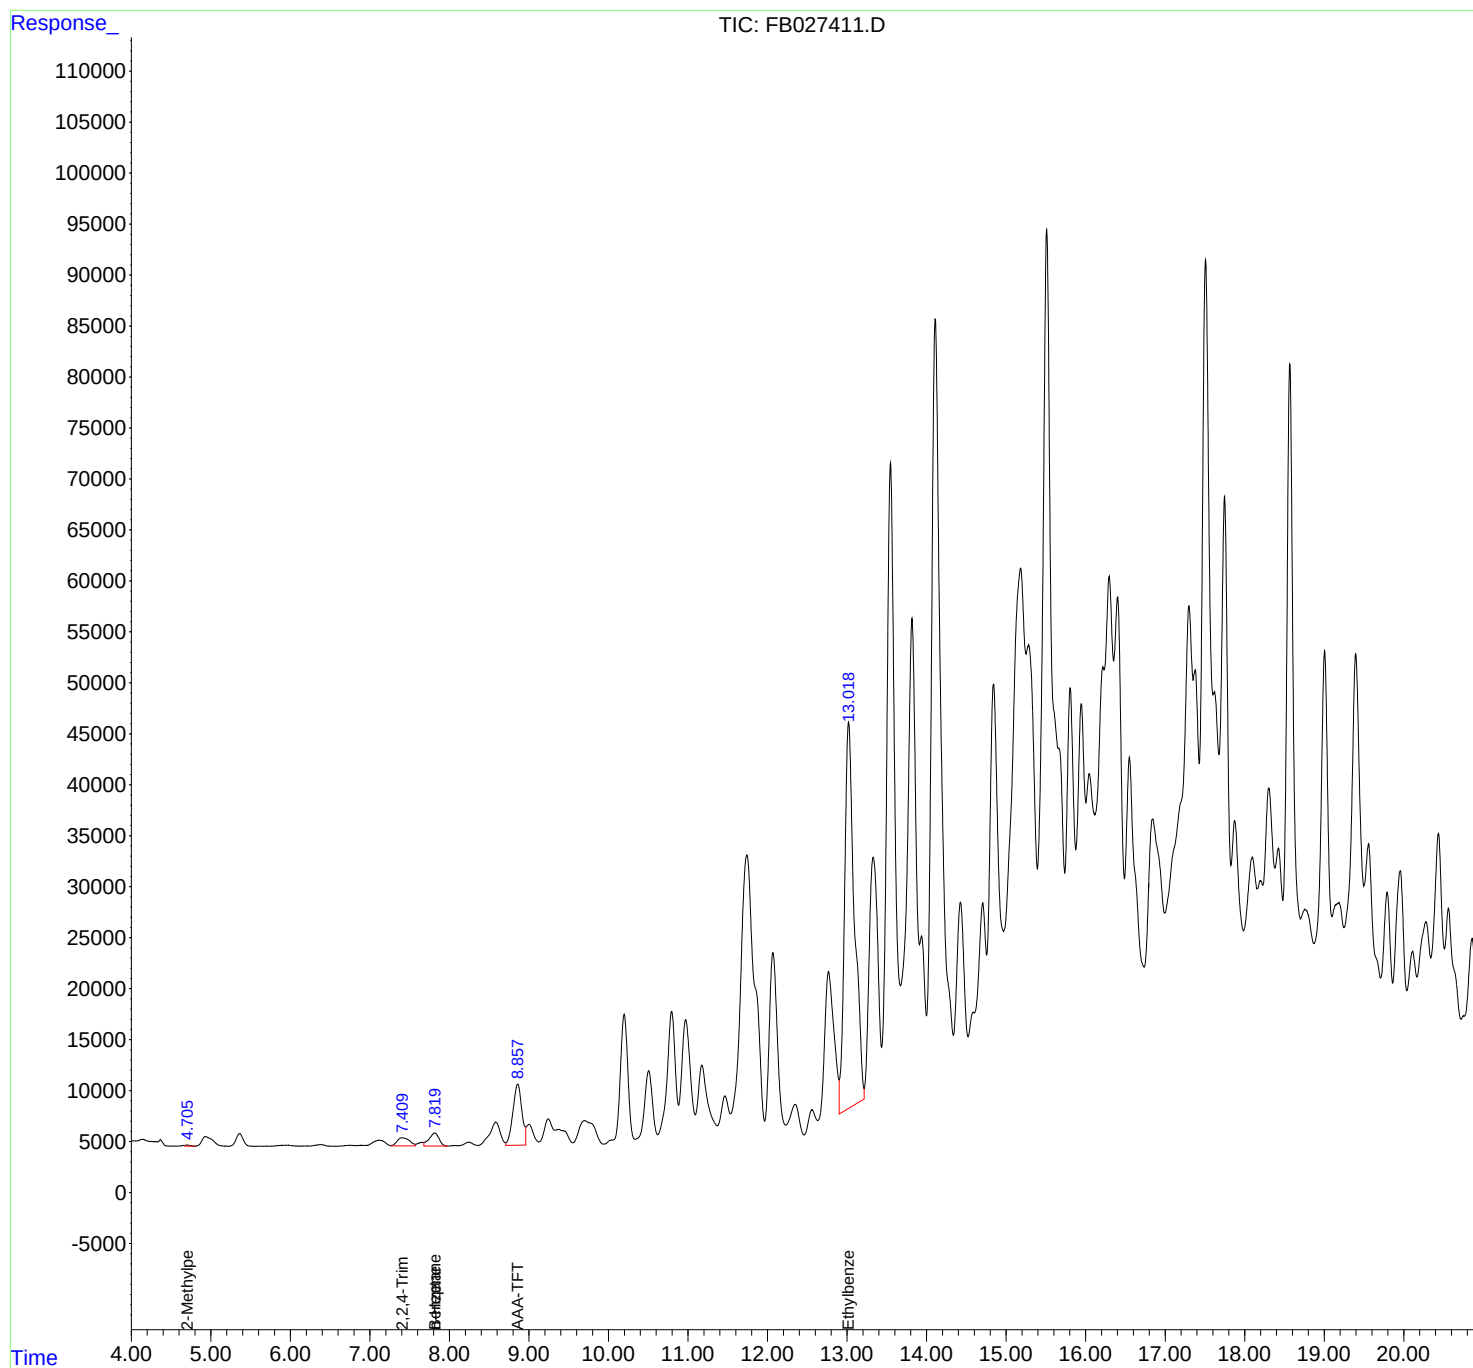


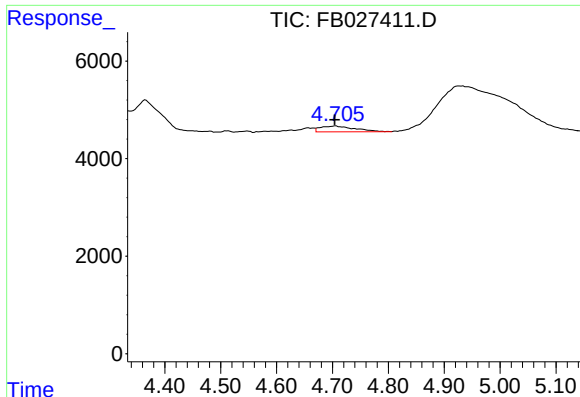

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.002 min
Response: 5010
Conc: 0.30 ng/ml

Instrument :
FID_B
ClientSampleId :

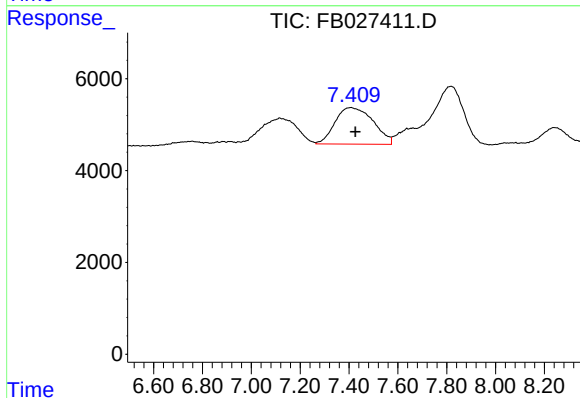


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.017 min
Response: 86262
Conc: 4.91 ng/ml

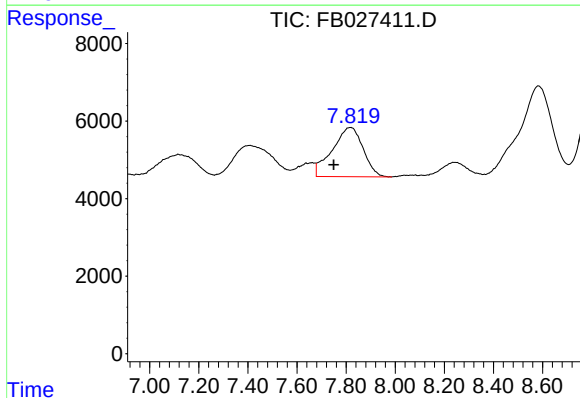


#3 n-Heptane

R.T.: 7.819 min
Delta R.T.: 0.070 min
Response: 110787
Conc: 6.32 ng/ml

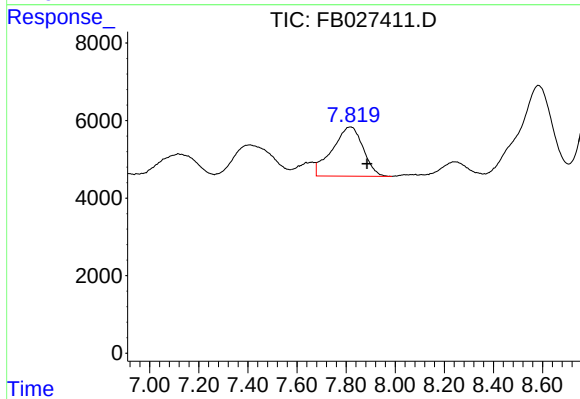

#4 Benzene


R.T.: 7.819 min
Delta R.T.: -0.066 min
Response: 110787
Conc: 5.43 ng/ml

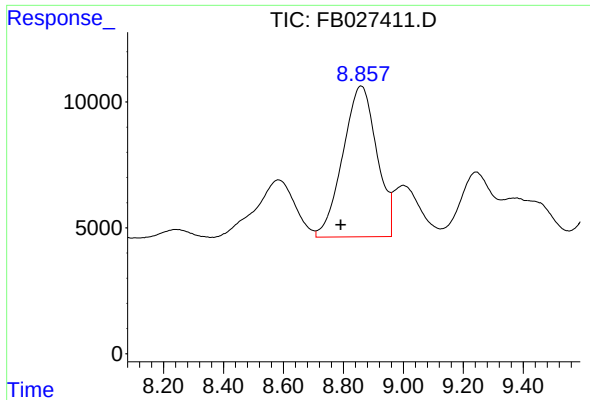

#5 AAA-TFT

R.T.: 8.859 min
Delta R.T.: 0.068 min
Response: 471305
Conc: 42.02 ng/ml

Instrument :
FID_B
ClientSampleId :

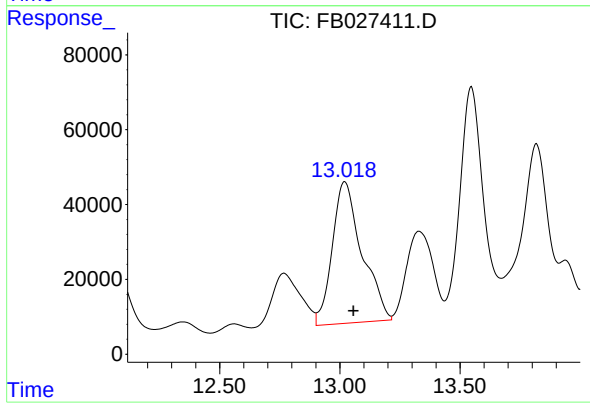

#7 Ethylbenzene

R.T.: 13.020 min
Delta R.T.: -0.036 min
Response: 3252529
Conc: 179.60 ng/ml