

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061322\
 Data File : FB027406.D
 Signal(s) : FID2B.CH
 Acq On : 13 Jun 2022 17:20
 Operator : AJ/MA
 Sample : BSF0613S2
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0613S2

Integration File: SAMPLE.e
 Quant Time: Jun 13 18:01:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	225727	20.124 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	472821	28.065 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	537780	30.628 ng/ml
3) t n-Heptane	7.755	148278	8.464 ng/ml
4) t Benzene	7.892	187019	9.171 ng/ml
6) t Toluene	10.625	535166	27.640 ng/ml
7) t Ethylbenzene	13.062	173230	9.566 ng/ml
8) t m-Xylene	13.195	350026	19.636 ng/ml
9) t O-Xylene	13.922	353246	20.330 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	370988	21.596 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061322\
Data File : FB027406.D
Signal(s) : FID2B.CH
Acq On : 13 Jun 2022 17:20
Operator : AJ/MA
Sample : BSF0613S2
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0613S2

Integration File: SAMPLE.e
Quant Time: Jun 13 18:01:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

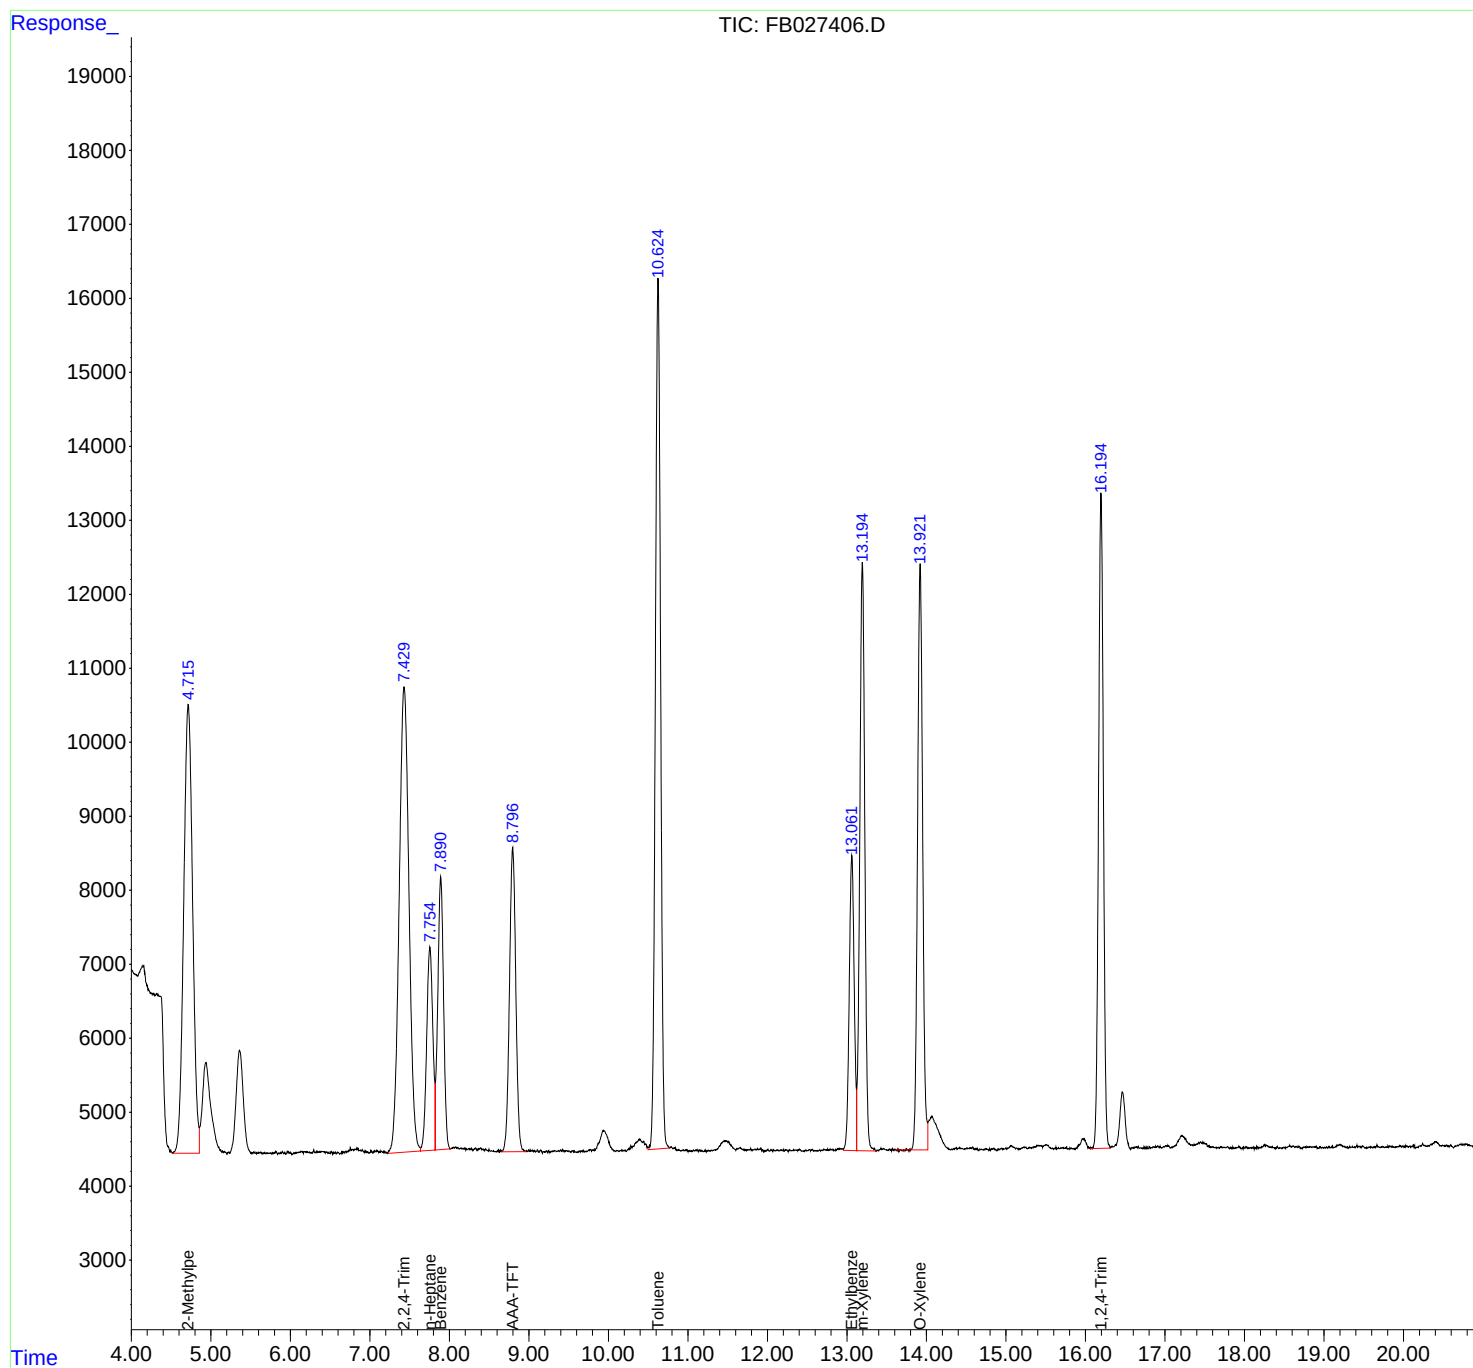


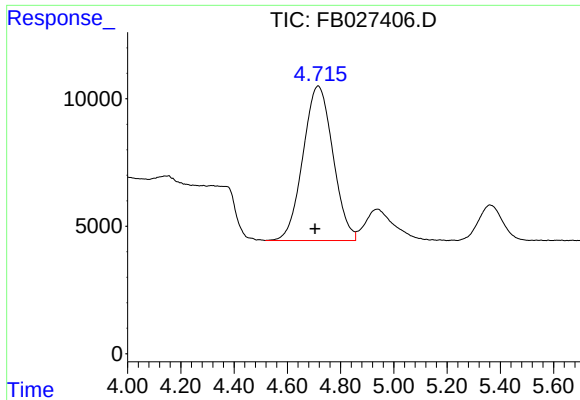

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.012 min
Response: 472821
Conc: 28.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0613S2

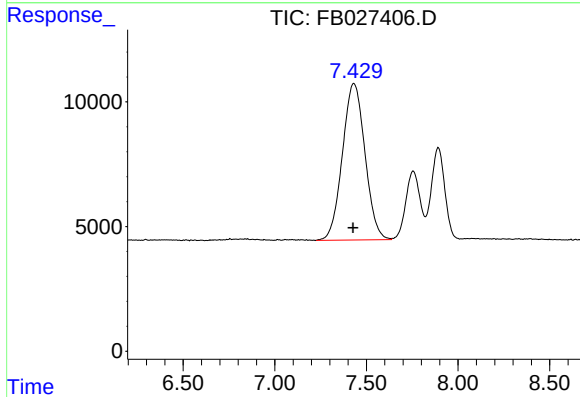


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.005 min
Response: 537780
Conc: 30.63 ng/ml

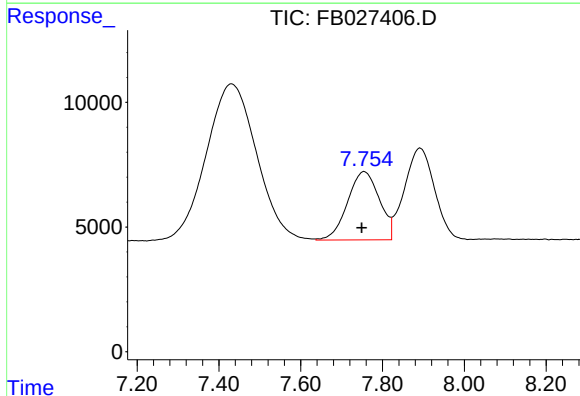


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.006 min
Response: 148278
Conc: 8.46 ng/ml

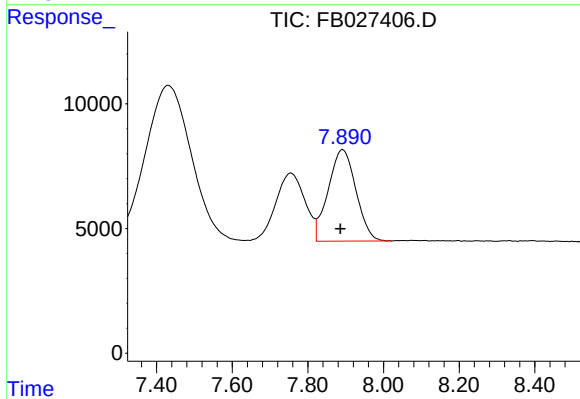

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.006 min
Response: 187019
Conc: 9.17 ng/ml

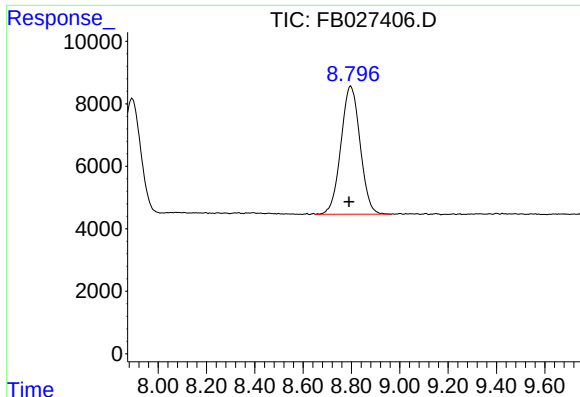

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 225727
Conc: 20.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0613S2

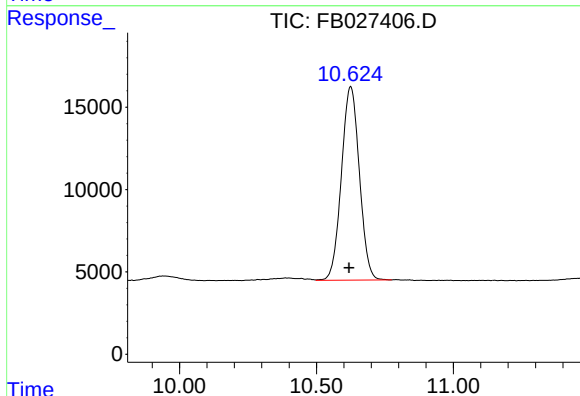


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 535166
Conc: 27.64 ng/ml

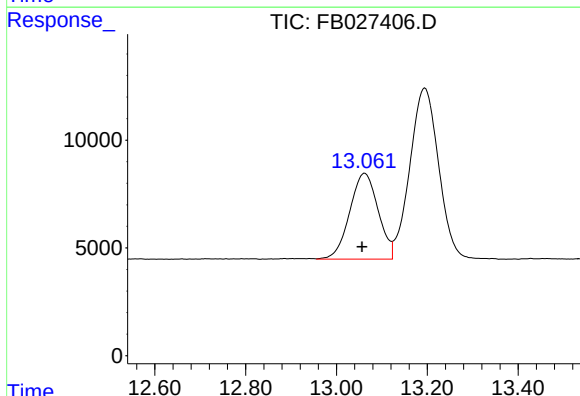


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.006 min
Response: 173230
Conc: 9.57 ng/ml

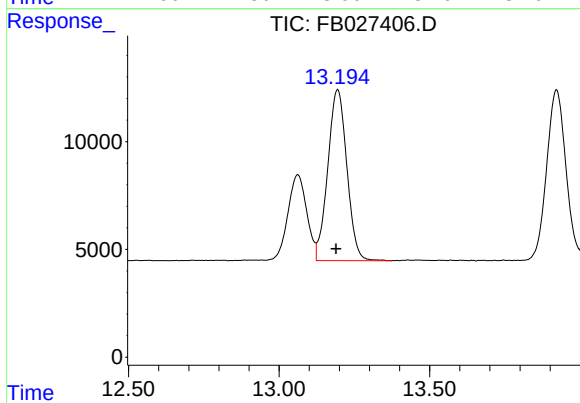

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.006 min
Response: 350026
Conc: 19.64 ng/ml

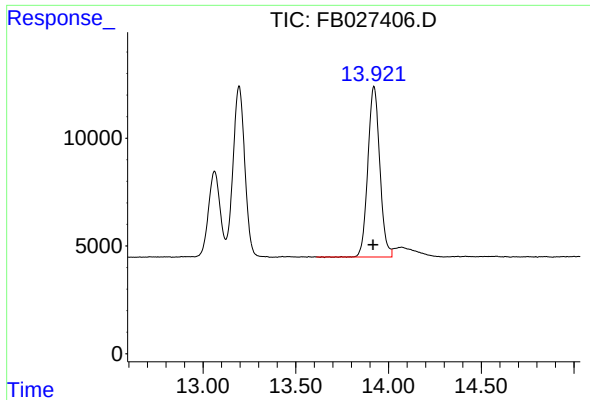

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.006 min
Response: 353246
Conc: 20.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0613S2

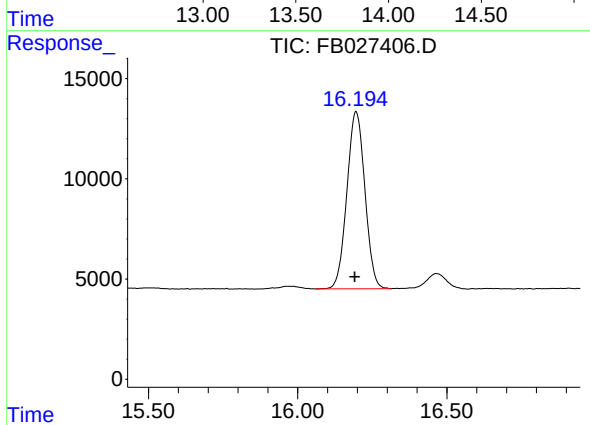

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.005 min
Response: 370988
Conc: 21.60 ng/ml