

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061322\
 Data File : FB027418.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 1:56
 Operator : AJ/MA
 Sample : BSF0613S3
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0613S3

Integration File: SAMPLE.e
 Quant Time: Jun 14 03:06:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	232191	20.700 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	508379	30.176 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	543381	30.947 ng/ml
3) t n-Heptane	7.751	173392	9.898 ng/ml
4) t Benzene	7.889	202990	9.954 ng/ml
6) t Toluene	10.622	571400	29.511 ng/ml
7) t Ethylbenzene	13.058	177908	9.824 ng/ml
8) t m-Xylene	13.191	353217	19.815 ng/ml
9) t O-Xylene	13.918	348717	20.069 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	351159	20.442 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061322\
Data File : FB027418.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 1:56
Operator : AJ/MA
Sample : BSF0613S3
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0613S3

Integration File: SAMPLE.e
Quant Time: Jun 14 03:06:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

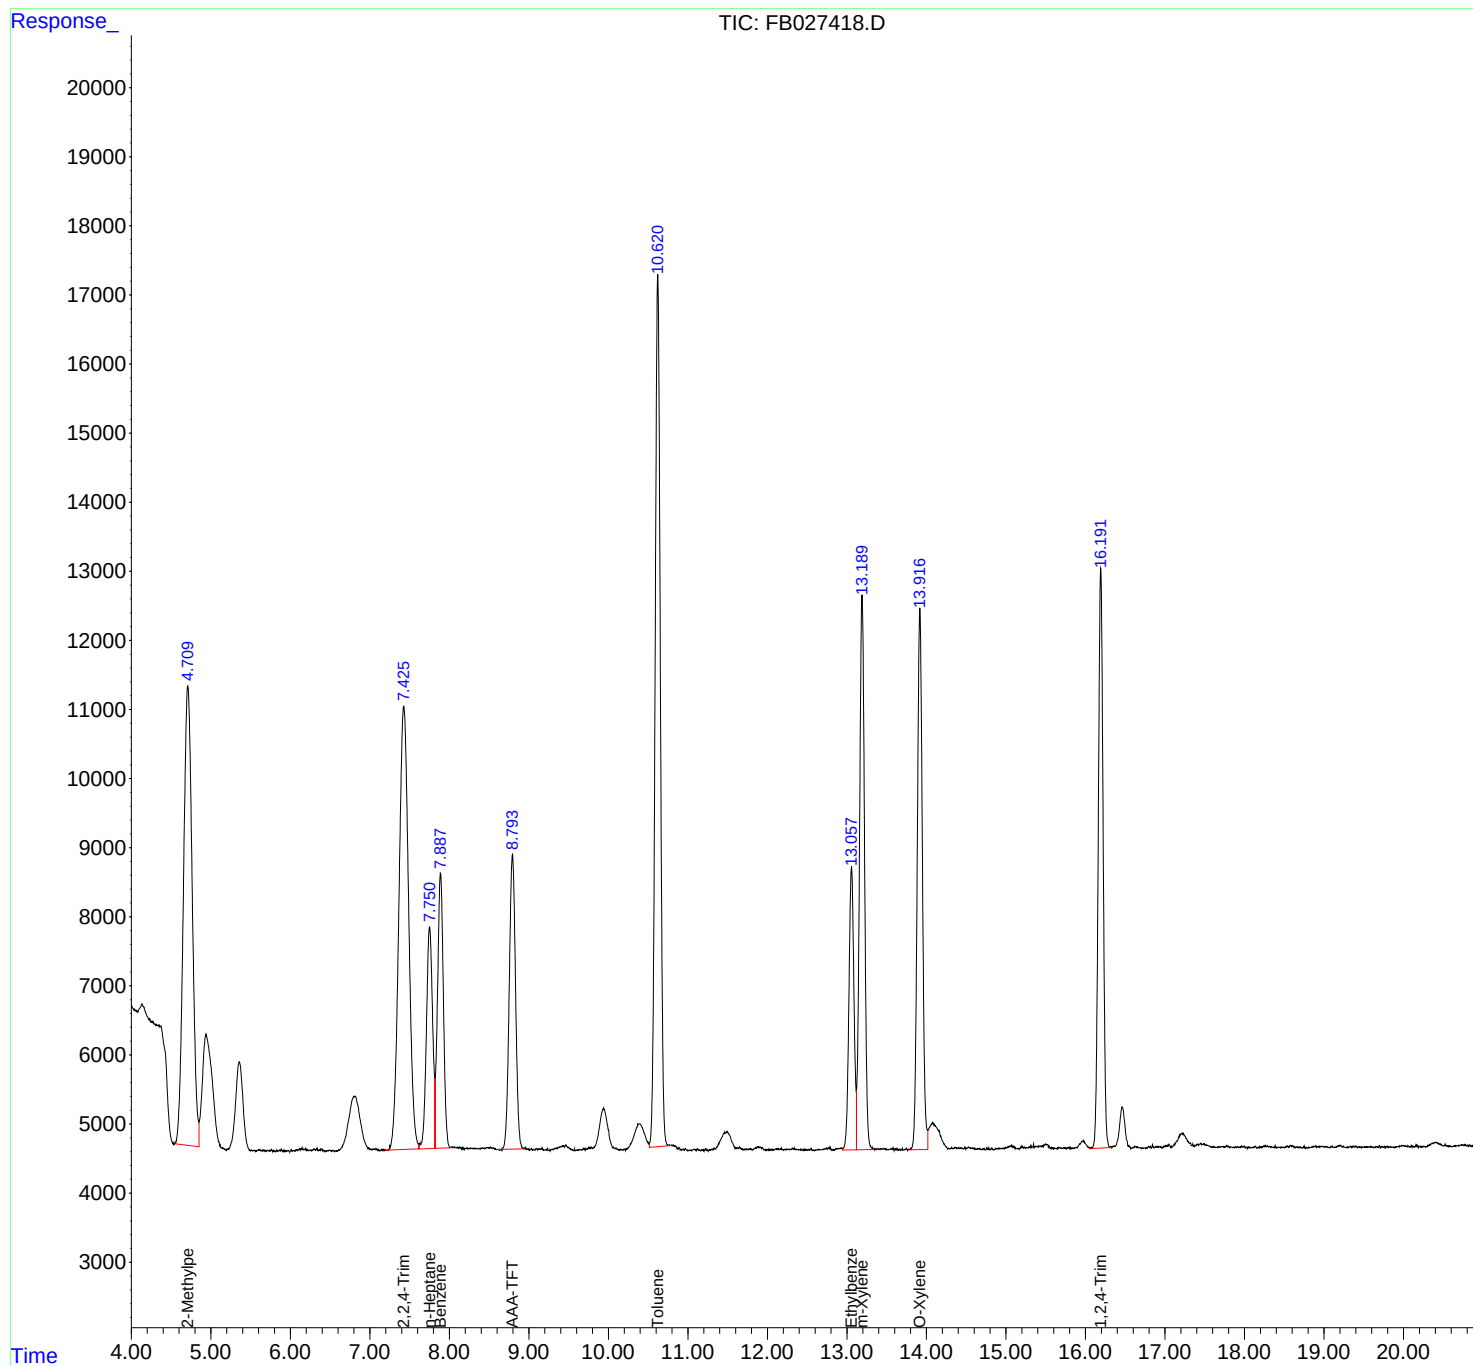


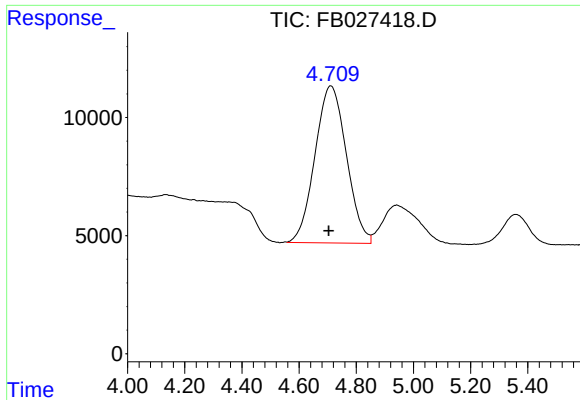

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.007 min
Response: 508379
Conc: 30.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0613S3

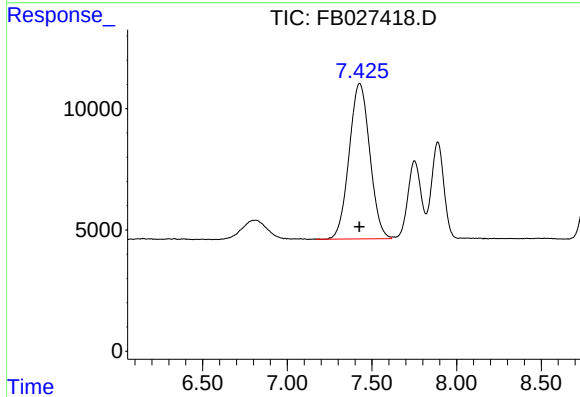


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 543381
Conc: 30.95 ng/ml

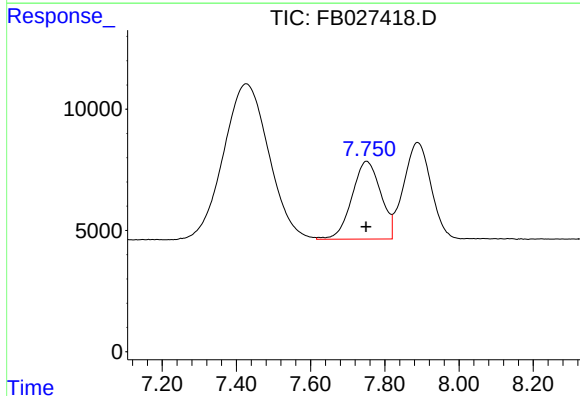


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 173392
Conc: 9.90 ng/ml

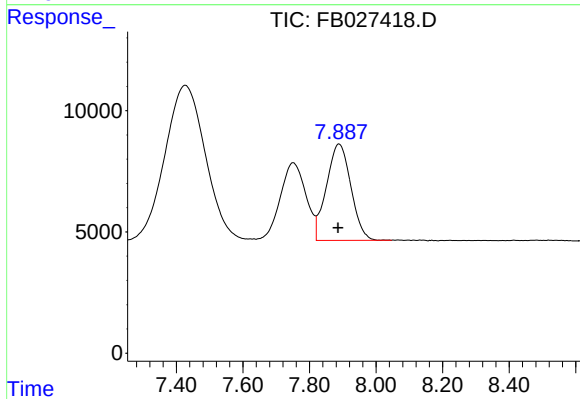

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 202990
Conc: 9.95 ng/ml

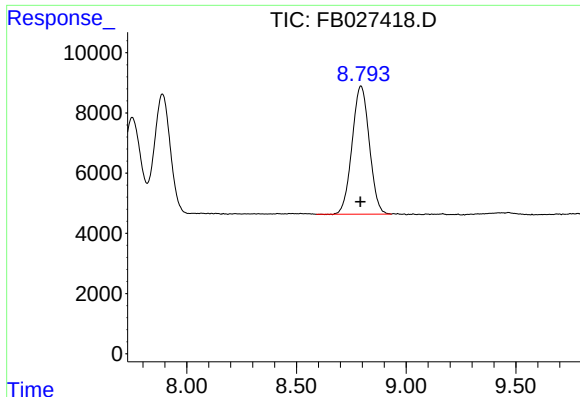

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 232191
Conc: 20.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0613S3

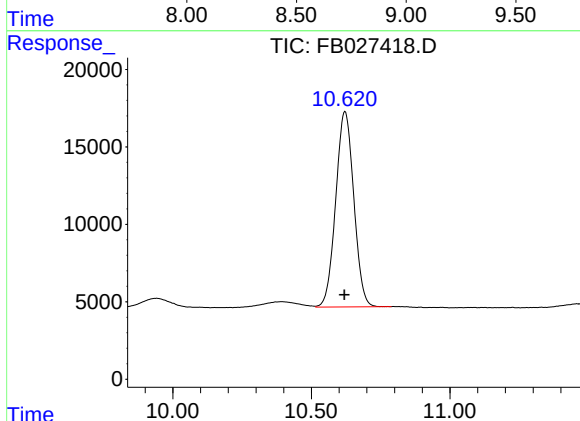


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 571400
Conc: 29.51 ng/ml

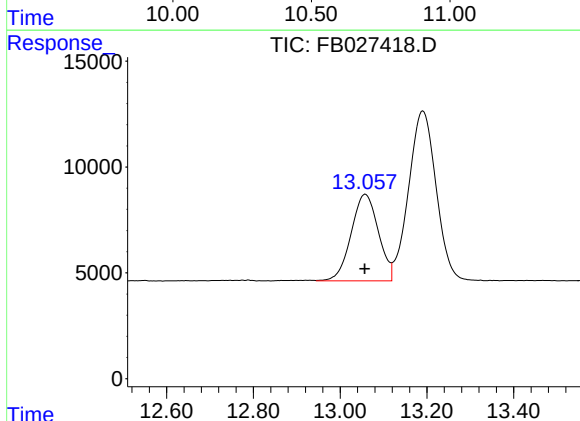


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 177908
Conc: 9.82 ng/ml

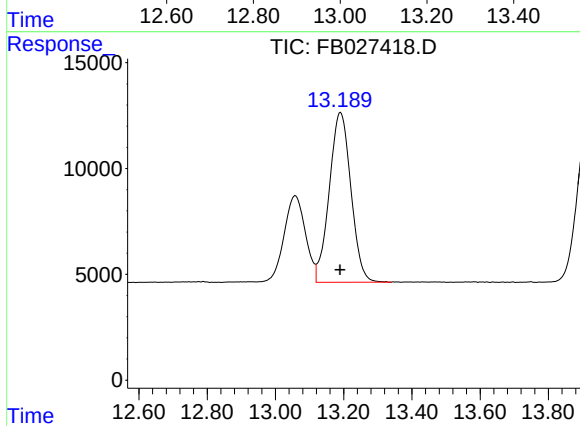

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 353217
Conc: 19.81 ng/ml

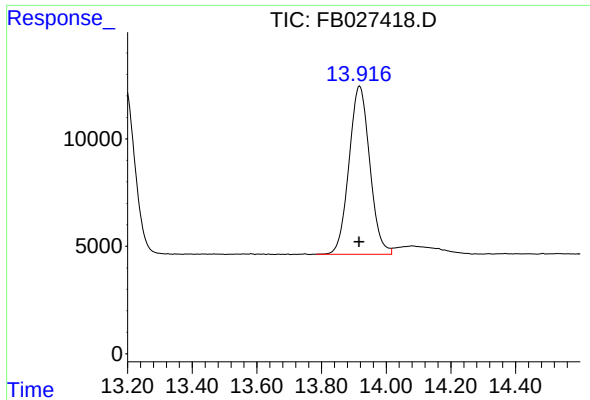

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 348717
Conc: 20.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0613S3

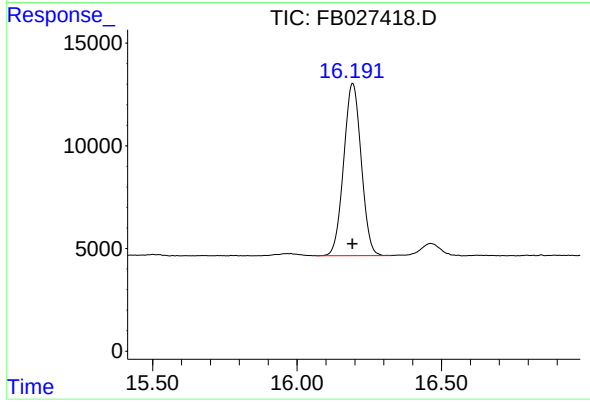

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 351159
Conc: 20.44 ng/ml