

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
 Data File : FB021391.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2019 22:39
 Operator : MJ/SJ
 Sample : K3369-13MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 15 03:00:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	310211	21.040 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.860	746437	19.855 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	806877	23.627 ng/ml
3) t n-Heptane	7.947	248366	7.618 ng/ml
4) t Benzene	8.087	283979	8.227 ng/ml
6) t Toluene	10.830	684683	28.887 ng/ml
7) t Ethylbenzene	13.275	204955	8.771 ng/ml
8) t m-Xylene	13.408	439727	17.617 ng/ml
9) t O-Xylene	14.137	461713	17.699 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	448479	16.700 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
Data File : FB021391.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2019 22:39
Operator : MJ/SJ
Sample : K3369-13MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 15 03:00:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

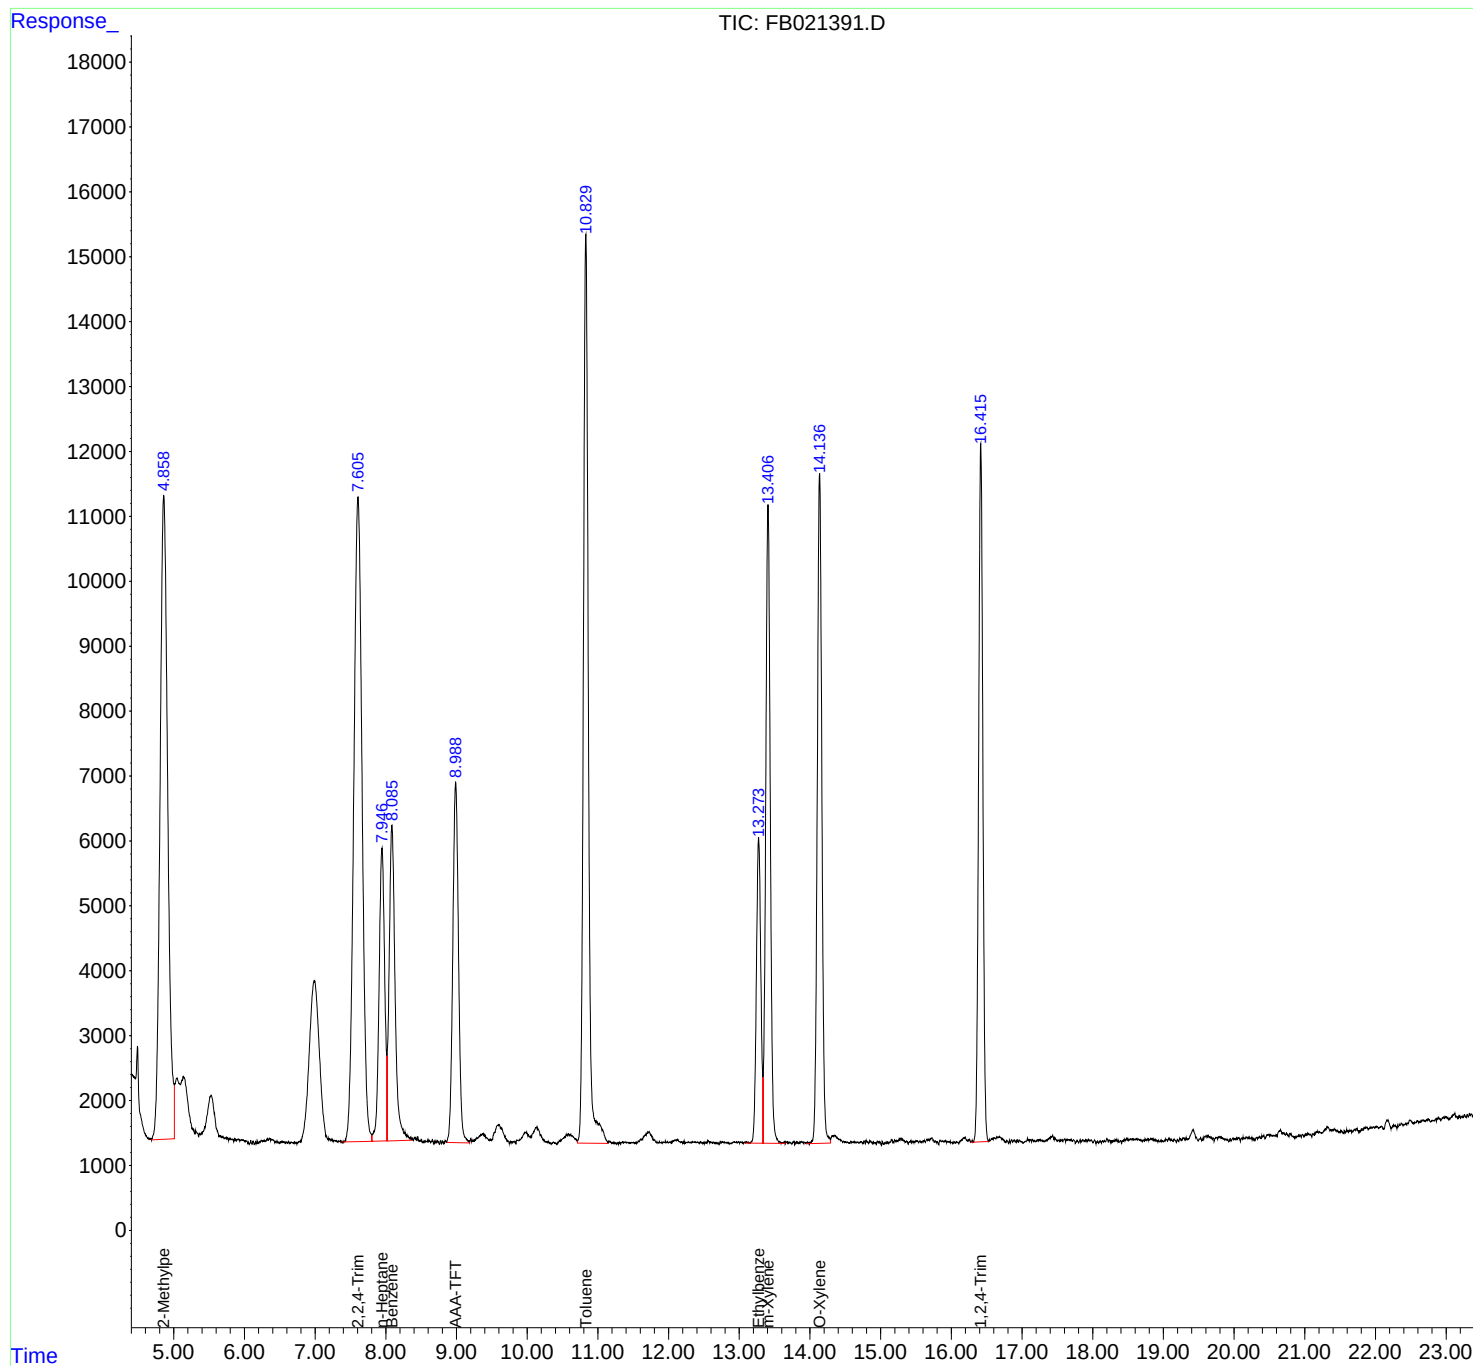

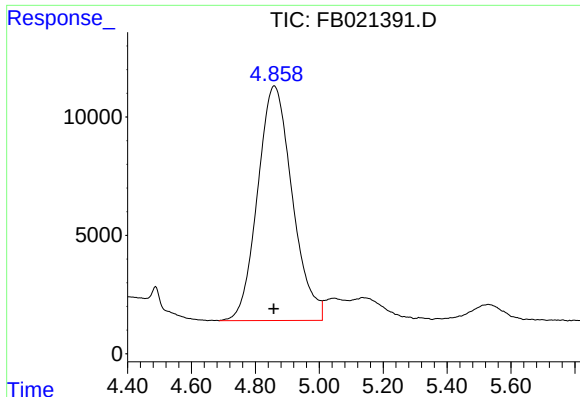


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: 0.002 min
Response: 746437
Conc: 19.86 ng/ml

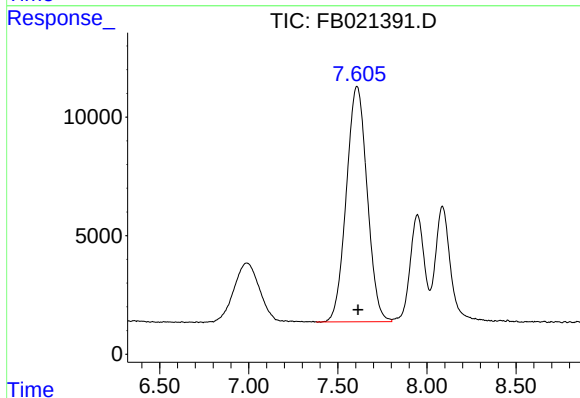


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: -0.007 min
Response: 806877
Conc: 23.63 ng/ml

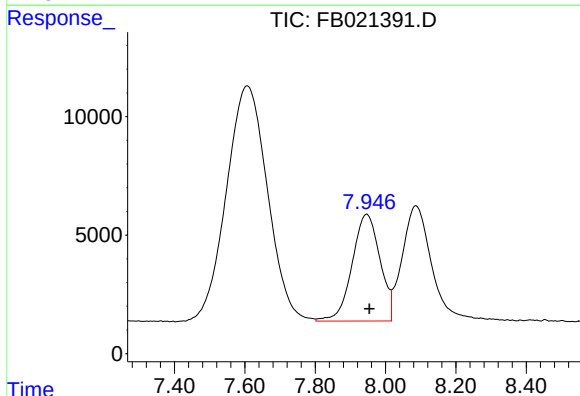


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: -0.007 min
Response: 248366
Conc: 7.62 ng/ml

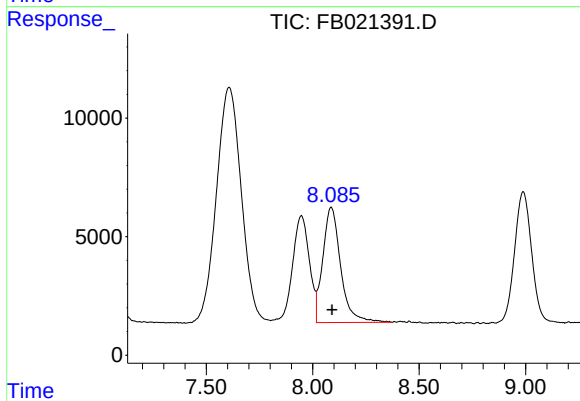


#4 Benzene

R.T.: 8.087 min
Delta R.T.: -0.003 min
Response: 283979
Conc: 8.23 ng/ml

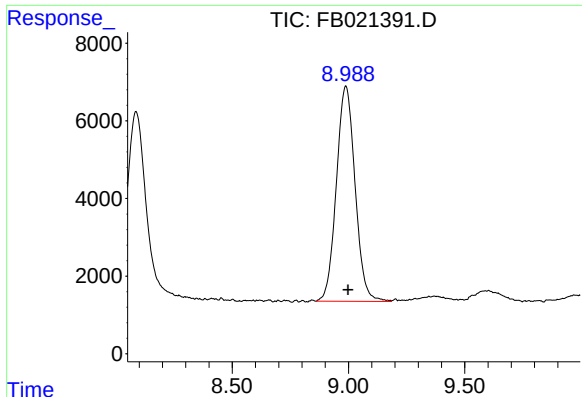


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.009 min
Response: 310211
Conc: 21.04 ng/ml

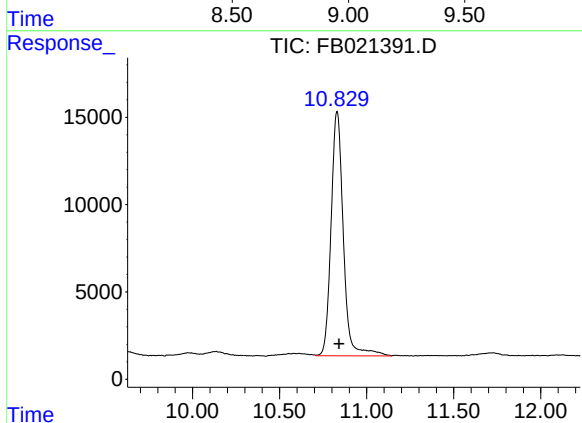


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.012 min
Response: 684683
Conc: 28.89 ng/ml

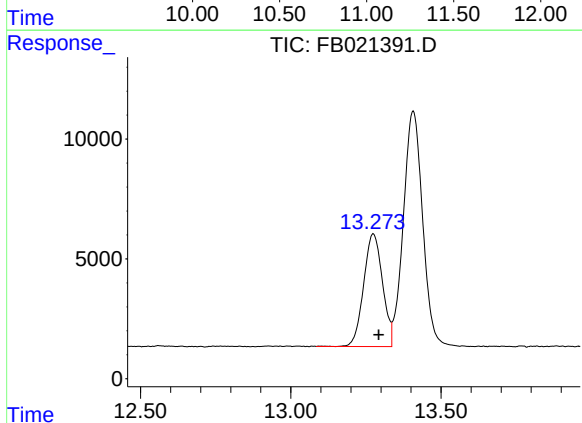


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.018 min
Response: 204955
Conc: 8.77 ng/ml

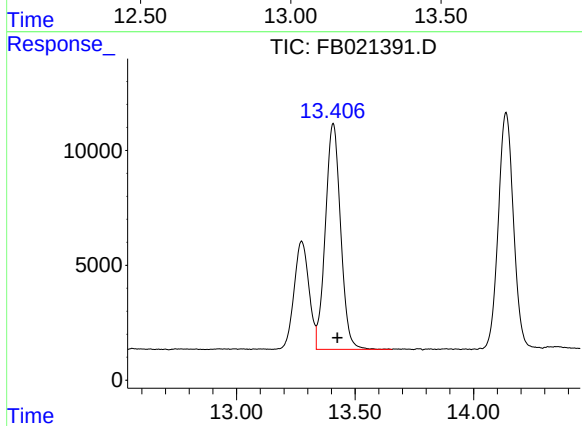


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.018 min
Response: 439727
Conc: 17.62 ng/ml

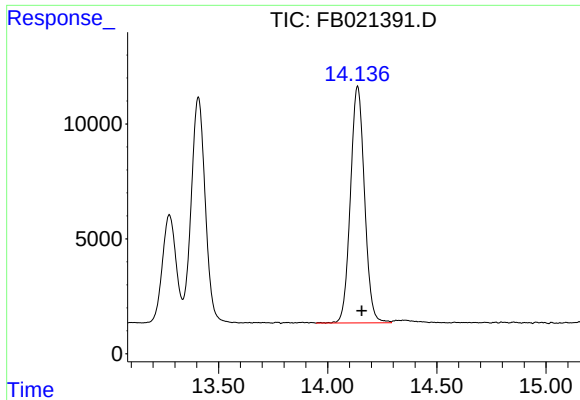

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.020 min
Response: 461713
Conc: 17.70 ng/ml

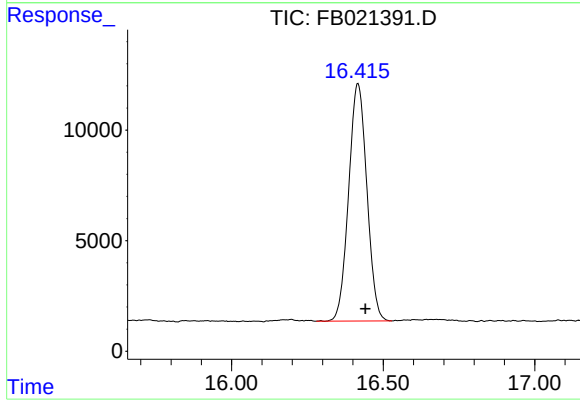

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.024 min
Response: 448479
Conc: 16.70 ng/ml