

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
 Data File : FB021392.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2019 23:09
 Operator : MJ/SJ
 Sample : K3366-01
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 15 03:00:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	272718	18.497 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.848	10939	0.291 ng/ml
2) t	2,2,4-Trimethylpentane	7.562	19530	0.572 ng/ml
3) t	n-Heptane	7.943	84825	2.602 ng/ml
4) t	Benzene	8.088	40160	1.163 ng/ml
6) t	Toluene	10.831	33802	1.426 ng/ml
7) t	Ethylbenzene	13.273	45231	1.936 ng/ml
8) t	m-Xylene	13.404	109542	4.389 ng/ml
9) t	O-Xylene	14.138	65864	2.525 ng/ml
10) t	1,2,4-Trimethylbenzene	16.419	13809	0.514 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
Data File : FB021392.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2019 23:09
Operator : MJ/SJ
Sample : K3366-01
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 15 03:00:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

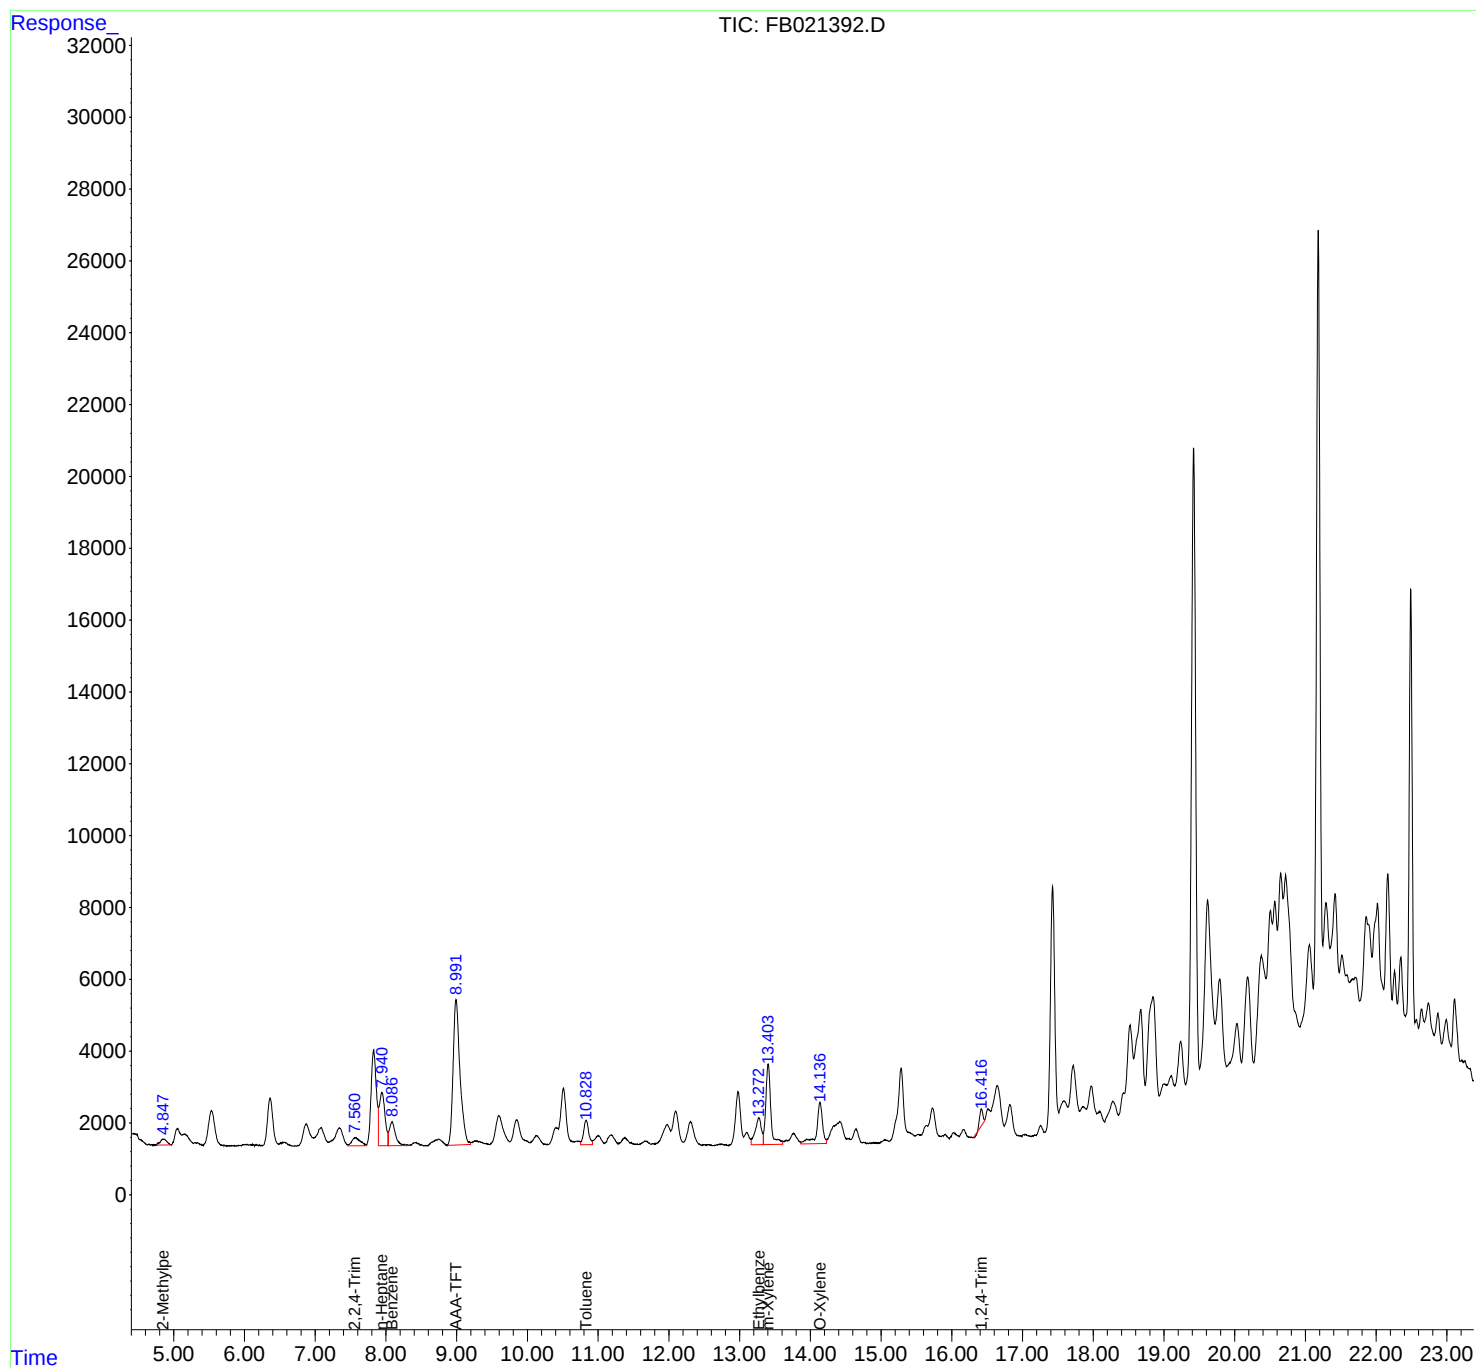

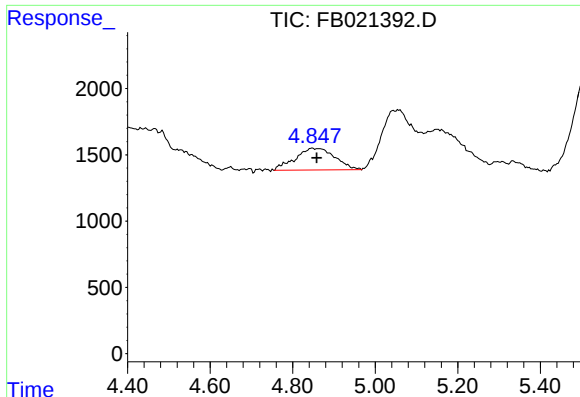


#1 2-Methylpentane

R.T.: 4.848 min
Delta R.T.: -0.010 min
Response: 10939
Conc: 0.29 ng/ml

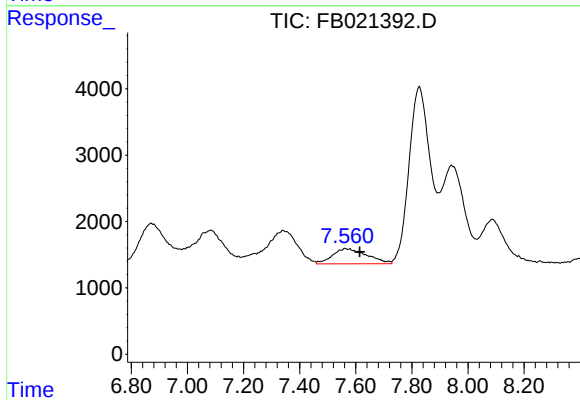


#2 2,2,4-Trimethylpentane

R.T.: 7.562 min
Delta R.T.: -0.052 min
Response: 19530
Conc: 0.57 ng/ml

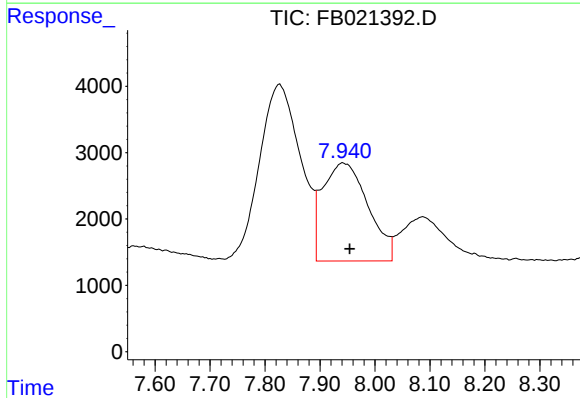


#3 n-Heptane

R.T.: 7.943 min
Delta R.T.: -0.011 min
Response: 84825
Conc: 2.60 ng/ml

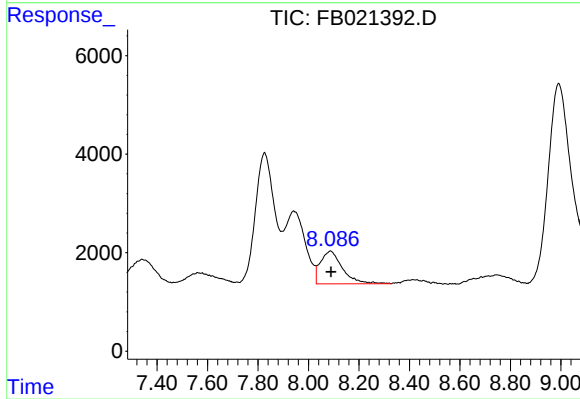


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.002 min
Response: 40160
Conc: 1.16 ng/ml

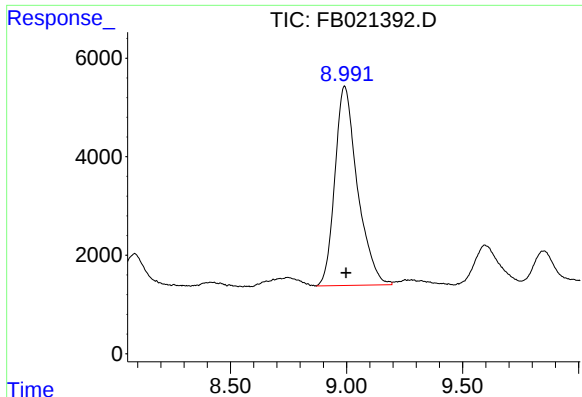


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: -0.006 min
Response: 272718
Conc: 18.50 ng/ml

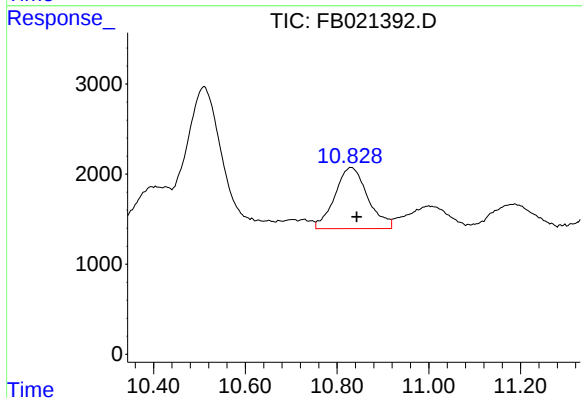


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.011 min
Response: 33802
Conc: 1.43 ng/ml

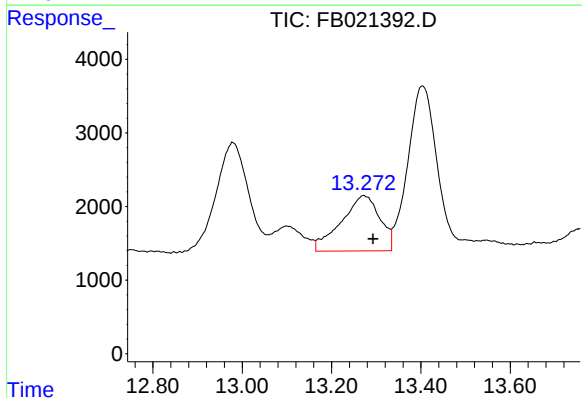


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: -0.020 min
Response: 45231
Conc: 1.94 ng/ml

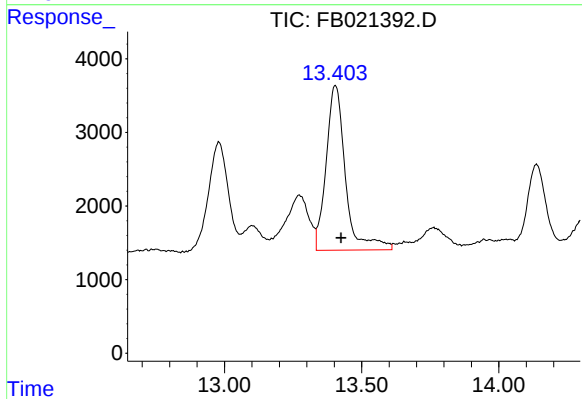


#8 m-Xylene

R.T.: 13.404 min
Delta R.T.: -0.021 min
Response: 109542
Conc: 4.39 ng/ml

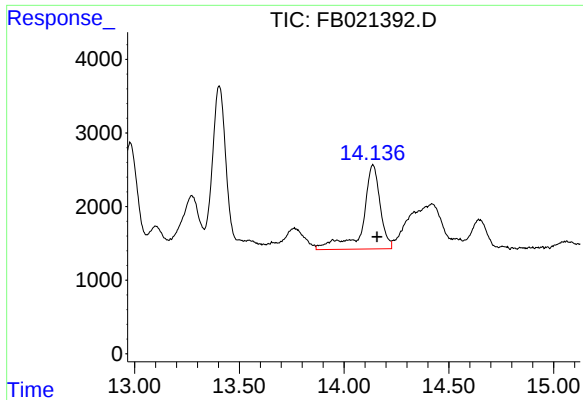

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.019 min
Response: 65864
Conc: 2.52 ng/ml

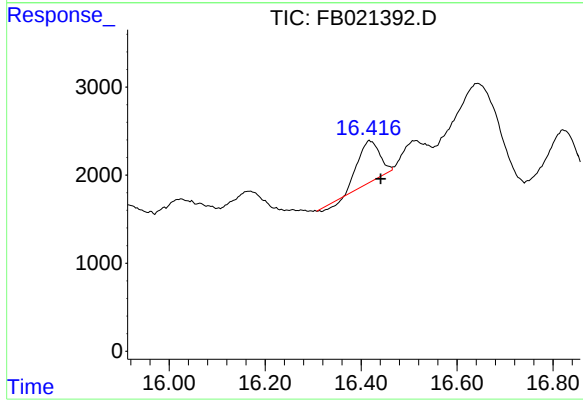

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: -0.022 min
Response: 13809
Conc: 0.51 ng/ml