

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
 Data File : FB021393.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2019 23:39
 Operator : MJ/SJ
 Sample : K3366-02
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 15 03:01:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	269144	18.254 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	19658	0.523 ng/ml
2) t 2,2,4-Trimethylpentane	7.574	22544	0.660 ng/ml
3) t n-Heptane	7.945	96399	2.957 ng/ml
4) t Benzene	8.086	43053	1.247 ng/ml
6) t Toluene	10.832	45752	1.930 ng/ml
7) t Ethylbenzene	13.275	43759	1.873 ng/ml
8) t m-Xylene	13.405	109770	4.398 ng/ml
9) t O-Xylene	14.138	54714	2.097 ng/ml
10) t 1,2,4-Trimethylbenzene	16.421	10552	0.393 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
Data File : FB021393.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2019 23:39
Operator : MJ/SJ
Sample : K3366-02
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 15 03:01:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

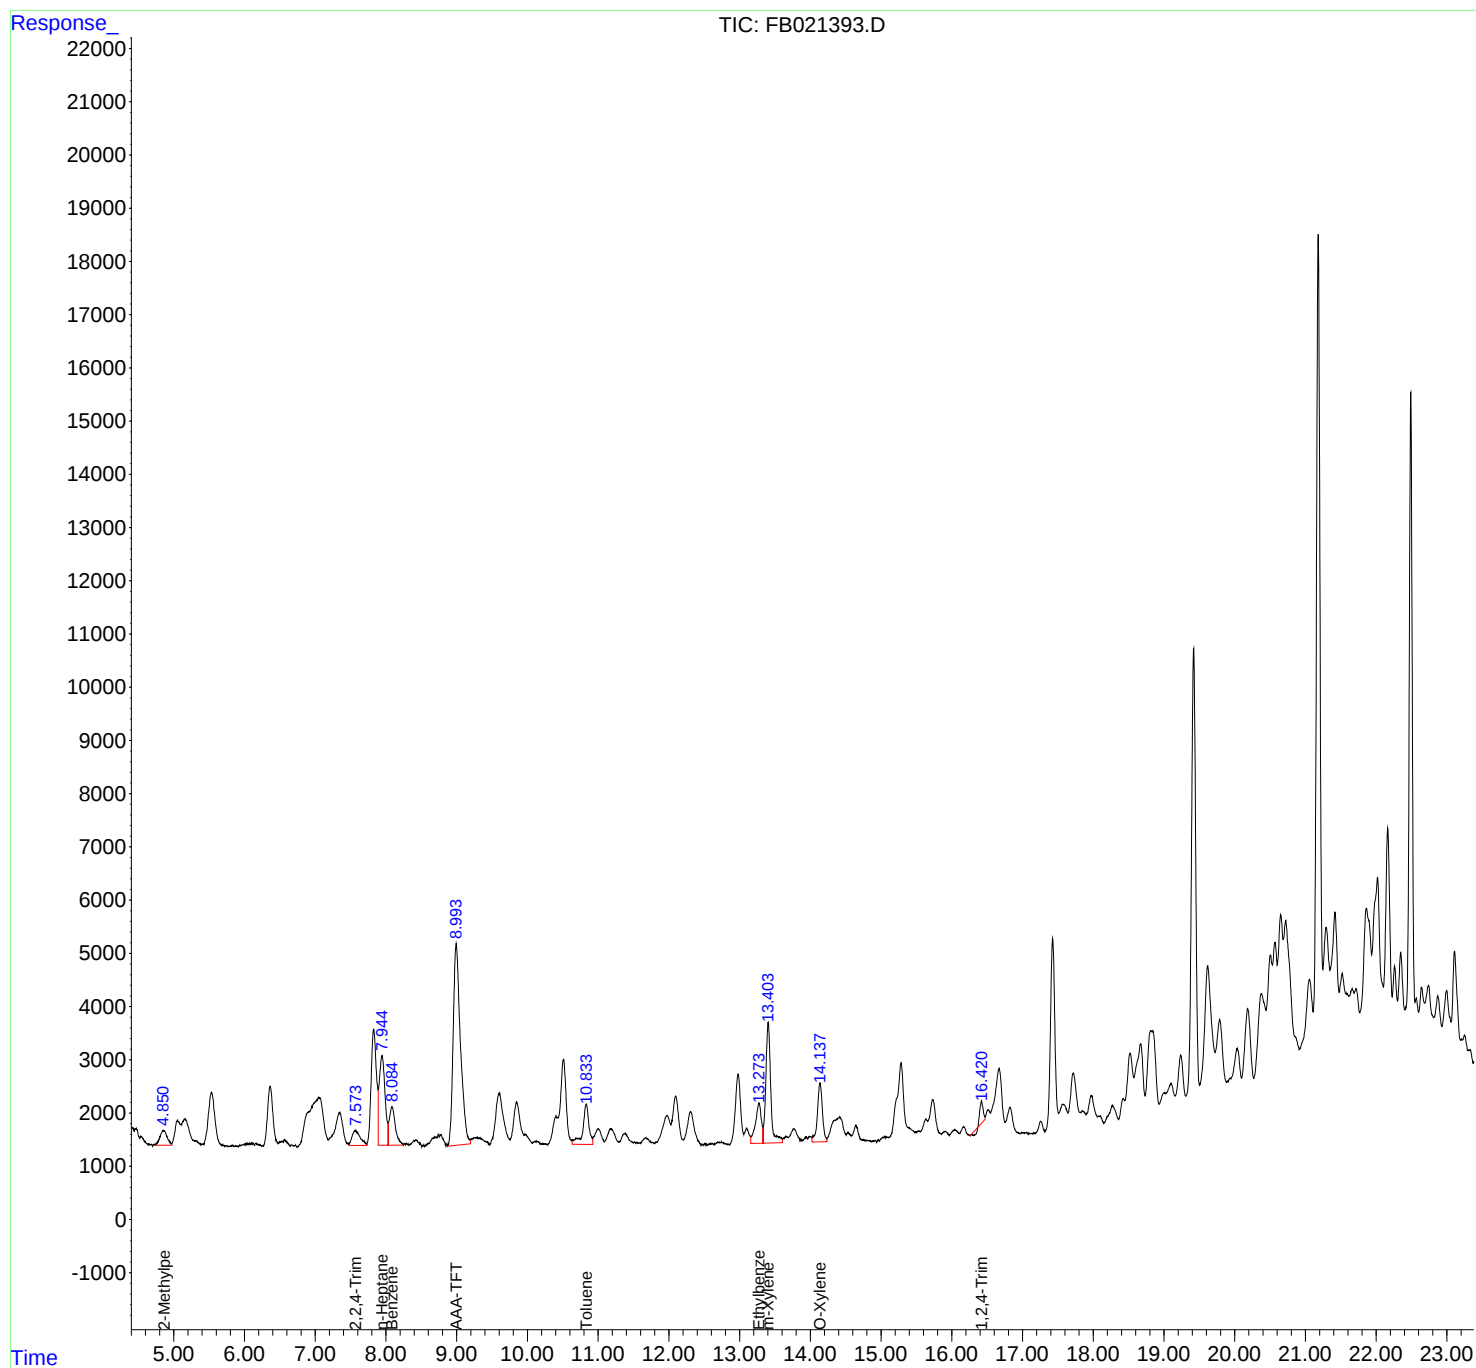

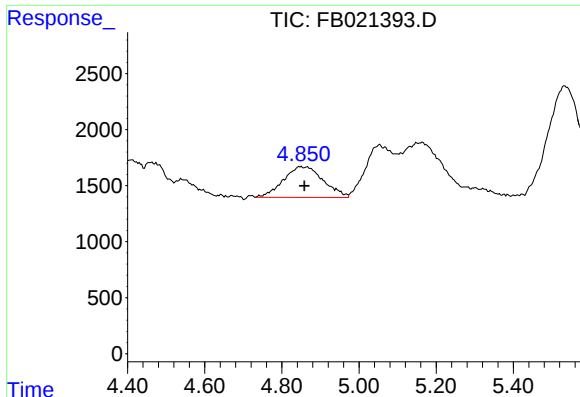


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: 0.008 min
Response: 19658
Conc: 0.52 ng/ml

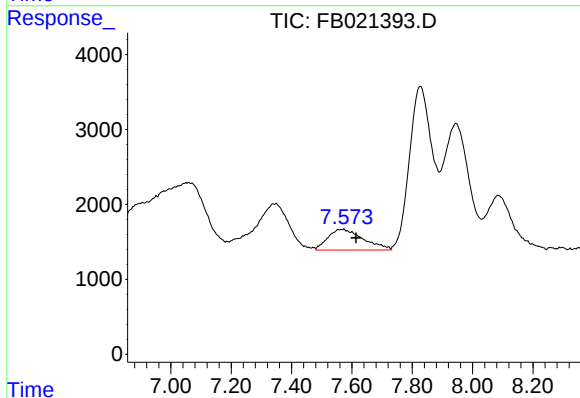


#2 2,2,4-Trimethylpentane

R.T.: 7.574 min
Delta R.T.: -0.040 min
Response: 22544
Conc: 0.66 ng/ml

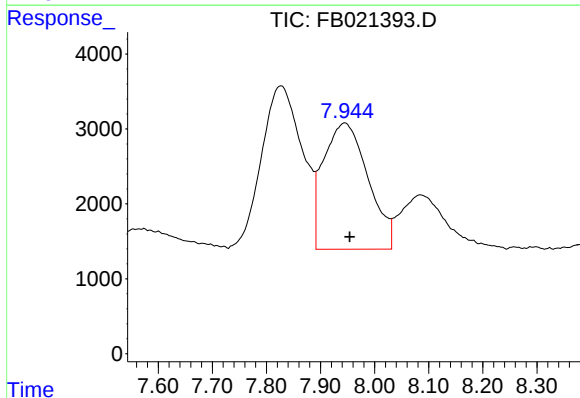


#3 n-Heptane

R.T.: 7.945 min
Delta R.T.: -0.009 min
Response: 96399
Conc: 2.96 ng/ml

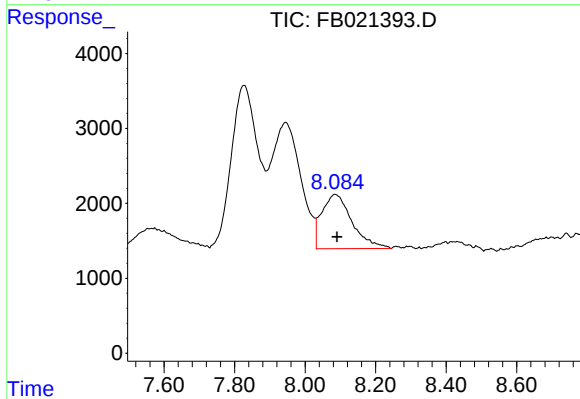


#4 Benzene

R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 43053
Conc: 1.25 ng/ml

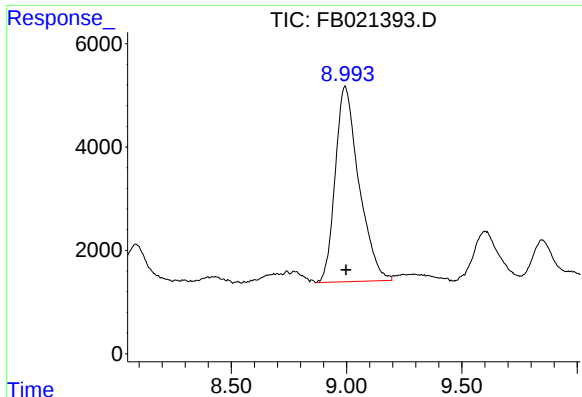


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: -0.005 min
Response: 269144
Conc: 18.25 ng/ml

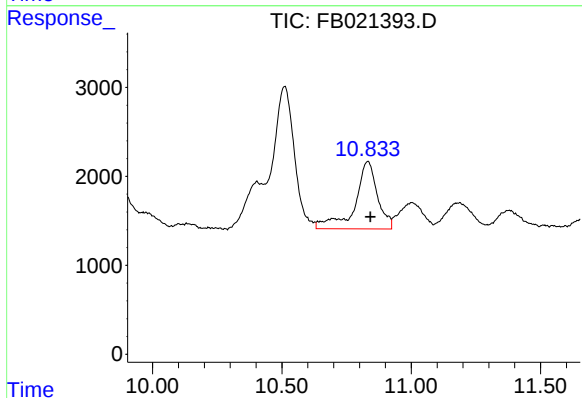


#6 Toluene

R.T.: 10.832 min
Delta R.T.: -0.010 min
Response: 45752
Conc: 1.93 ng/ml

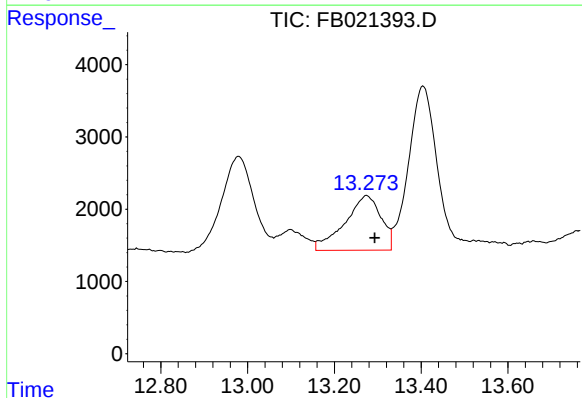


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.018 min
Response: 43759
Conc: 1.87 ng/ml

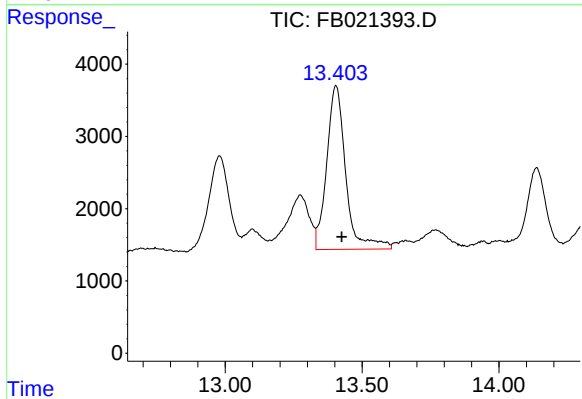


#8 m-Xylene

R.T.: 13.405 min
Delta R.T.: -0.021 min
Response: 109770
Conc: 4.40 ng/ml

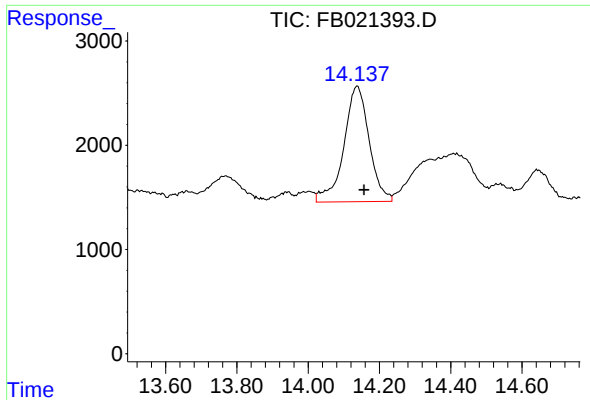

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.019 min
Response: 54714
Conc: 2.10 ng/ml

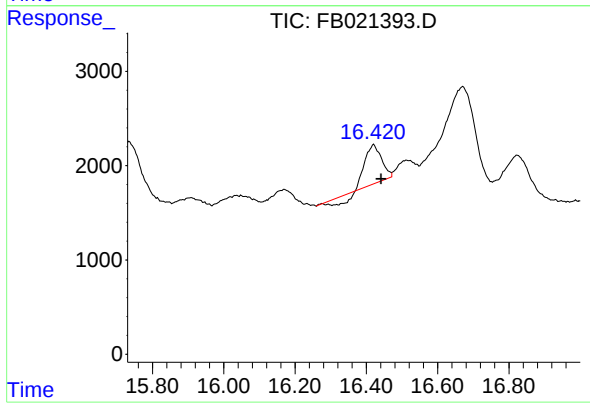

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min
Delta R.T.: -0.020 min
Response: 10552
Conc: 0.39 ng/ml