

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
 Data File : FB021390.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2019 22:08
 Operator : MJ/SJ
 Sample : K3369-13MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 14 22:55:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	298133	20.220 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	718347	19.108 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	809328	23.699 ng/ml
3) t n-Heptane	7.947	246156	7.551 ng/ml
4) t Benzene	8.088	277766	8.047 ng/ml
6) t Toluene	10.830	670758	28.299 ng/ml
7) t Ethylbenzene	13.275	204740	8.762 ng/ml
8) t m-Xylene	13.407	439317	17.601 ng/ml
9) t O-Xylene	14.137	461055	17.674 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	444150	16.538 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061419\
Data File : FB021390.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2019 22:08
Operator : MJ/SJ
Sample : K3369-13MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 14 22:55:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

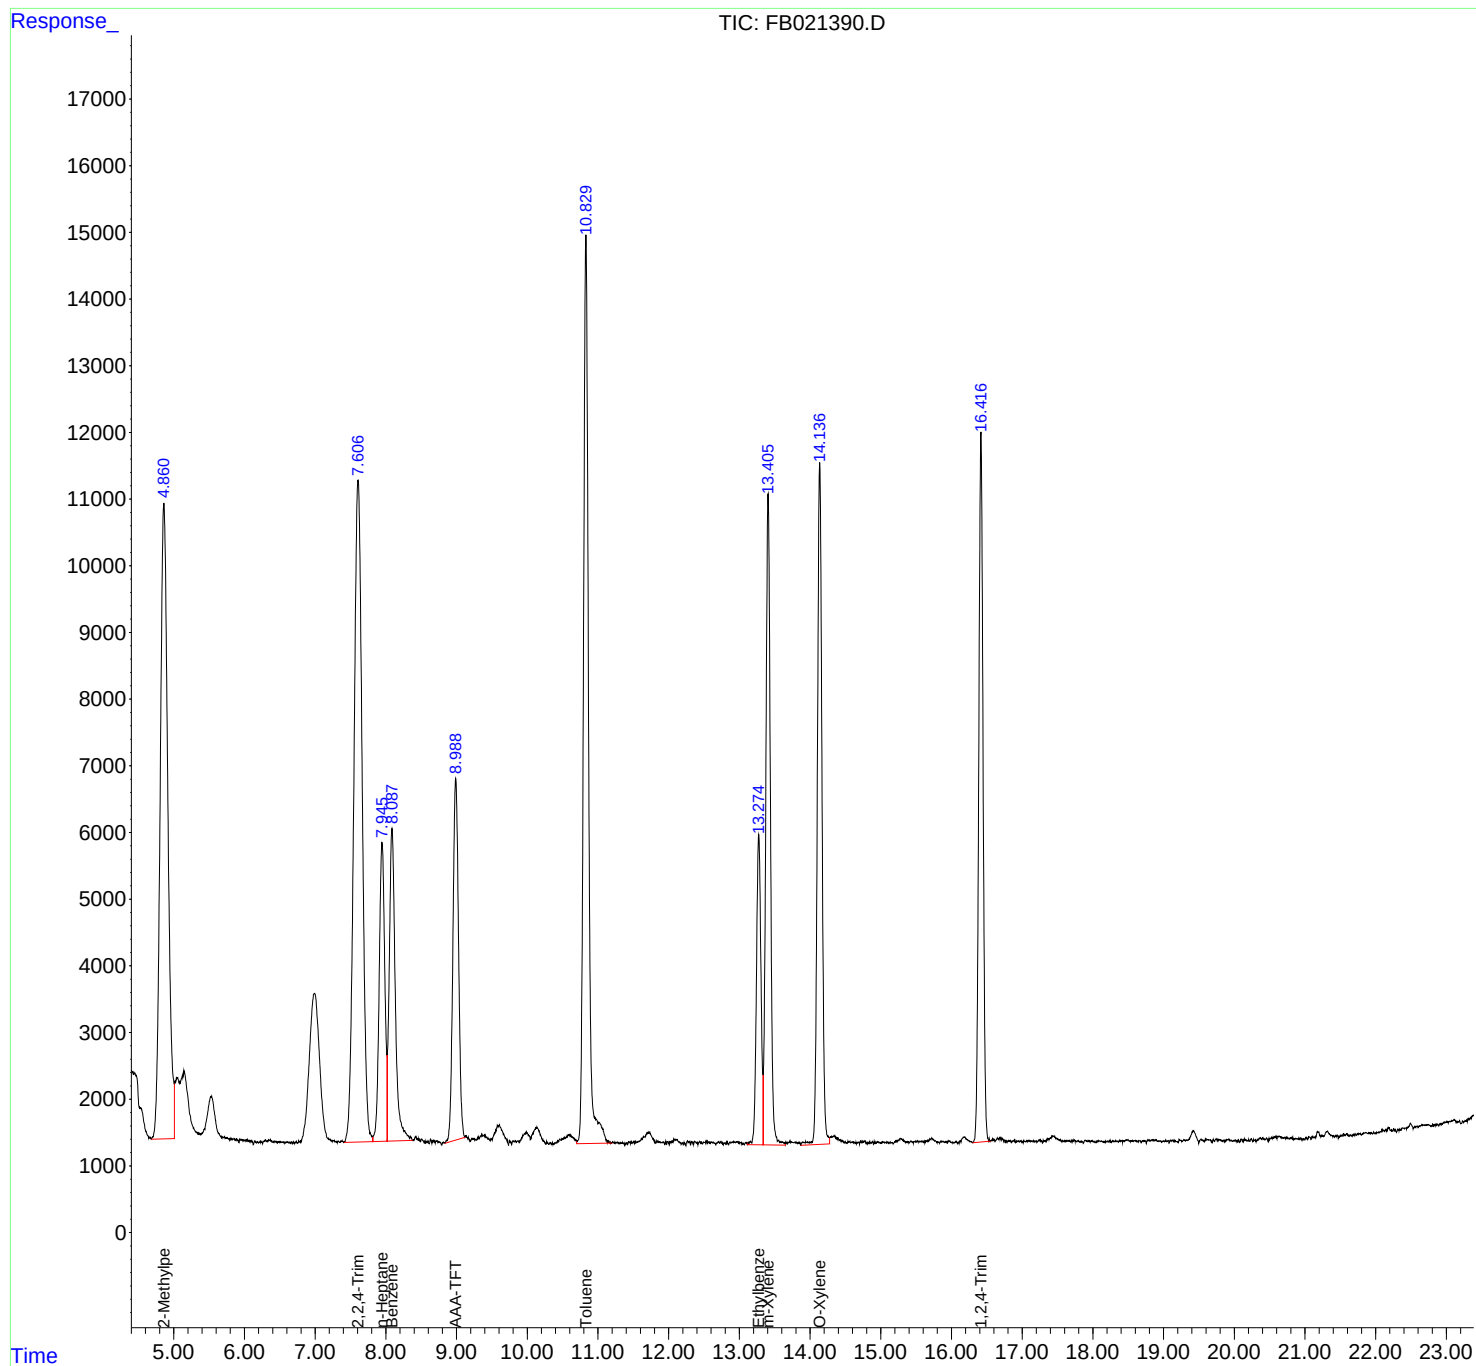

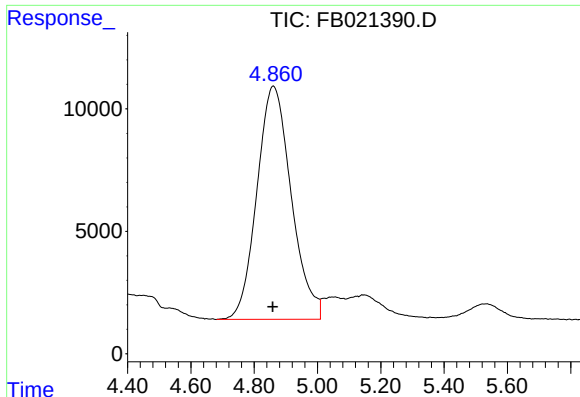


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: 0.003 min
Response: 718347
Conc: 19.11 ng/ml

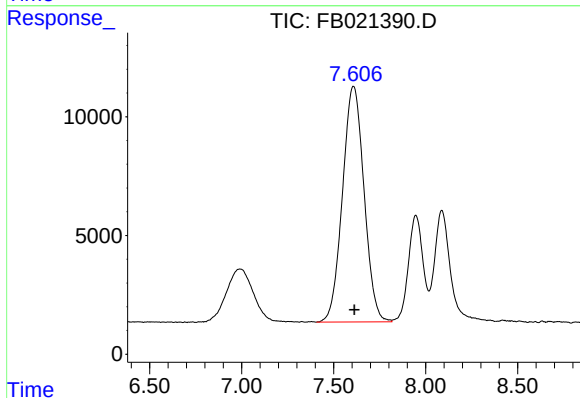


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: -0.006 min
Response: 809328
Conc: 23.70 ng/ml

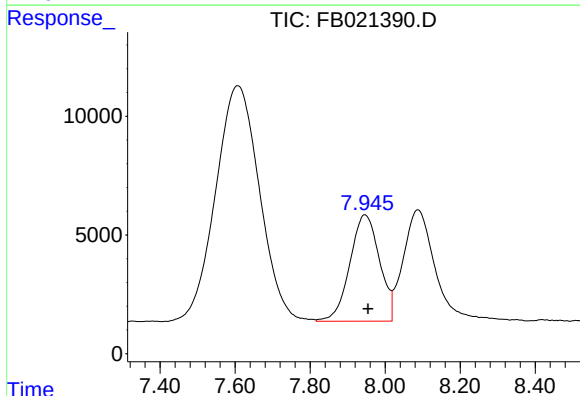


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: -0.007 min
Response: 246156
Conc: 7.55 ng/ml

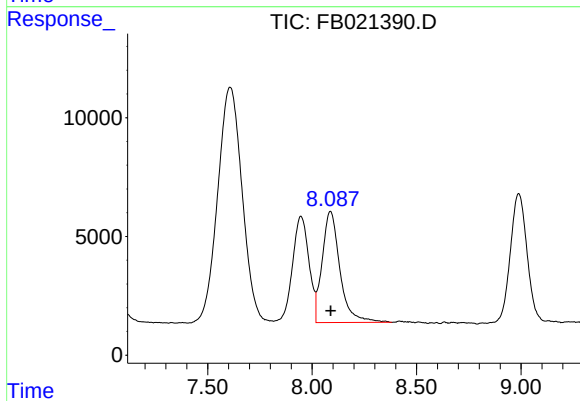


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.002 min
Response: 277766
Conc: 8.05 ng/ml

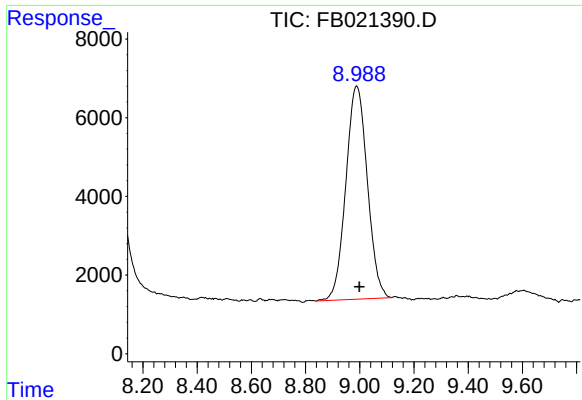


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.009 min
Response: 298133
Conc: 20.22 ng/ml

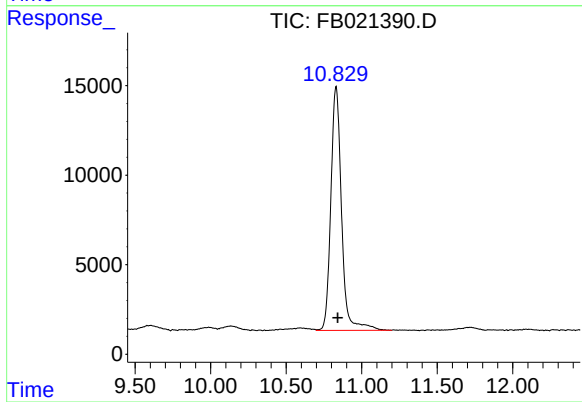


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.012 min
Response: 670758
Conc: 28.30 ng/ml

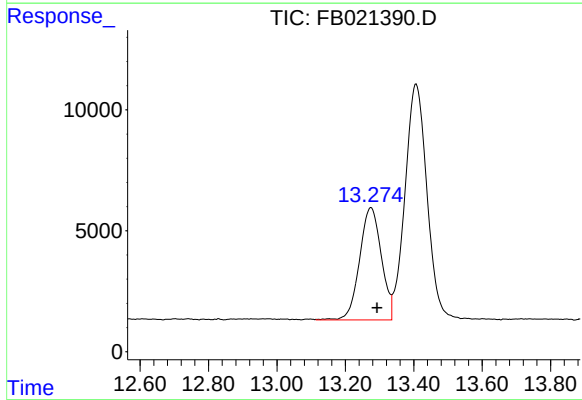


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.018 min
Response: 204740
Conc: 8.76 ng/ml

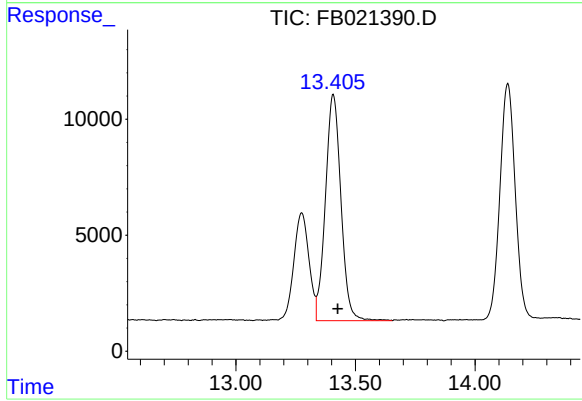


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.019 min
Response: 439317
Conc: 17.60 ng/ml

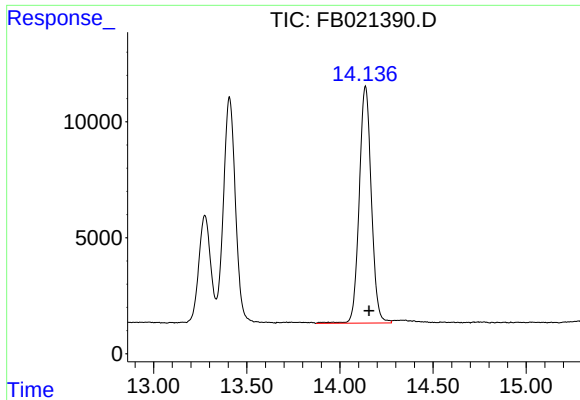

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.020 min
Response: 461055
Conc: 17.67 ng/ml

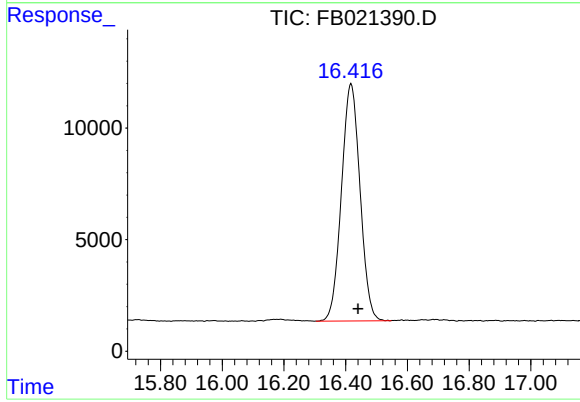

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.023 min
Response: 444150
Conc: 16.54 ng/ml