

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027437.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 21:20
 Operator : AJ/MA
 Sample : N3334-23 50X
 Misc : 5.06G/5.00 ML MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 15 03:15:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.832	596646	53.193 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.696	13653	0.810 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	718	0.041 ng/ml
3) t n-Heptane	7.788	96852	5.528 ng/ml
7) t Ethylbenzene	13.023	941524	51.991 ng/ml
8) t m-Xylene	13.180	114776	6.439 ng/ml
9) t O-Xylene	13.926	302969	17.436 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	923885	53.782 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027437.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 21:20
Operator : AJ/MA
Sample : N3334-23 50X
Misc : 5.06G/5.00 ML MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 15 03:15:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

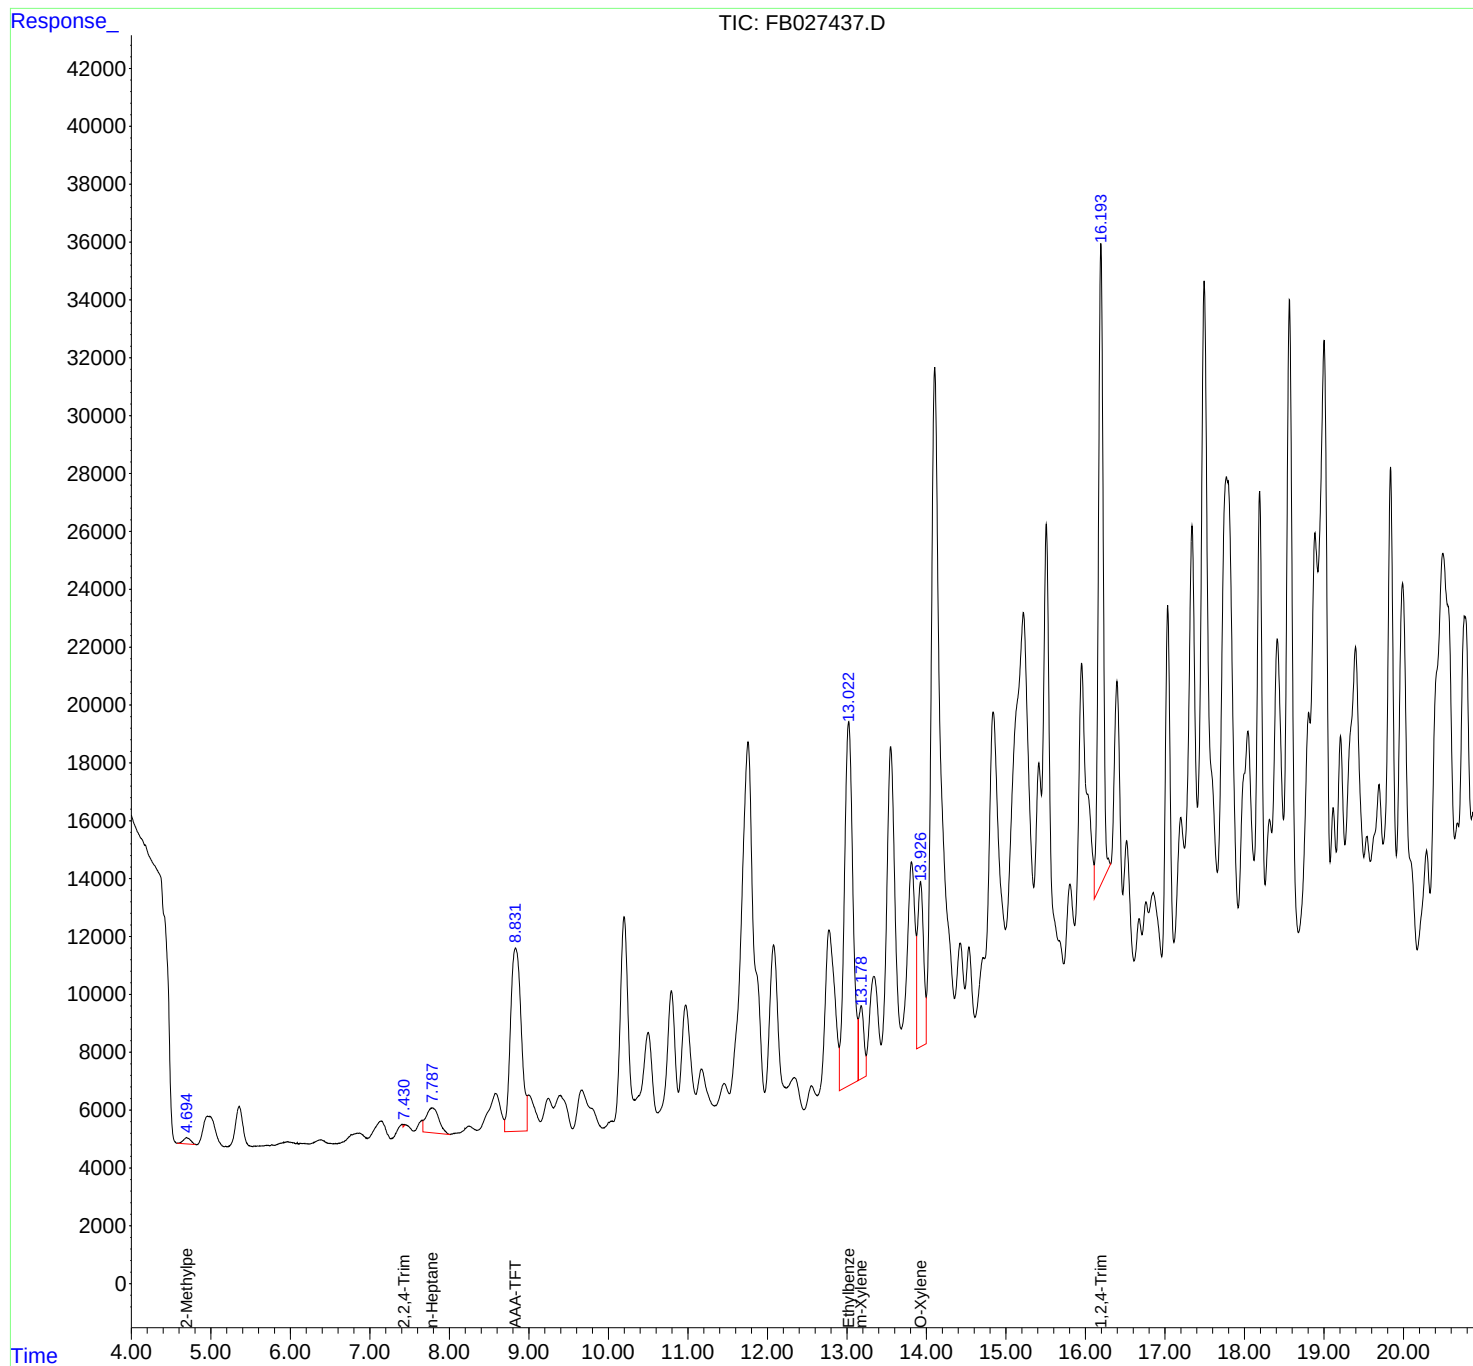


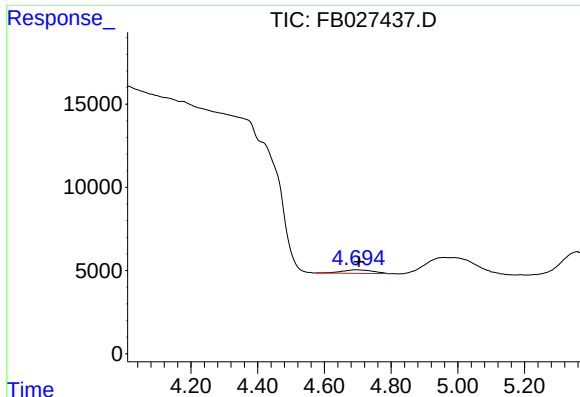

#1 2-Methylpentane


R.T.: 4.696 min
Delta R.T.: -0.008 min
Response: 13653
Conc: 0.81 ng/ml

Instrument :
FID_B
ClientSampleId :

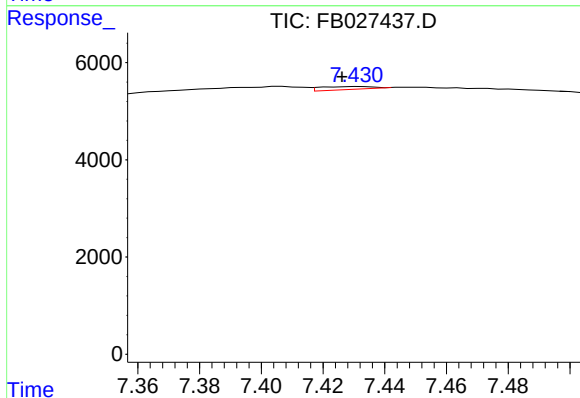


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: 0.006 min
Response: 718
Conc: 0.04 ng/ml

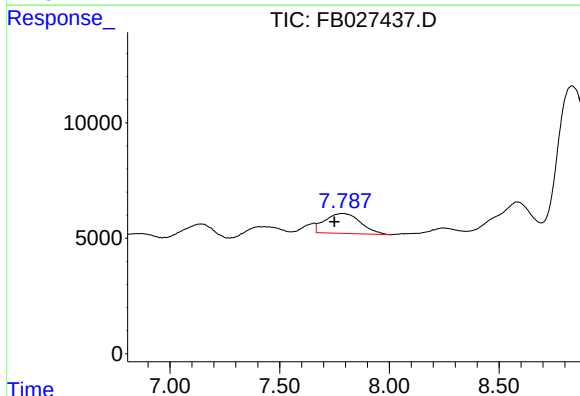


#3 n-Heptane

R.T.: 7.788 min
Delta R.T.: 0.038 min
Response: 96852
Conc: 5.53 ng/ml

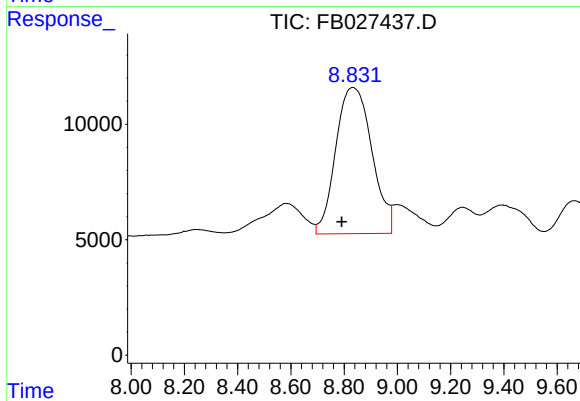

#5 AAA-TFT


R.T.: 8.832 min
Delta R.T.: 0.041 min
Response: 596646
Conc: 53.19 ng/ml

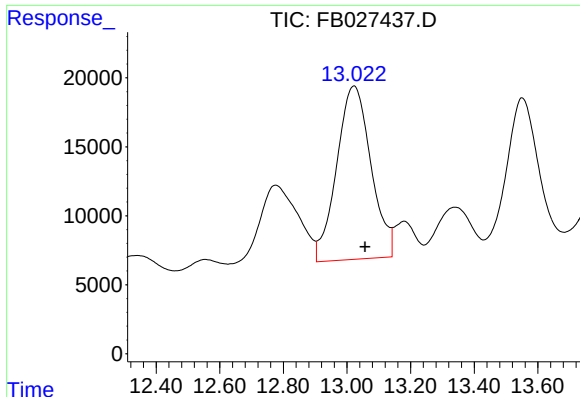

#7 Ethylbenzene


R.T.: 13.023 min
Delta R.T.: -0.034 min
Response: 941524
Conc: 51.99 ng/ml

Instrument :
FID_B
ClientSampleId :

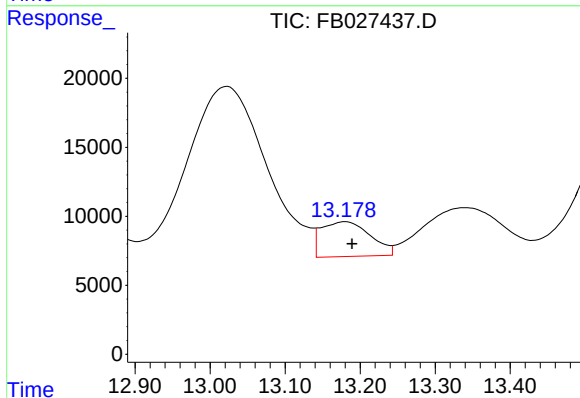


#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.009 min
Response: 114776
Conc: 6.44 ng/ml

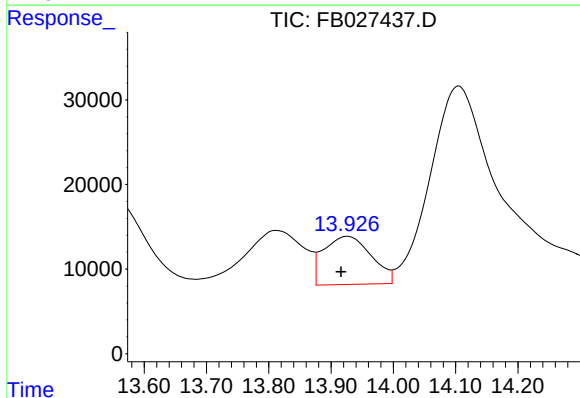

#9 o-Xylene

R.T.: 13.926 min
Delta R.T.: 0.010 min
Response: 302969
Conc: 17.44 ng/ml

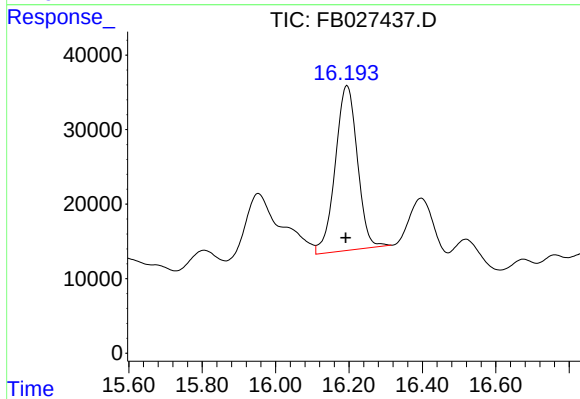

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 923885
Conc: 53.78 ng/ml