

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027438.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 21:57
 Operator : AJ/MA
 Sample : N3334-17
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 15 03:15:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1) t	2-Methylpentane	4.713	2050362	121.703 ng/ml
2) t	2,2,4-Trimethylpentane	7.389	4759185	271.049 ng/ml
3) t	n-Heptane	7.759	9173061	523.613 ng/ml
7) t	Ethylbenzene	13.032	16454985	908.643 ng/ml
8) t	m-Xylene	13.185	5538556	310.700 ng/ml
9) t	O-Xylene	13.925	7221770	415.618 ng/ml
10) t	1,2,4-Trimethylbenzene	16.201	8352607	486.229 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027438.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 21:57
Operator : AJ/MA
Sample : N3334-17
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 15 03:15:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

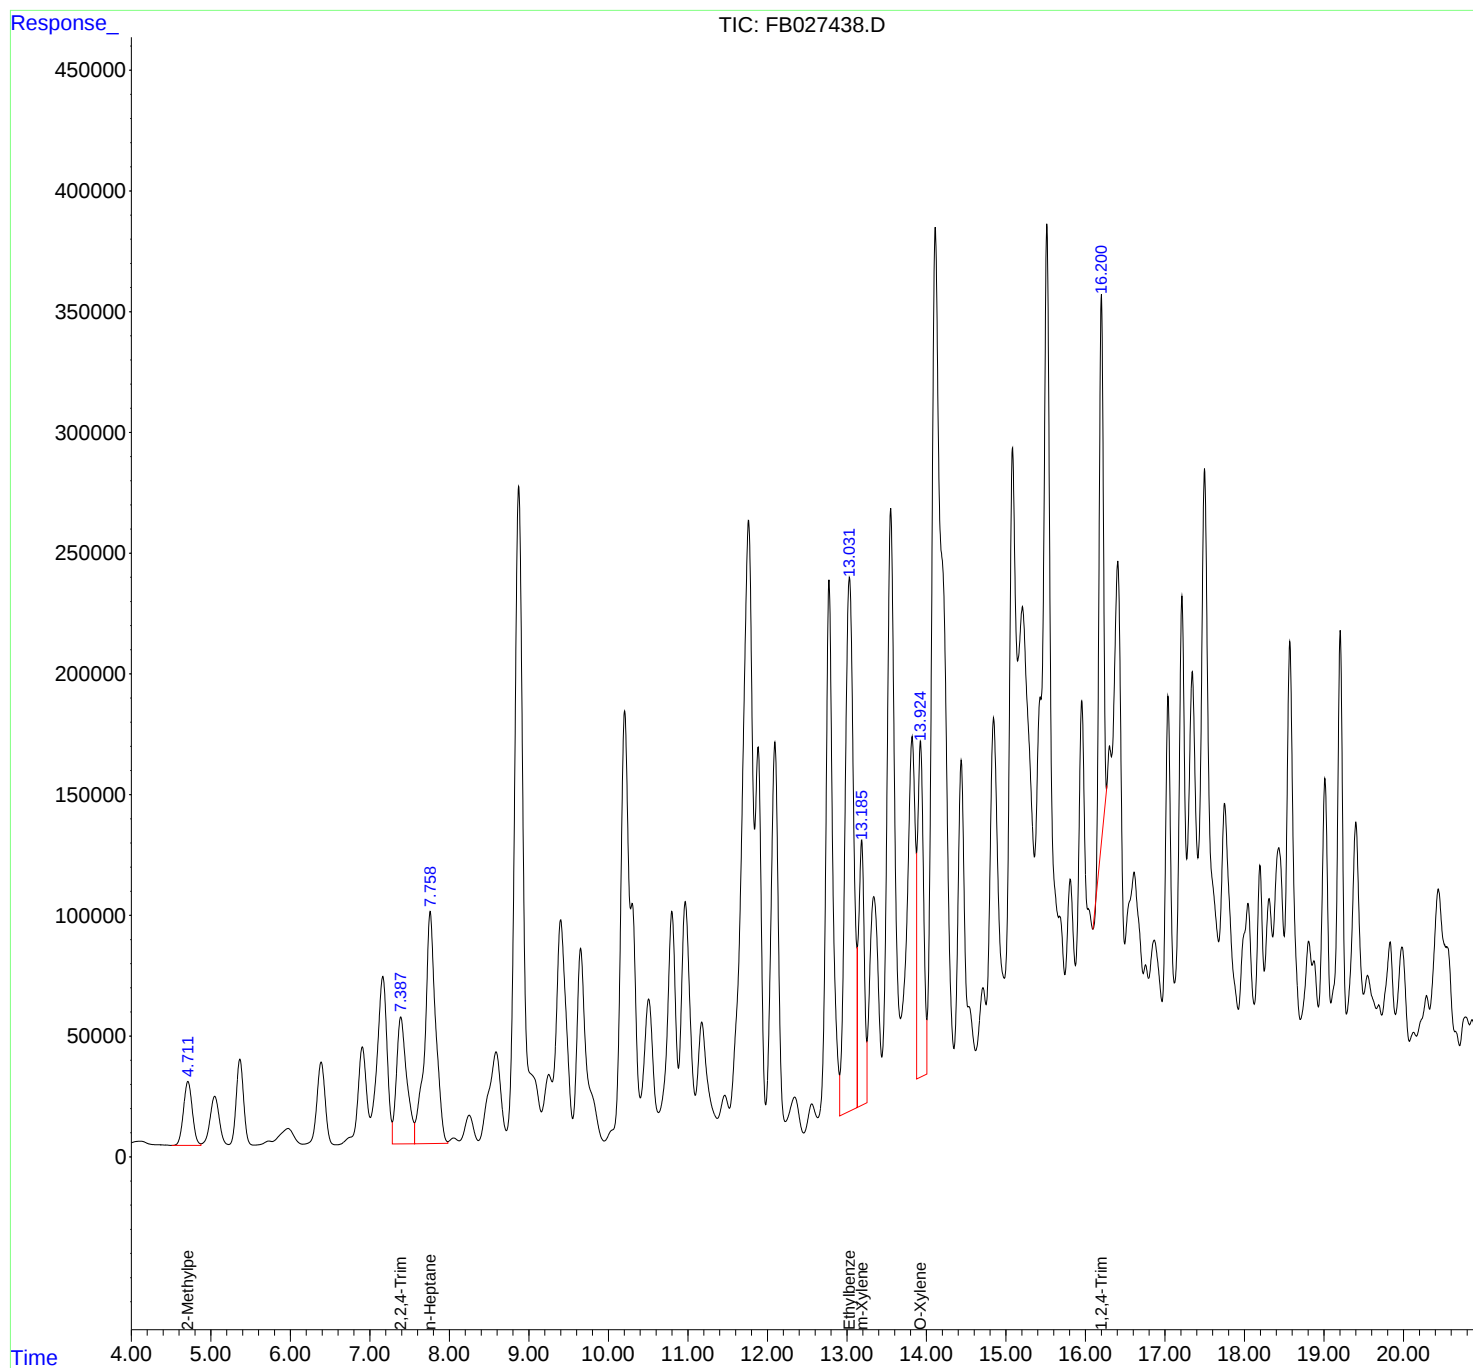


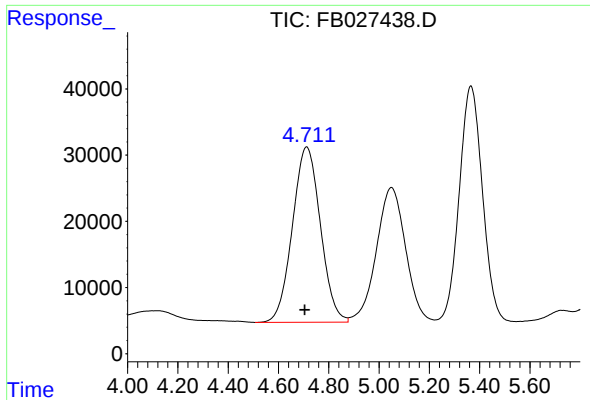

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.009 min
Response: 2050362
Conc: 121.70 ng/ml

Instrument :
FID_B
ClientSampleId :

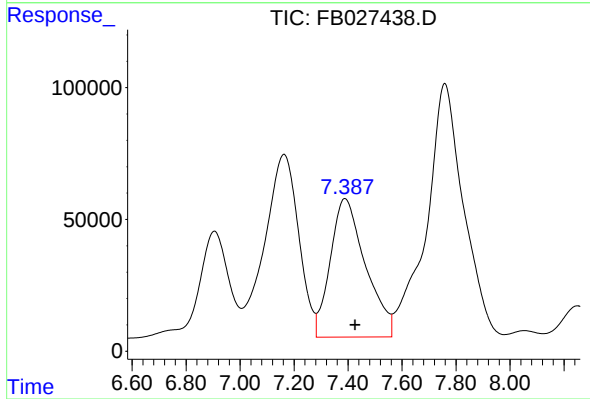


#2 2,2,4-Trimethylpentane

R.T.: 7.389 min
Delta R.T.: -0.037 min
Response: 4759185
Conc: 271.05 ng/ml

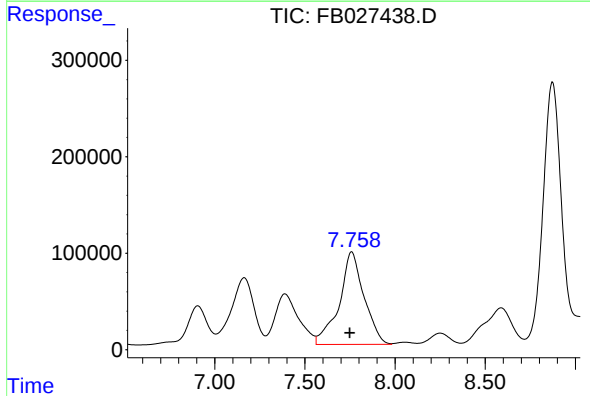


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.009 min
Response: 9173061
Conc: 523.61 ng/ml

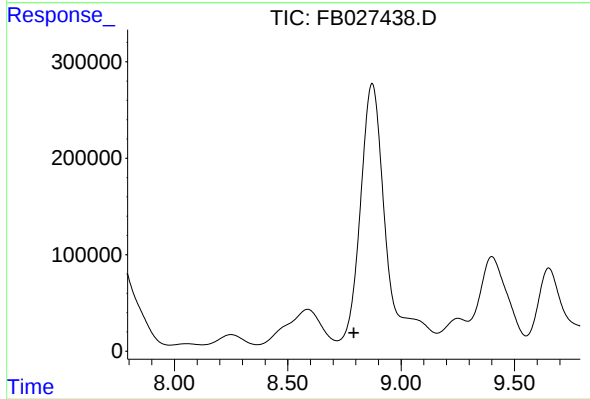

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T. : 8.791 min
Response: 0
Conc: N.D.

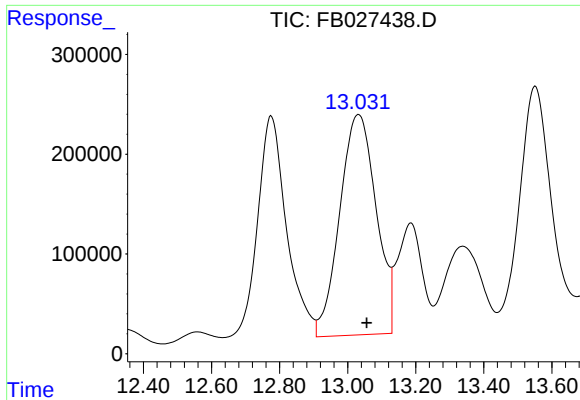

#7 Ethylbenzene


R.T.: 13.032 min
Delta R.T.: -0.025 min
Response: 16454985
Conc: 908.64 ng/ml

Instrument :
FID_B
ClientSampleId :

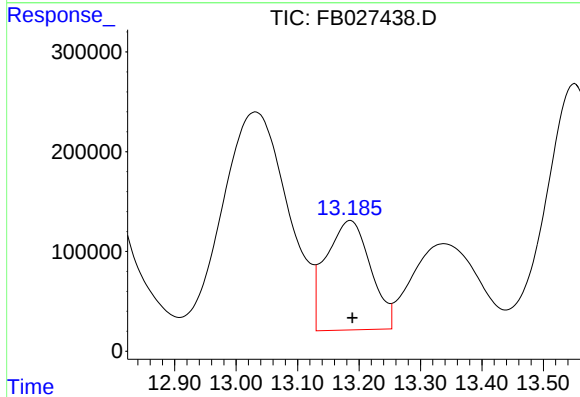


#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.004 min
Response: 5538556
Conc: 310.70 ng/ml

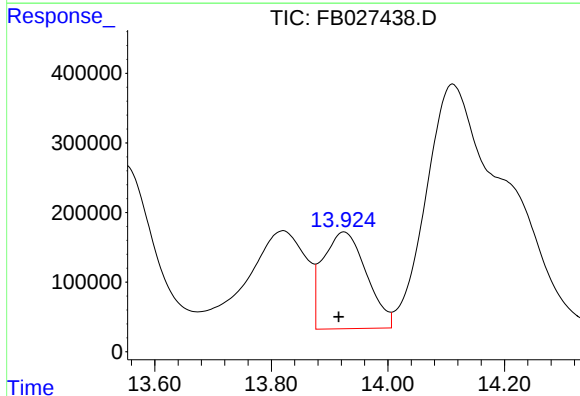

#9 o-Xylene

R.T.: 13.925 min
Delta R.T.: 0.009 min
Response: 7221770
Conc: 415.62 ng/ml

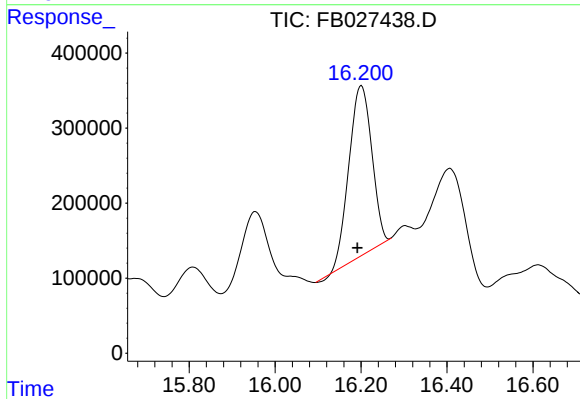

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.010 min
Response: 8352607
Conc: 486.23 ng/ml