

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027439.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 22:34
 Operator : AJ/MA
 Sample : N3334-23MS
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 15 03:15:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.857	704095	62.772 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	40713	2.417 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	157882	8.992 ng/ml
3) t n-Heptane	7.780	334546	19.096 ng/ml
6) t Toluene	10.633	59252	3.060 ng/ml
7) t Ethylbenzene	13.021	1649376	91.078 ng/ml
9) t O-Xylene	13.926	270654	15.576 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	259681	15.117 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027439.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 22:34
Operator : AJ/MA
Sample : N3334-23MS
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 15 03:15:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

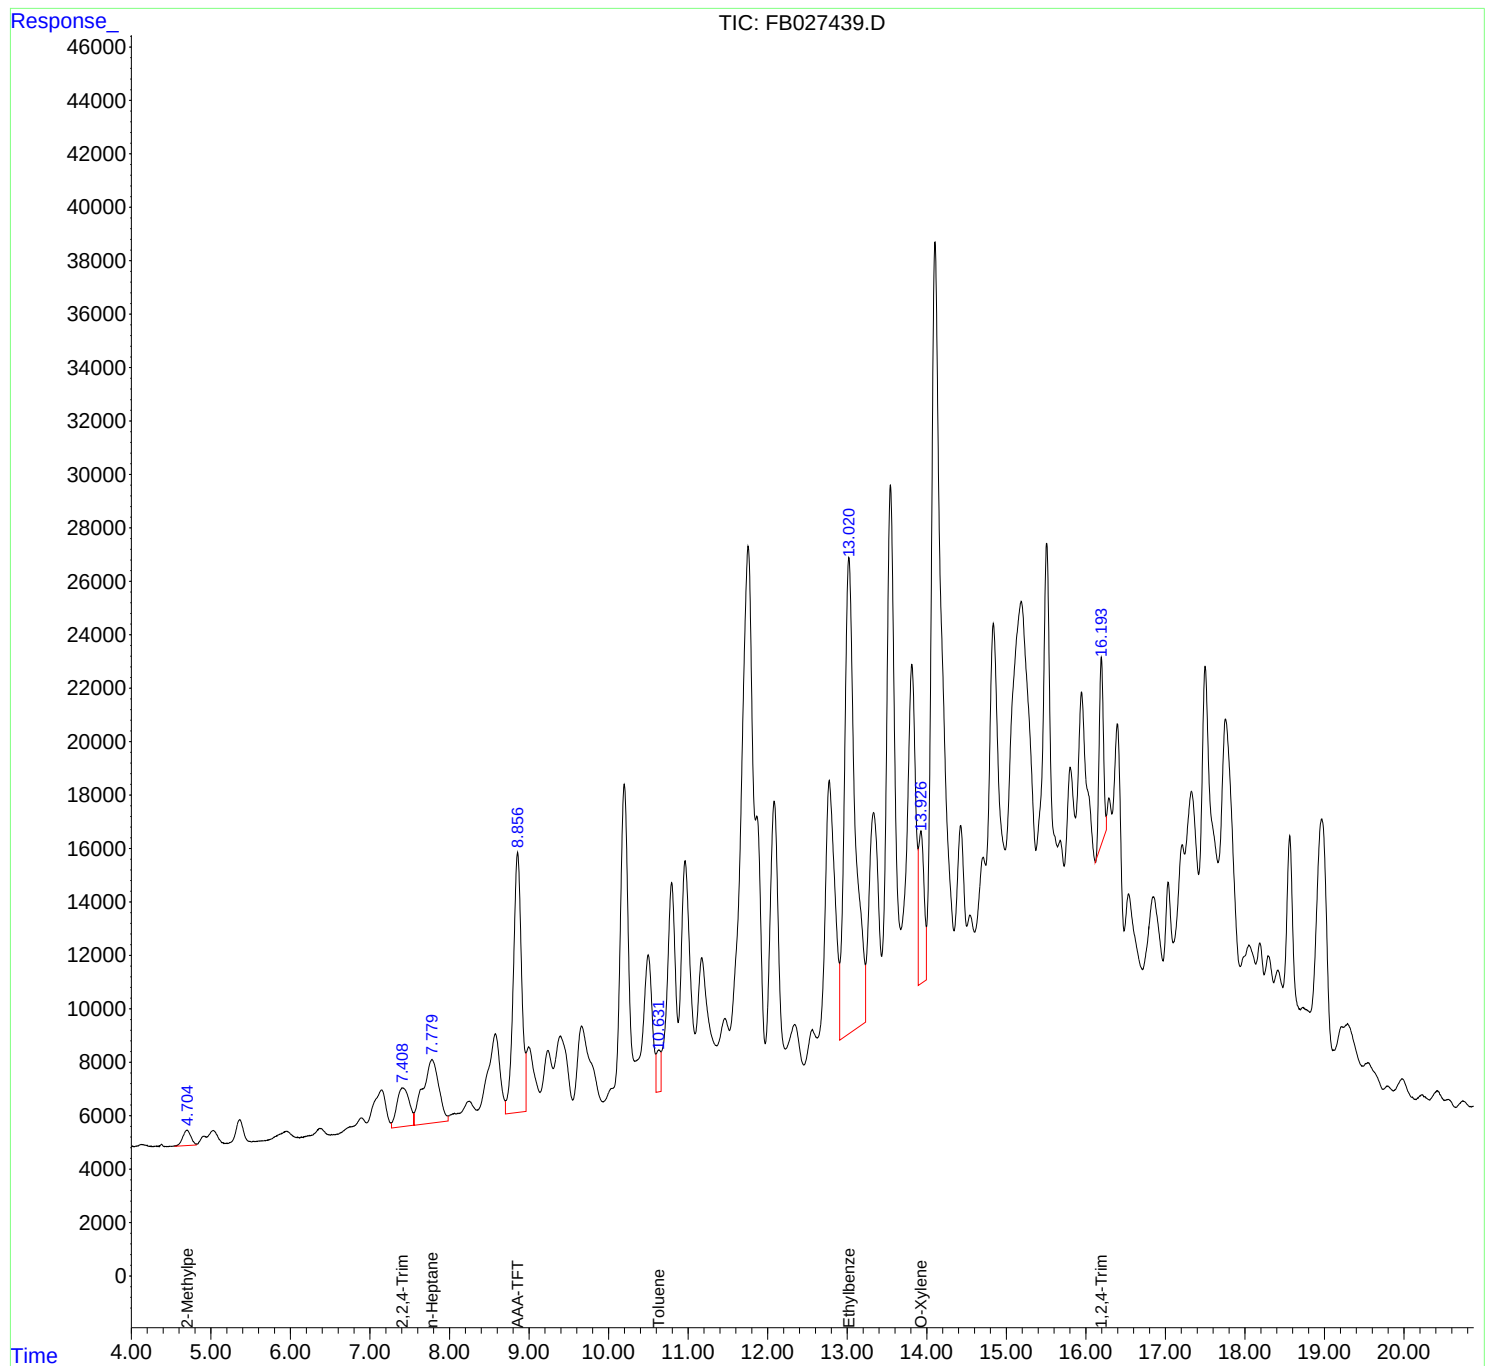


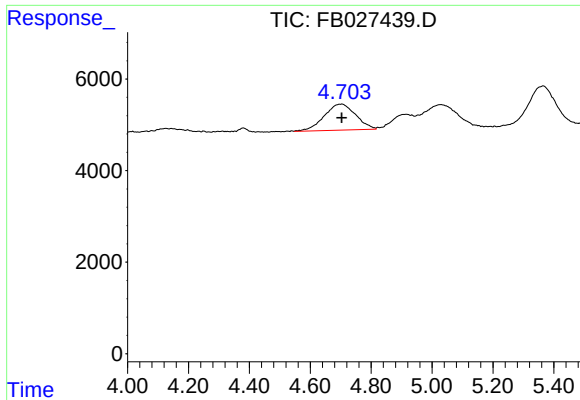

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.001 min
Response: 40713
Conc: 2.42 ng/ml

Instrument :
FID_B
ClientSampleId :

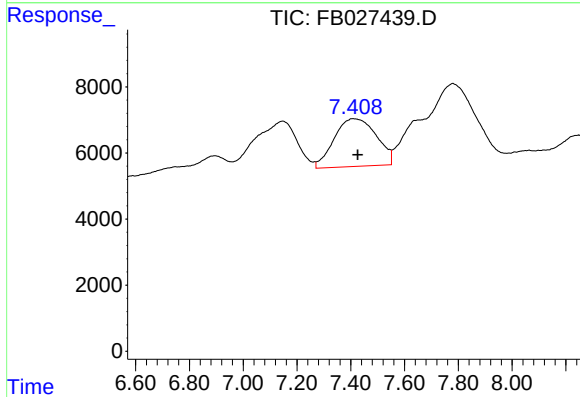


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.017 min
Response: 157882
Conc: 8.99 ng/ml

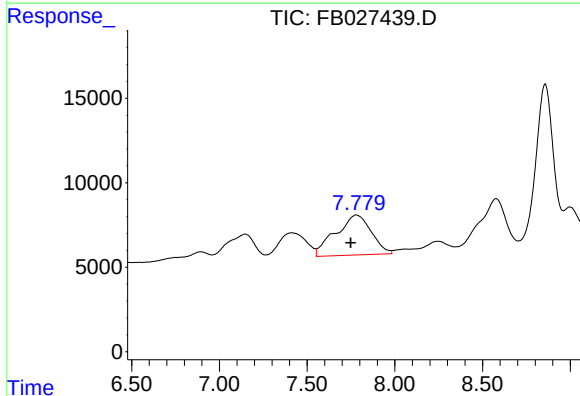


#3 n-Heptane

R.T.: 7.780 min
Delta R.T.: 0.031 min
Response: 334546
Conc: 19.10 ng/ml

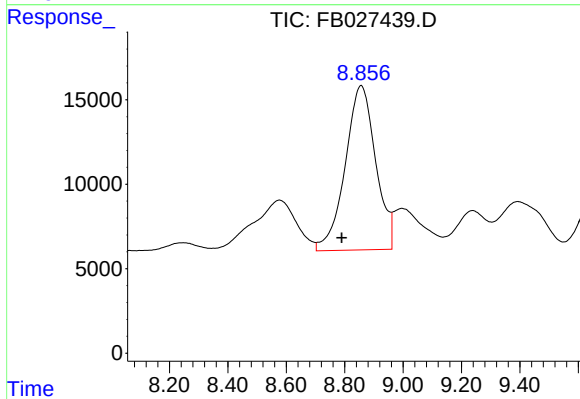

#5 AAA-TFT


R.T.: 8.857 min
Delta R.T.: 0.066 min
Response: 704095
Conc: 62.77 ng/ml

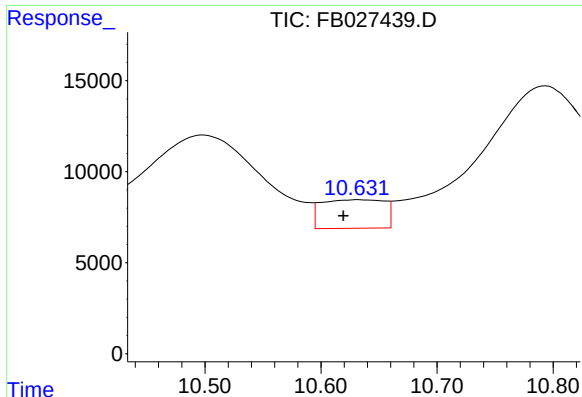

#6 Toluene


R.T.: 10.633 min
Delta R.T.: 0.013 min
Response: 59252
Conc: 3.06 ng/ml

Instrument :
FID_B
ClientSampleId :

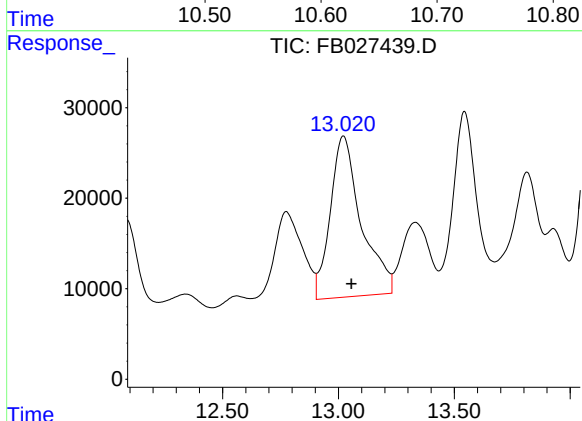


#7 Ethylbenzene

R.T.: 13.021 min
Delta R.T.: -0.035 min
Response: 1649376
Conc: 91.08 ng/ml

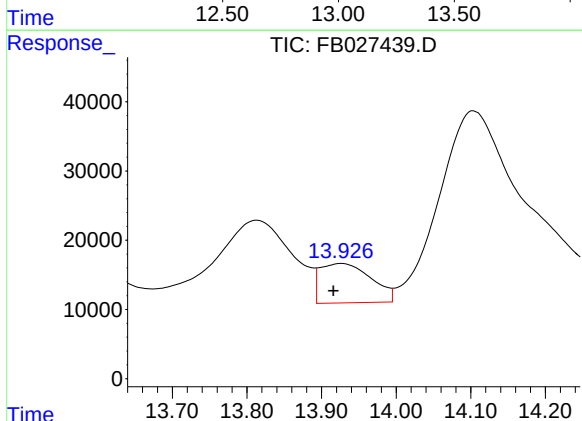

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.010 min
Response: 270654
Conc: 15.58 ng/ml

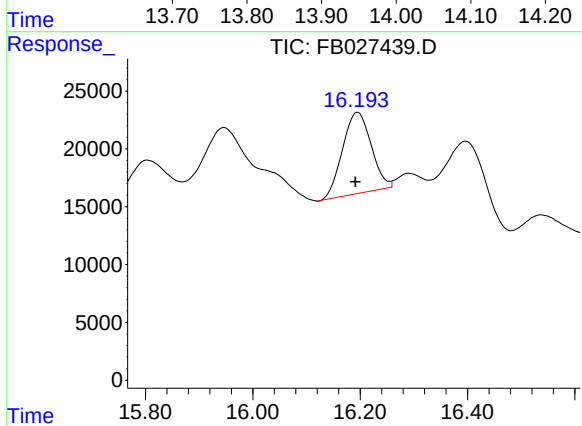

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 259681
Conc: 15.12 ng/ml