

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027440.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 23:11
 Operator : AJ/MA
 Sample : N3334-23MSD
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 15 03:15:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.858	1131353	100.863 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	60498	3.591 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	197359	11.240 ng/ml
3) t n-Heptane	7.784	462475	26.399 ng/ml
6) t Toluene	10.631	135584	7.003 ng/ml
7) t Ethylbenzene	13.022	4346565	240.017 ng/ml
9) t O-Xylene	13.924	879404	50.610 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	1455871	84.750 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027440.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 23:11
Operator : AJ/MA
Sample : N3334-23MSD
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 15 03:15:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

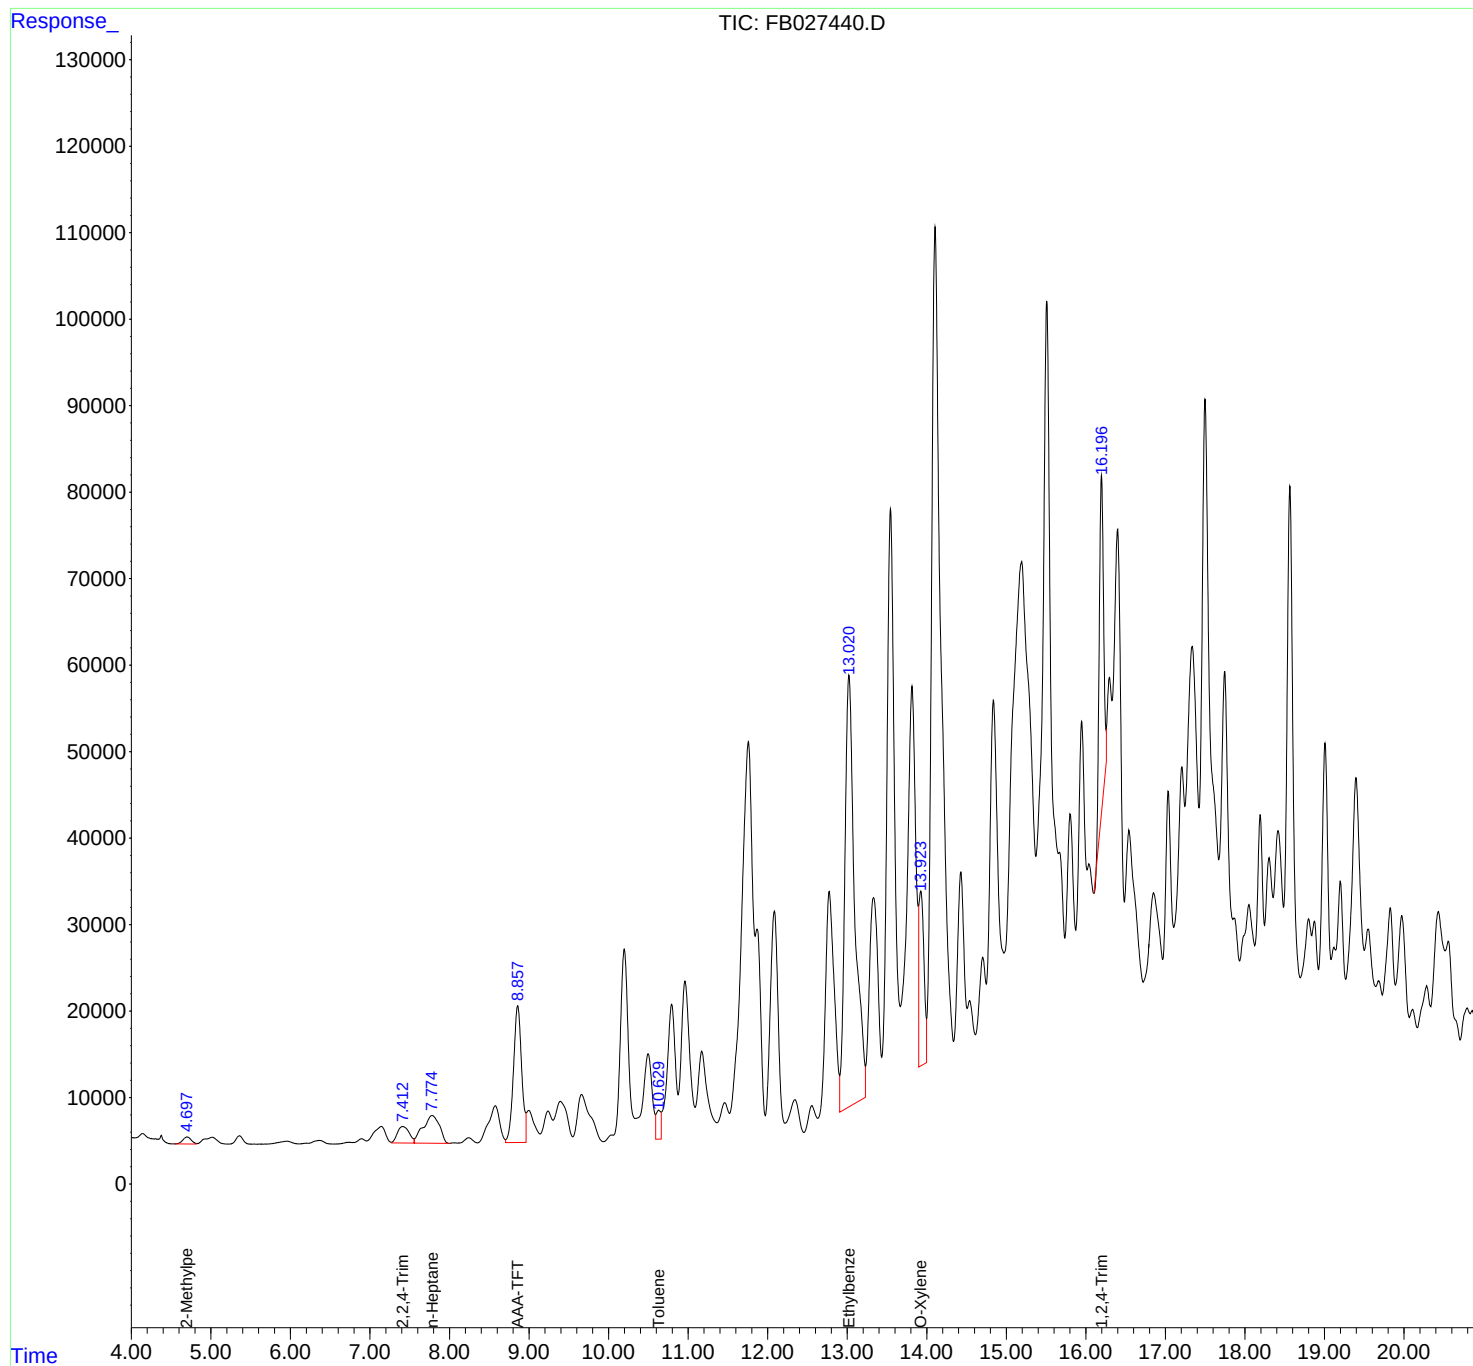


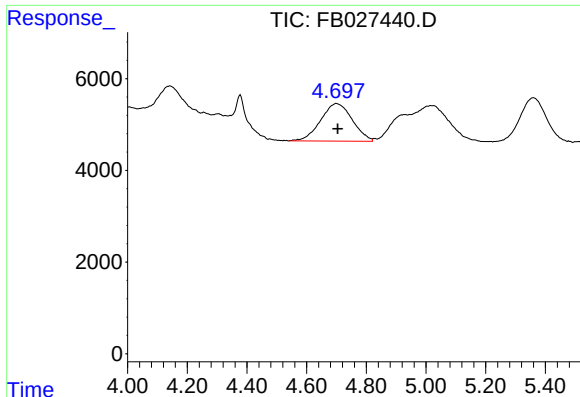

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.005 min
Response: 60498
Conc: 3.59 ng/ml

Instrument :
FID_B
ClientSampleId :

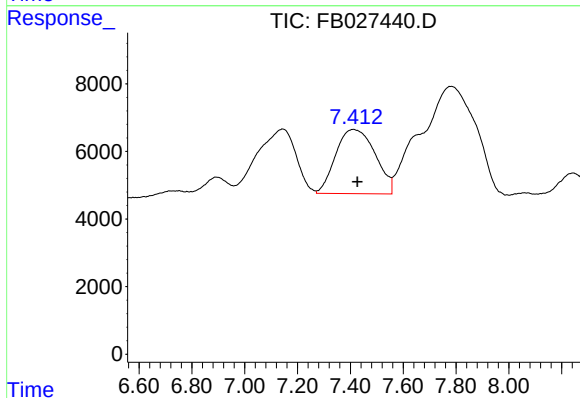


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.013 min
Response: 197359
Conc: 11.24 ng/ml

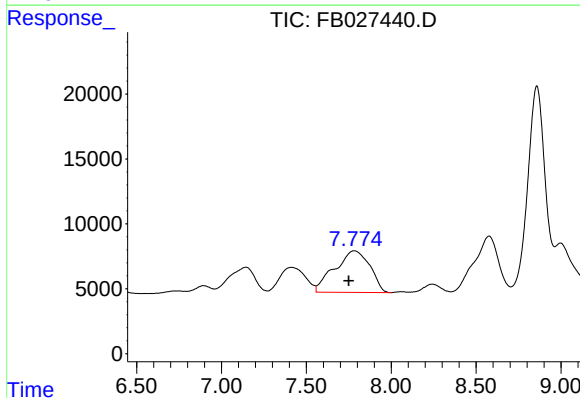


#3 n-Heptane

R.T.: 7.784 min
Delta R.T.: 0.034 min
Response: 462475
Conc: 26.40 ng/ml

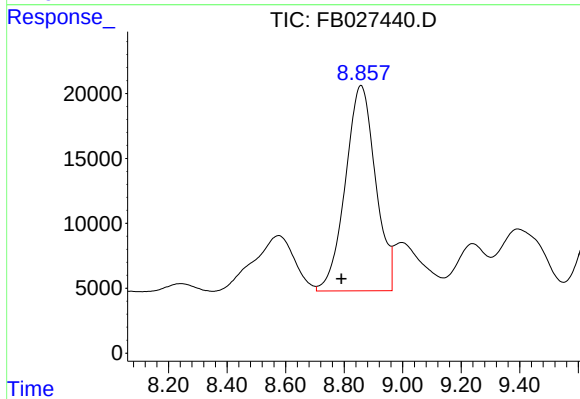

#5 AAA-TFT


R.T.: 8.858 min
Delta R.T.: 0.068 min
Response: 1131353
Conc: 100.86 ng/ml

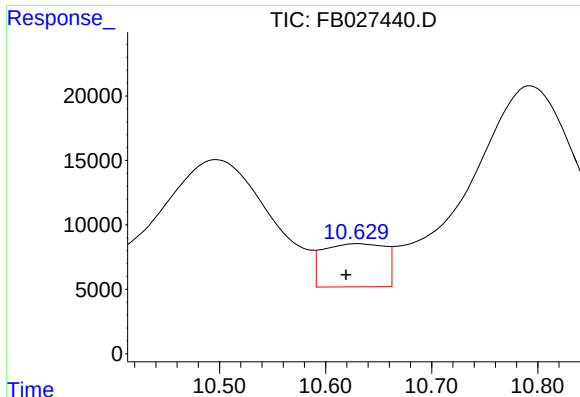

#6 Toluene


R.T.: 10.631 min
Delta R.T.: 0.011 min
Response: 135584
Conc: 7.00 ng/ml

Instrument :
FID_B
ClientSampleId :

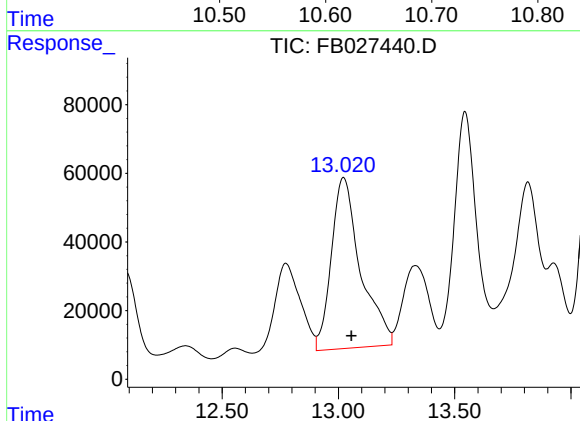


#7 Ethylbenzene

R.T.: 13.022 min
Delta R.T.: -0.034 min
Response: 4346565
Conc: 240.02 ng/ml

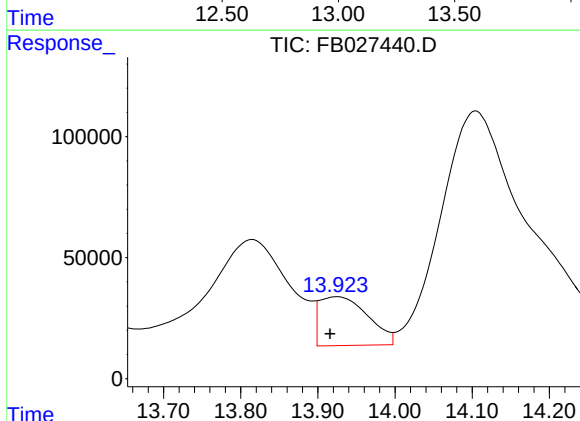

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.008 min
Response: 879404
Conc: 50.61 ng/ml

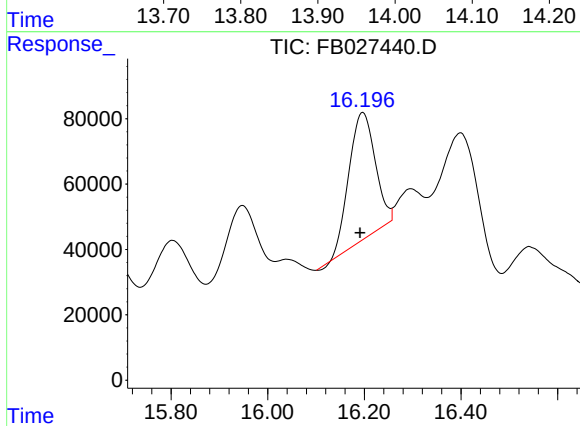

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.006 min
Response: 1455871
Conc: 84.75 ng/ml