

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027423.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 11:33
 Operator : AJ/MA
 Sample : BSF0614S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0614S1

Integration File: SAMPLE.e
 Quant Time: Jun 15 03:13:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	241645	21.543 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	457981	27.184 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	485937	27.676 ng/ml
3) t n-Heptane	7.750	157672	9.000 ng/ml
4) t Benzene	7.887	181596	8.905 ng/ml
6) t Toluene	10.619	514695	26.583 ng/ml
7) t Ethylbenzene	13.056	160562	8.866 ng/ml
8) t m-Xylene	13.189	320067	17.955 ng/ml
9) t O-Xylene	13.916	319571	18.392 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	324543	18.893 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027423.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 11:33
Operator : AJ/MA
Sample : BSF0614S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0614S1

Integration File: SAMPLE.e
Quant Time: Jun 15 03:13:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

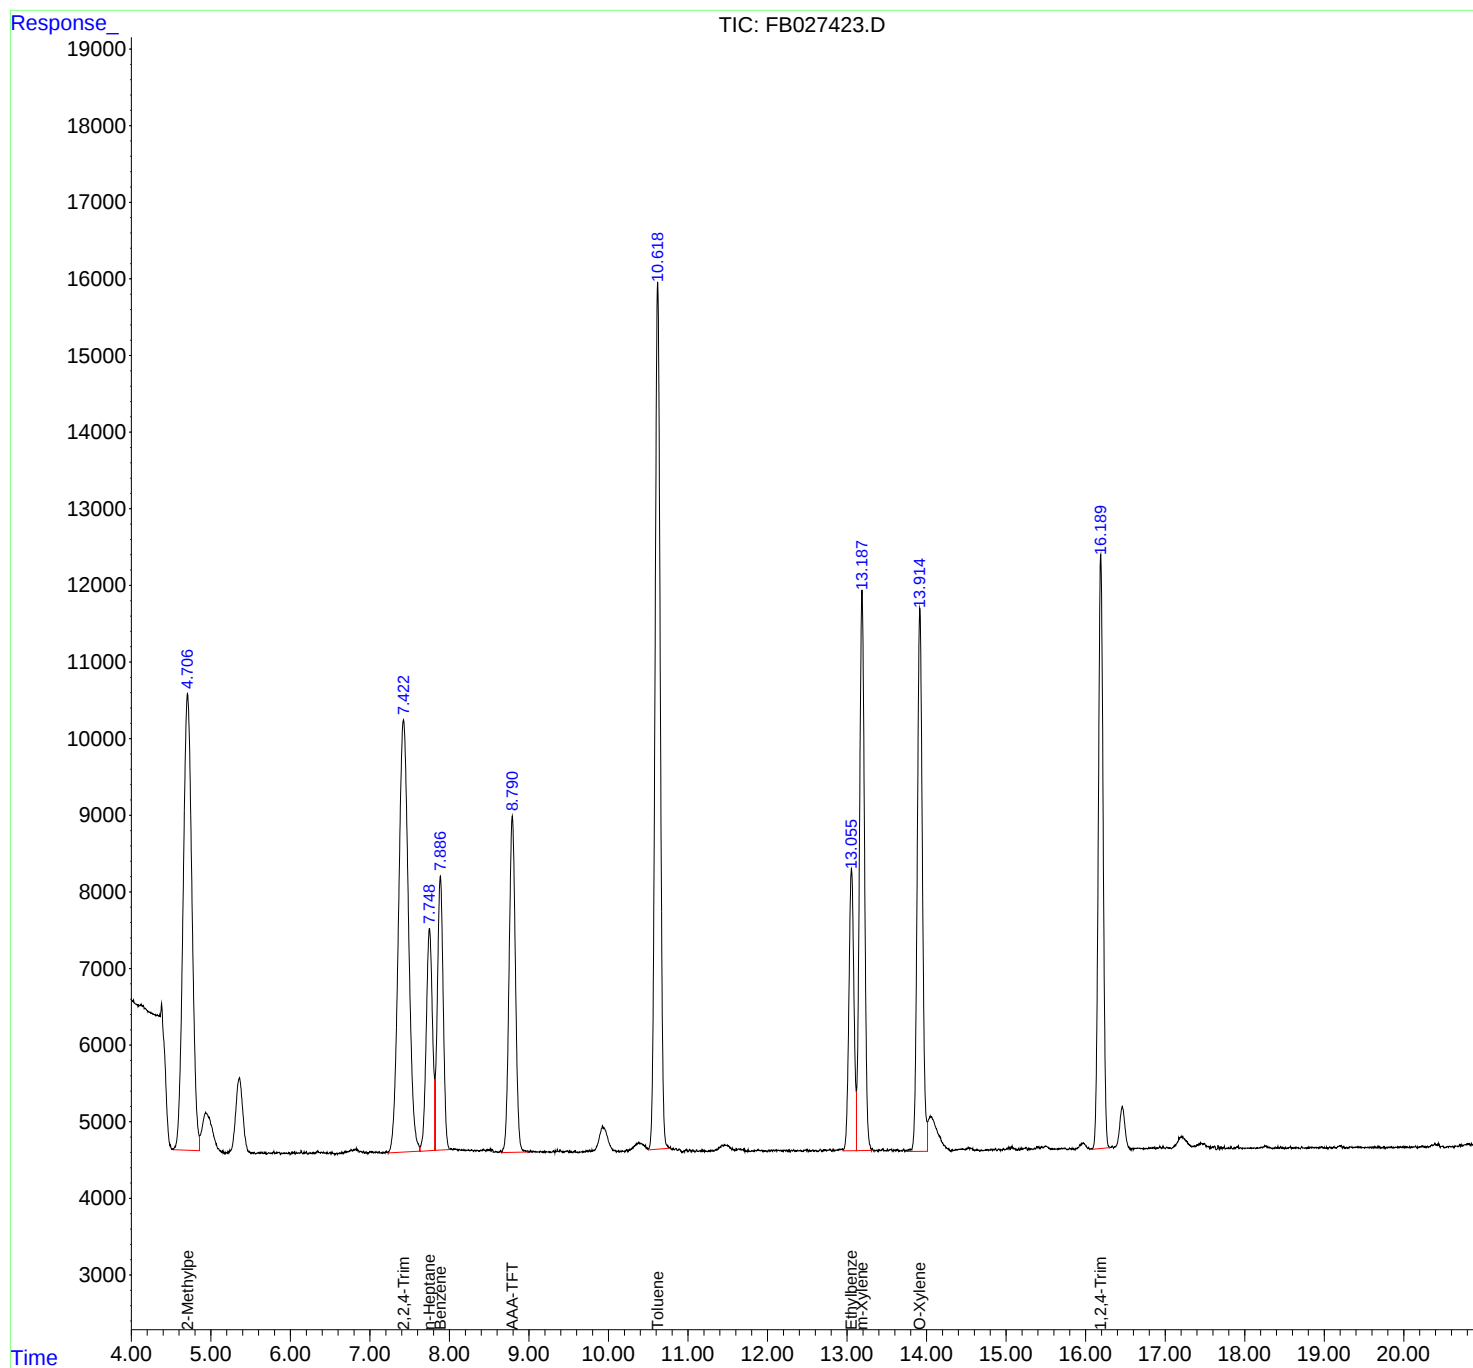


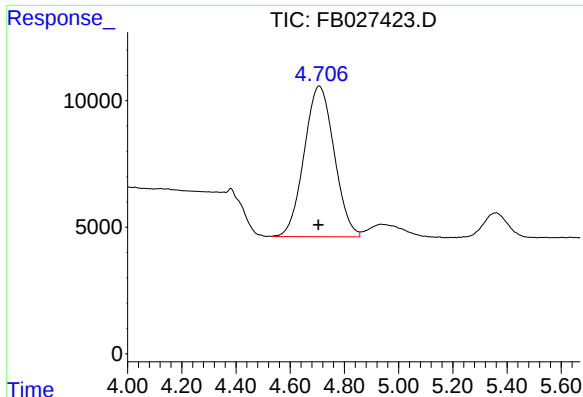

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.003 min
Response: 457981
Conc: 27.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S1

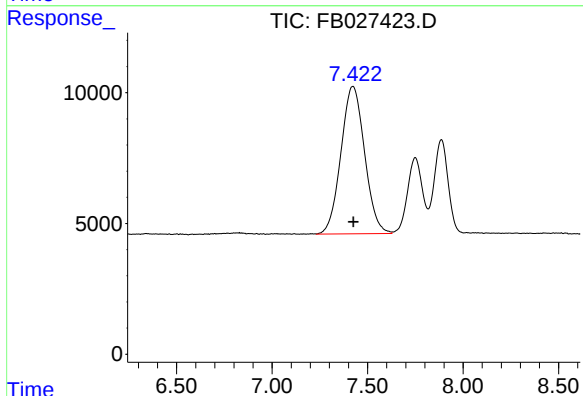


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.002 min
Response: 485937
Conc: 27.68 ng/ml

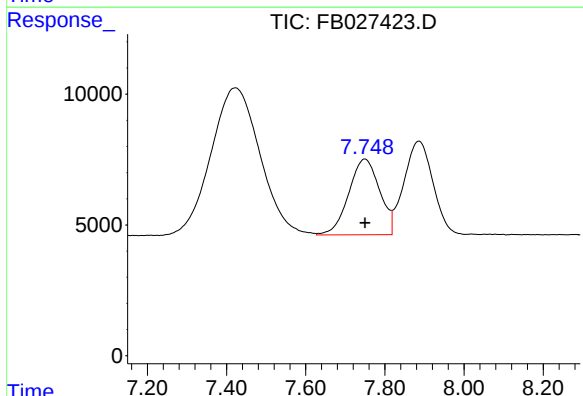


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 157672
Conc: 9.00 ng/ml

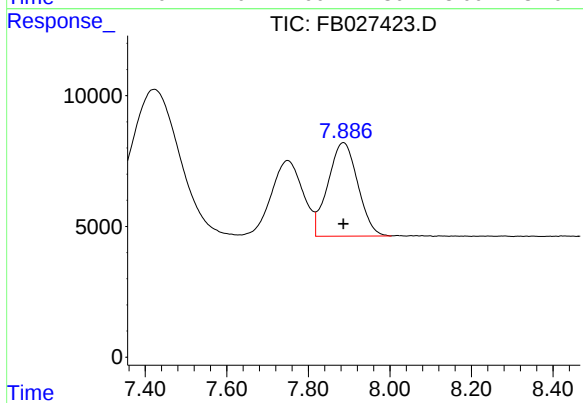

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 181596
Conc: 8.91 ng/ml

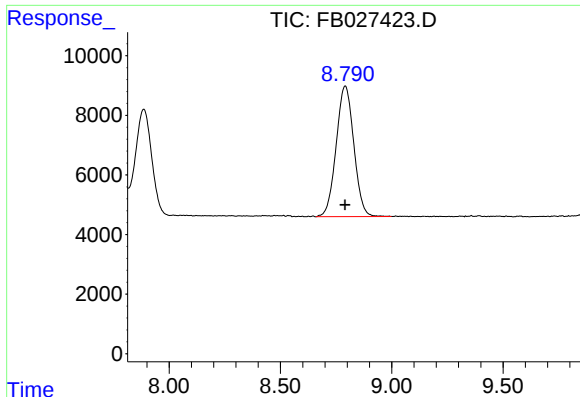

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 241645
Conc: 21.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S1

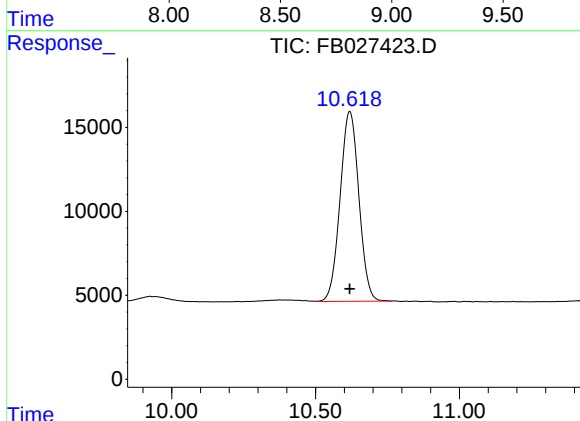


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 514695
Conc: 26.58 ng/ml

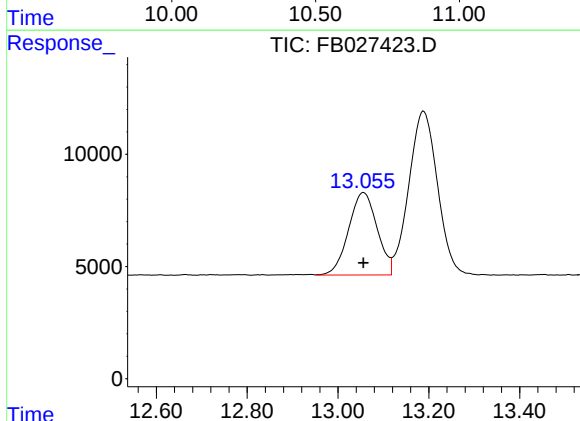


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 160562
Conc: 8.87 ng/ml

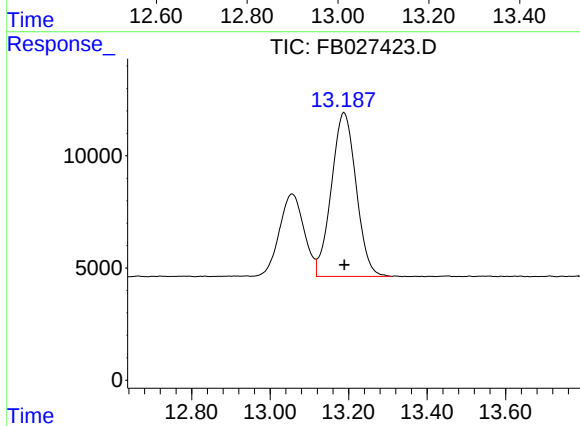

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 320067
Conc: 17.95 ng/ml

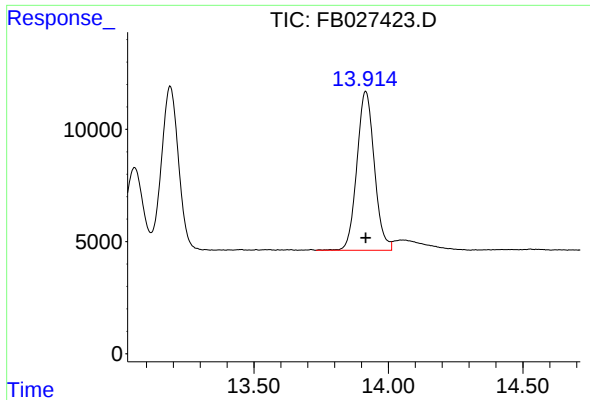

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 319571
Conc: 18.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S1

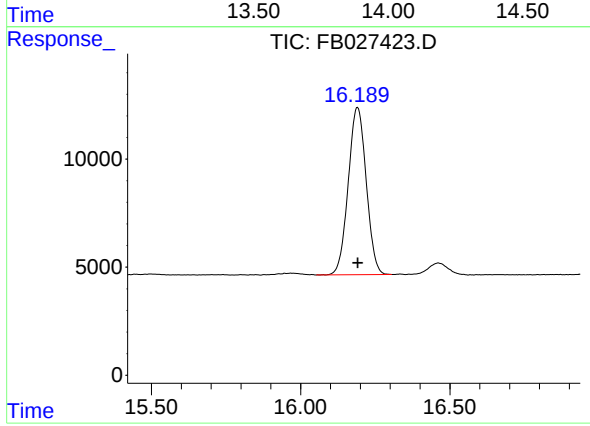

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 324543
Conc: 18.89 ng/ml