

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027429.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 15:48
 Operator : AJ/MA
 Sample : N3334-23MS
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-14A-1A-5-GRMS

Integration File: Calibration.e
 Quant Time: Jun 15 03:13:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.867	4003996	356.968 ng/mlm
Target Compounds			
1) t 2-Methylpentane	4.712	203972	12.107 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	902491	51.400 ng/ml
3) t n-Heptane	7.799	1905626	108.776 ng/ml
4) t Benzene	7.799	1495058	73.314 ng/mlm
6) t Toluene	10.798	2701769	139.539 ng/mlm
7) t Ethylbenzene	13.025	12230362	675.359 ng/ml
8) t m-Xylene	13.023	10460727	586.821 ng/mlm
9) t O-Xylene	13.927	1614692	92.927 ng/mlm
10) t 1,2,4-Trimethylbenzene	16.198	5447948	317.141 ng/mlm

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027429.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 15:48
Operator : AJ/MA
Sample : N3334-23MS
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-14A-1A-5-GRMS

Integration File: Calibration.e
Quant Time: Jun 15 03:13:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

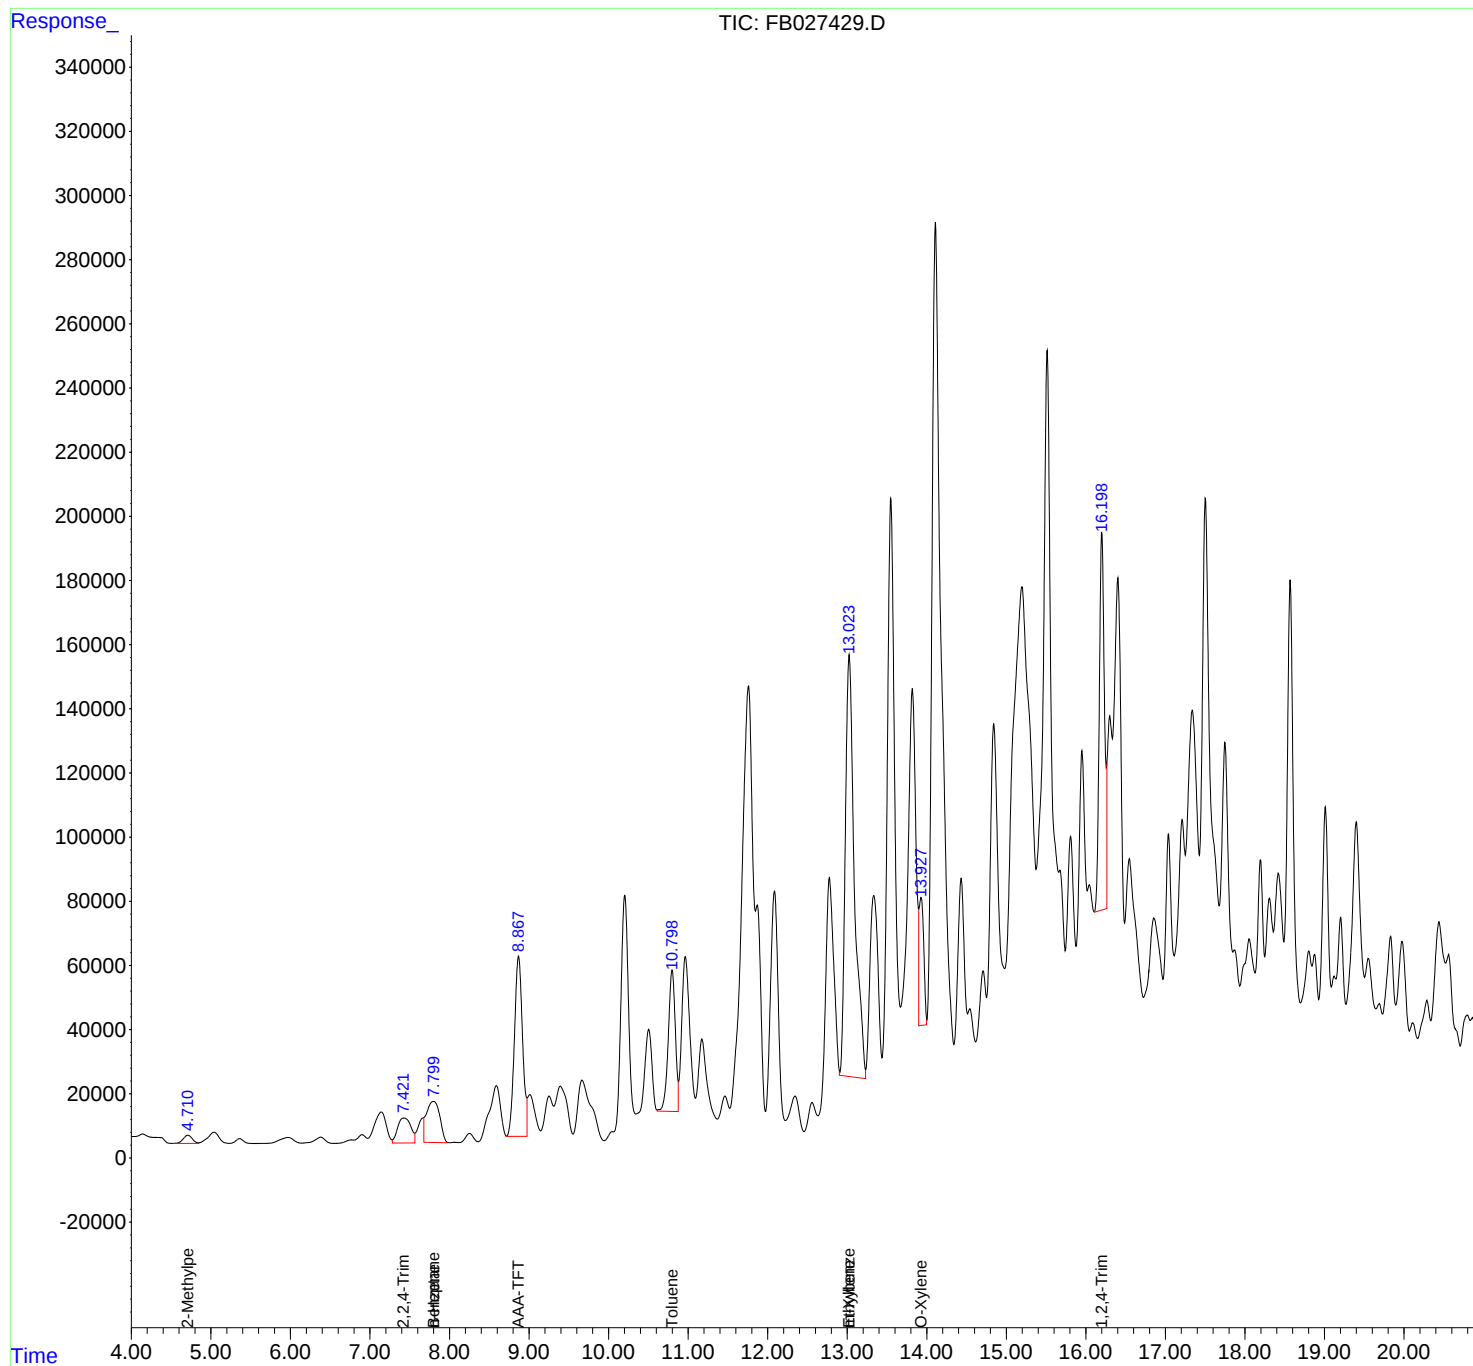


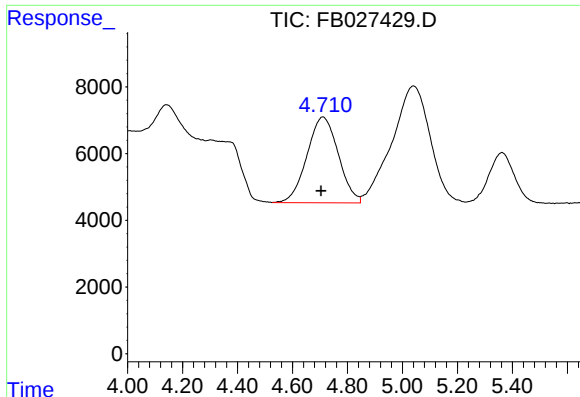

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.008 min
Response: 203972
Conc: 12.11 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14A-1A-5-GRMS

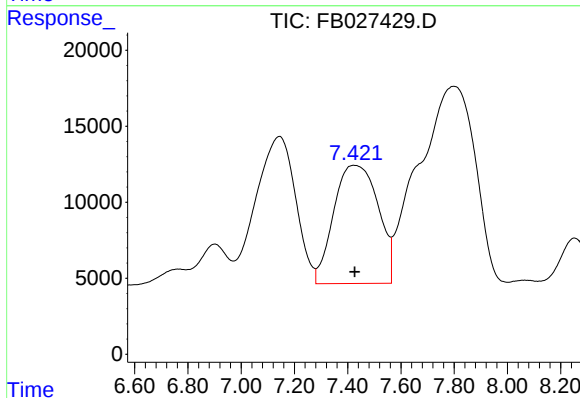


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.003 min
Response: 902491
Conc: 51.40 ng/ml

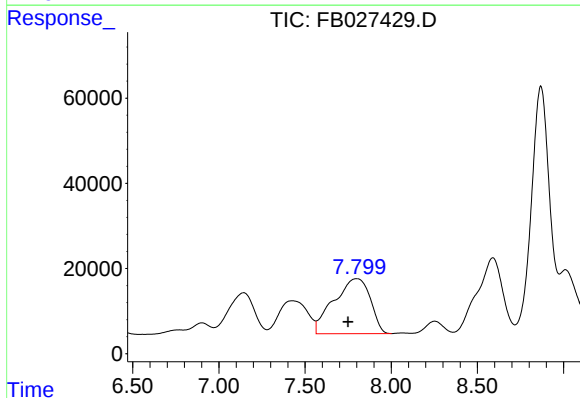


#3 n-Heptane

R.T.: 7.799 min
Delta R.T.: 0.050 min
Response: 1905626
Conc: 108.78 ng/ml

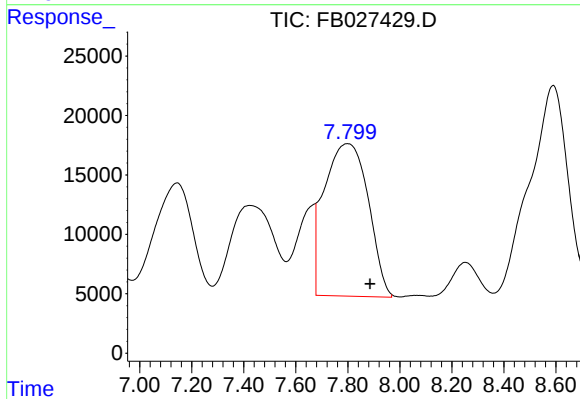

#4 Benzene


R.T.: 7.799 min
Delta R.T.: -0.087 min
Response: 1495058
Conc: 73.31 ng/ml m

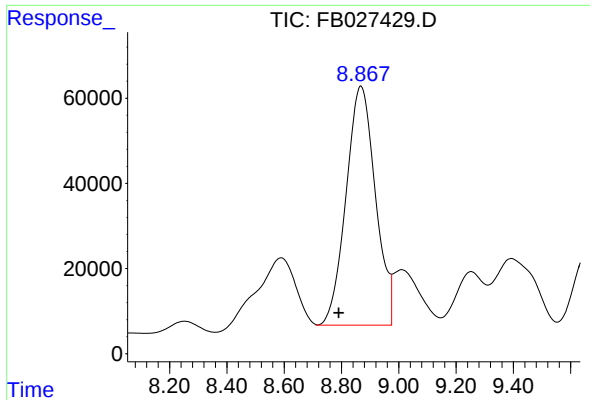

#5 AAA-TFT


R.T.: 8.867 min
Delta R.T.: 0.076 min
Response: 4003996
Conc: 356.97 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14A-1A-5-GRMS

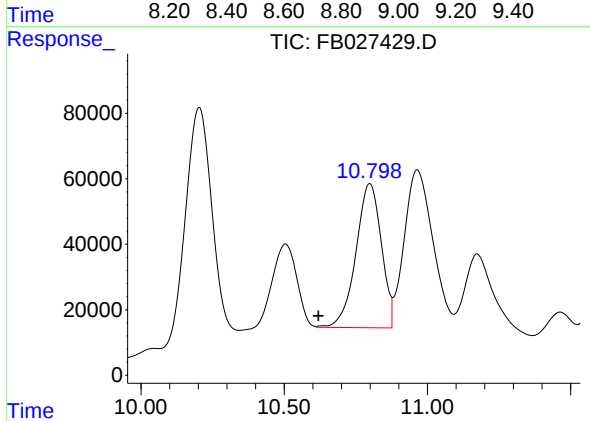


#6 Toluene

R.T.: 10.798 min
Delta R.T.: 0.178 min
Response: 2701769
Conc: 139.54 ng/ml m

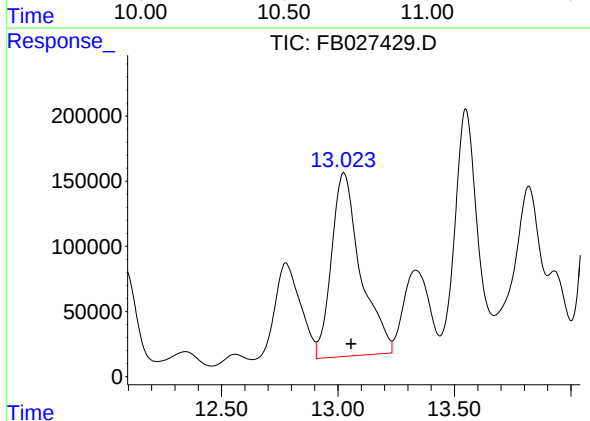


#7 Ethylbenzene

R.T.: 13.025 min
Delta R.T.: -0.031 min
Response: 12230362
Conc: 675.36 ng/ml

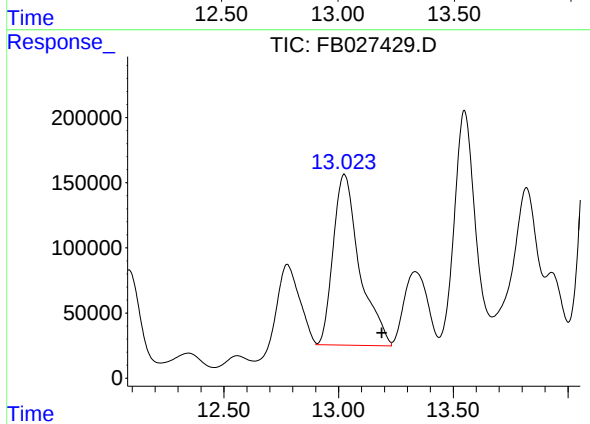

#8 m-Xylene


R.T.: 13.023 min
Delta R.T.: -0.166 min
Response: 10460727
Conc: 586.82 ng/ml m

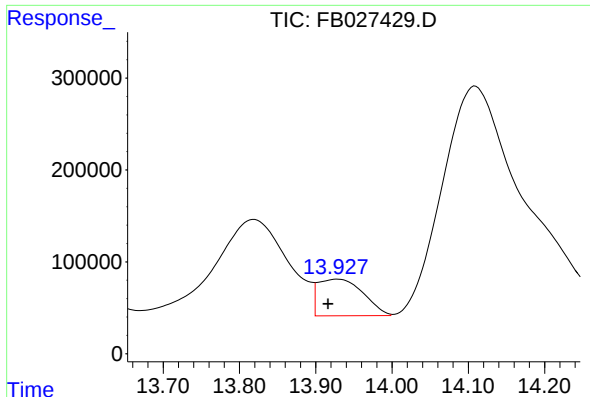

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.011 min
Response: 1614692
Conc: 92.93 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14A-1A-5-GRMS

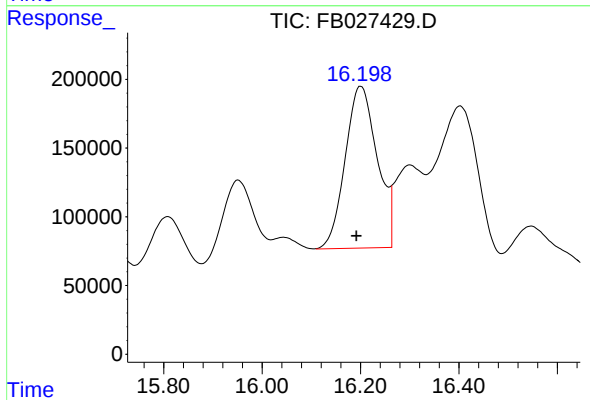

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.007 min
Response: 5447948
Conc: 317.14 ng/ml m