

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027432.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 17:39
 Operator : AJ/MA
 Sample : BSF0614S2
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0614S2

Integration File: SAMPLE.e
 Quant Time: Jun 15 03:14:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	236900	21.120 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	500228	29.692 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	525018	29.901 ng/ml
3) t n-Heptane	7.753	171560	9.793 ng/ml
4) t Benzene	7.890	200262	9.820 ng/ml
6) t Toluene	10.623	574159	29.654 ng/ml
7) t Ethylbenzene	13.060	178206	9.841 ng/ml
8) t m-Xylene	13.193	353222	19.815 ng/ml
9) t O-Xylene	13.920	343214	19.752 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	342929	19.963 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027432.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 17:39
Operator : AJ/MA
Sample : BSF0614S2
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0614S2

Integration File: SAMPLE.e
Quant Time: Jun 15 03:14:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

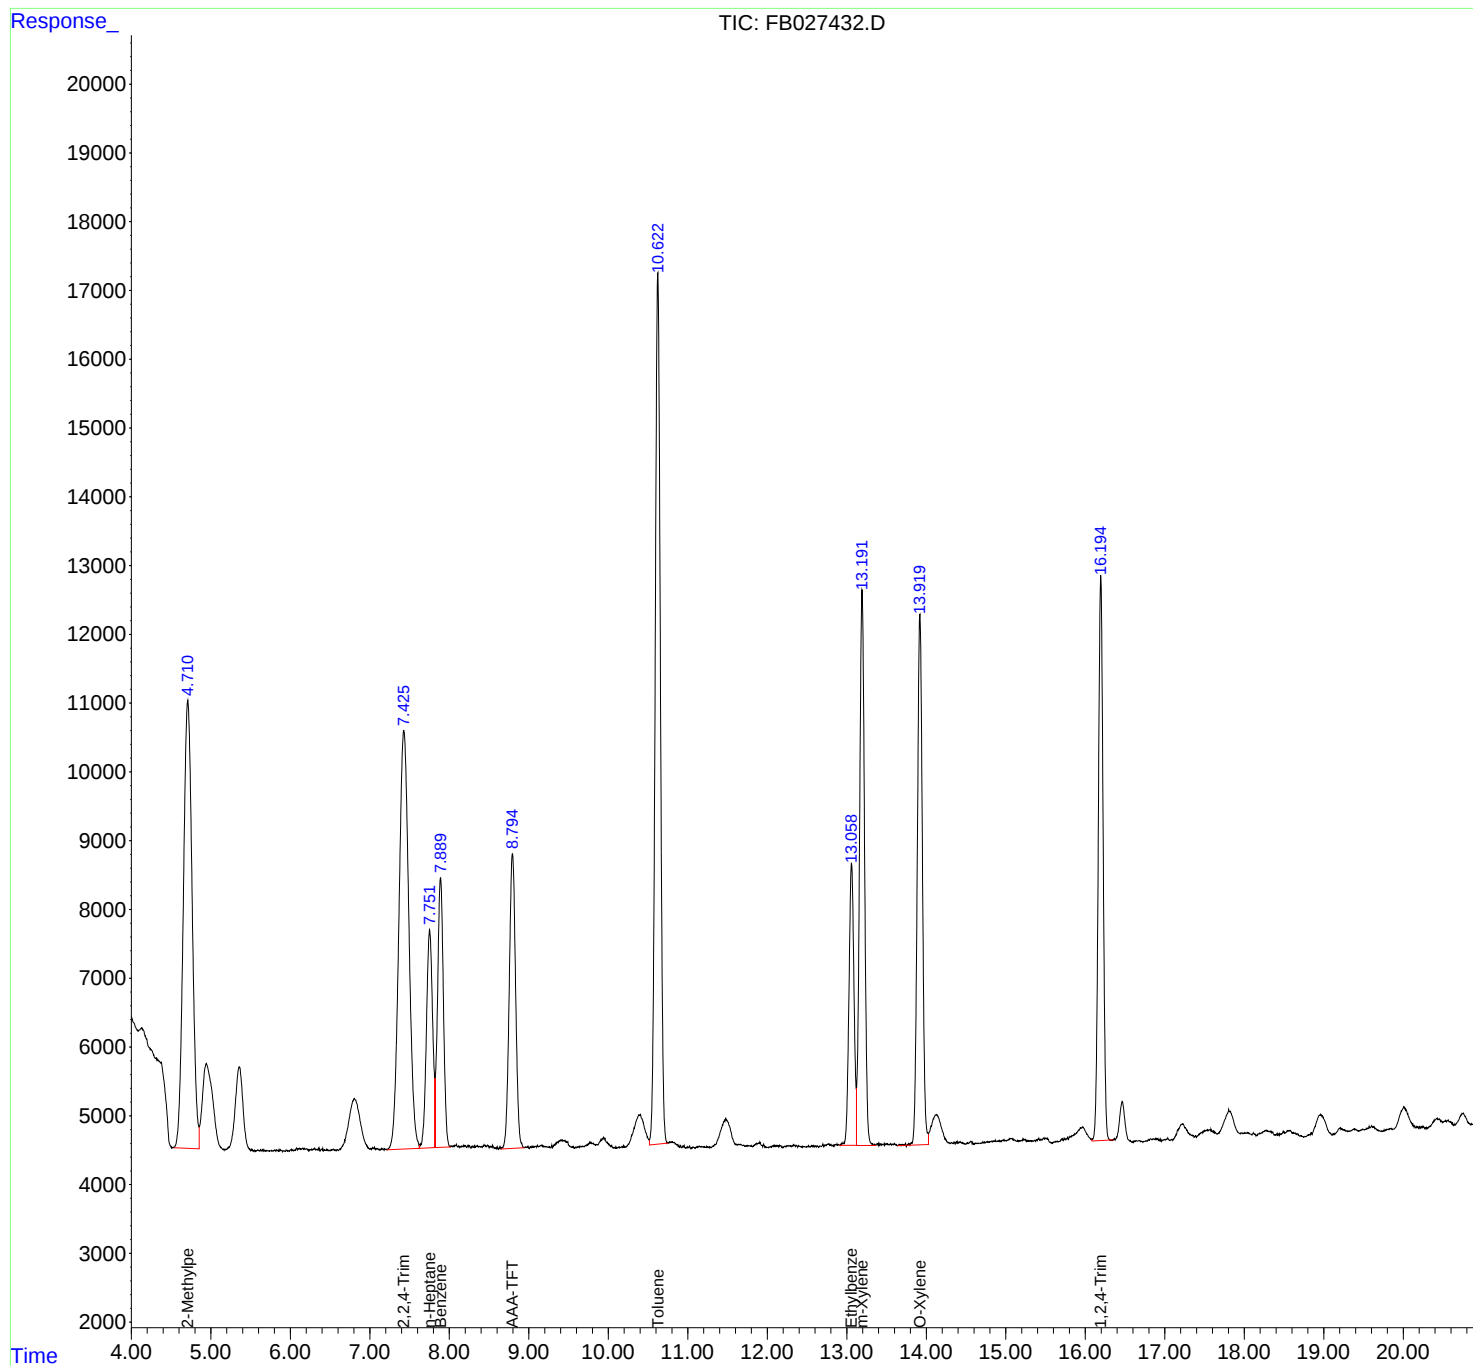


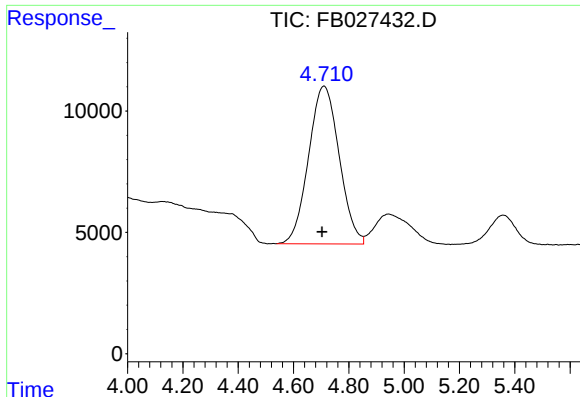

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.007 min
Response: 500228
Conc: 29.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S2

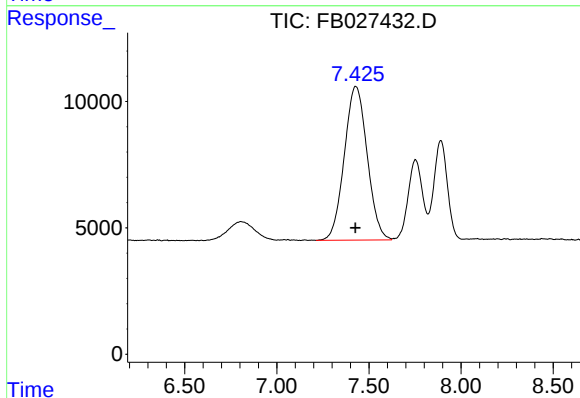


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 525018
Conc: 29.90 ng/ml

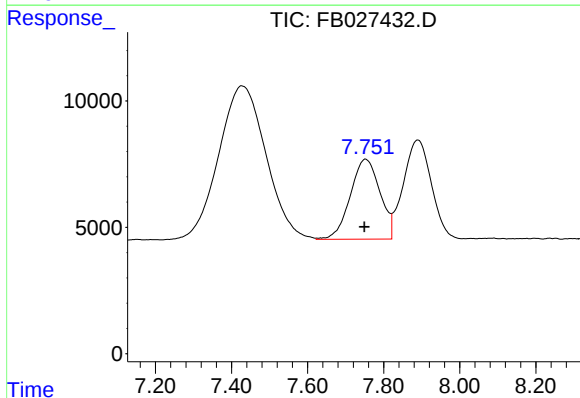


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 171560
Conc: 9.79 ng/ml

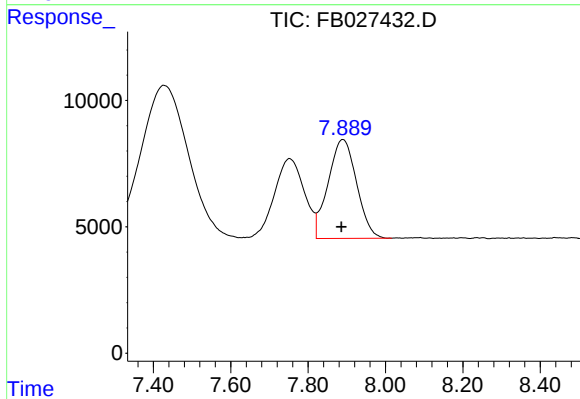

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.005 min
Response: 200262
Conc: 9.82 ng/ml

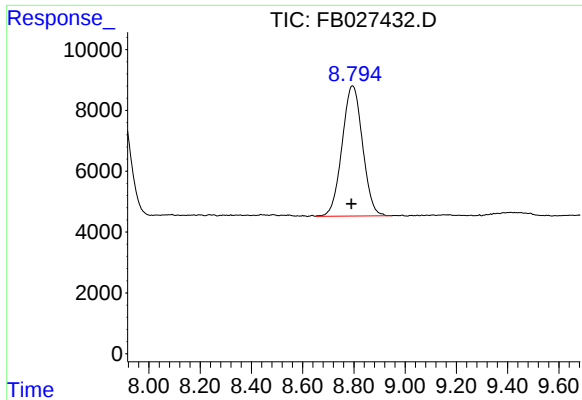

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 236900
Conc: 21.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S2

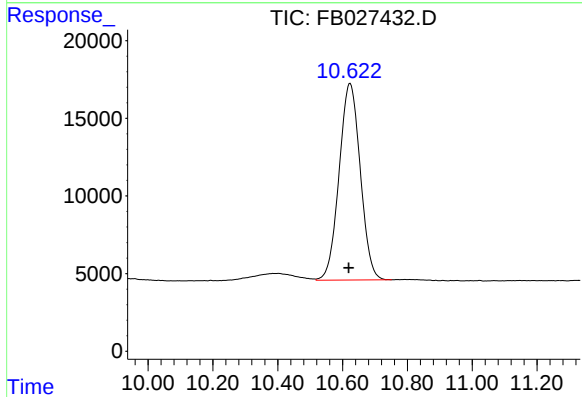


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 574159
Conc: 29.65 ng/ml

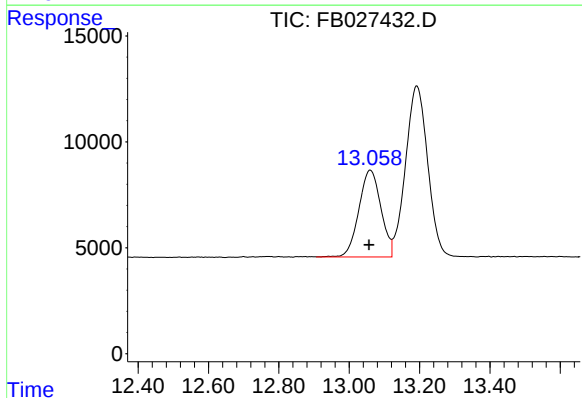


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.004 min
Response: 178206
Conc: 9.84 ng/ml

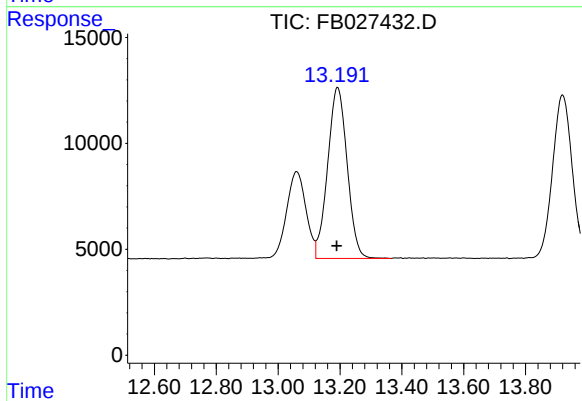

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.004 min
Response: 353222
Conc: 19.81 ng/ml

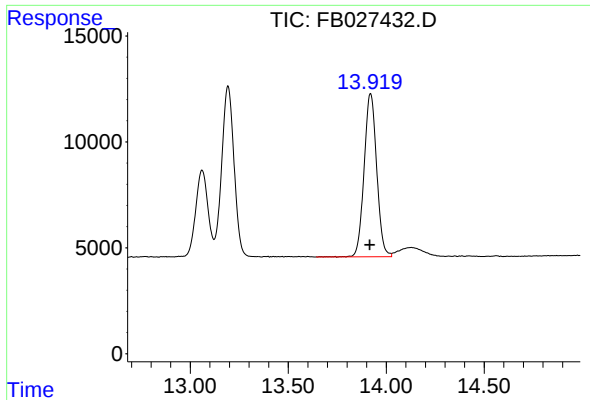

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 343214
Conc: 19.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S2

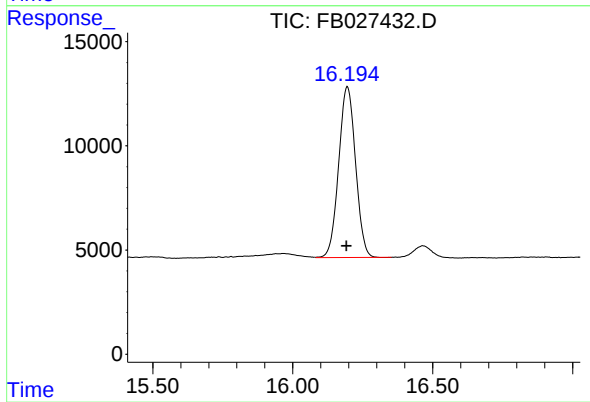

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.004 min
Response: 342929
Conc: 19.96 ng/ml