

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
 Data File : FB027440.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2022 23:11
 Operator : AJ/MA
 Sample : N3334-23MSD
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-14A-1A-5-GRMSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/15/2022
 Supervised By :Ankita Jodhani 06/15/2022

Integration File: SAMPLE.e
 Quant Time: Jun 15 03:15:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.858	1131353	100.863 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	60498	3.591 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	197359	11.240 ng/ml
3) t n-Heptane	7.784	462475	26.399 ng/ml
4) t Benzene	7.774	378647	18.568 ng/mlm
6) t Toluene	10.629	19556	1.010 ng/mlm
7) t Ethylbenzene	13.022	4346565	240.017 ng/ml
8) t m-Xylene	13.020	3721982	208.794 ng/mlm
9) t O-Xylene	13.924	543946	31.304 ng/mlm
10) t 1,2,4-Trimethylbenzene	16.196	2031613	118.266 ng/mlm

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061422\
Data File : FB027440.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2022 23:11
Operator : AJ/MA
Sample : N3334-23MSD
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
WC-14A-1A-5-GRMSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2022
Supervised By :Ankita Jodhani 06/15/2022

Integration File: SAMPLE.e
Quant Time: Jun 15 03:15:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

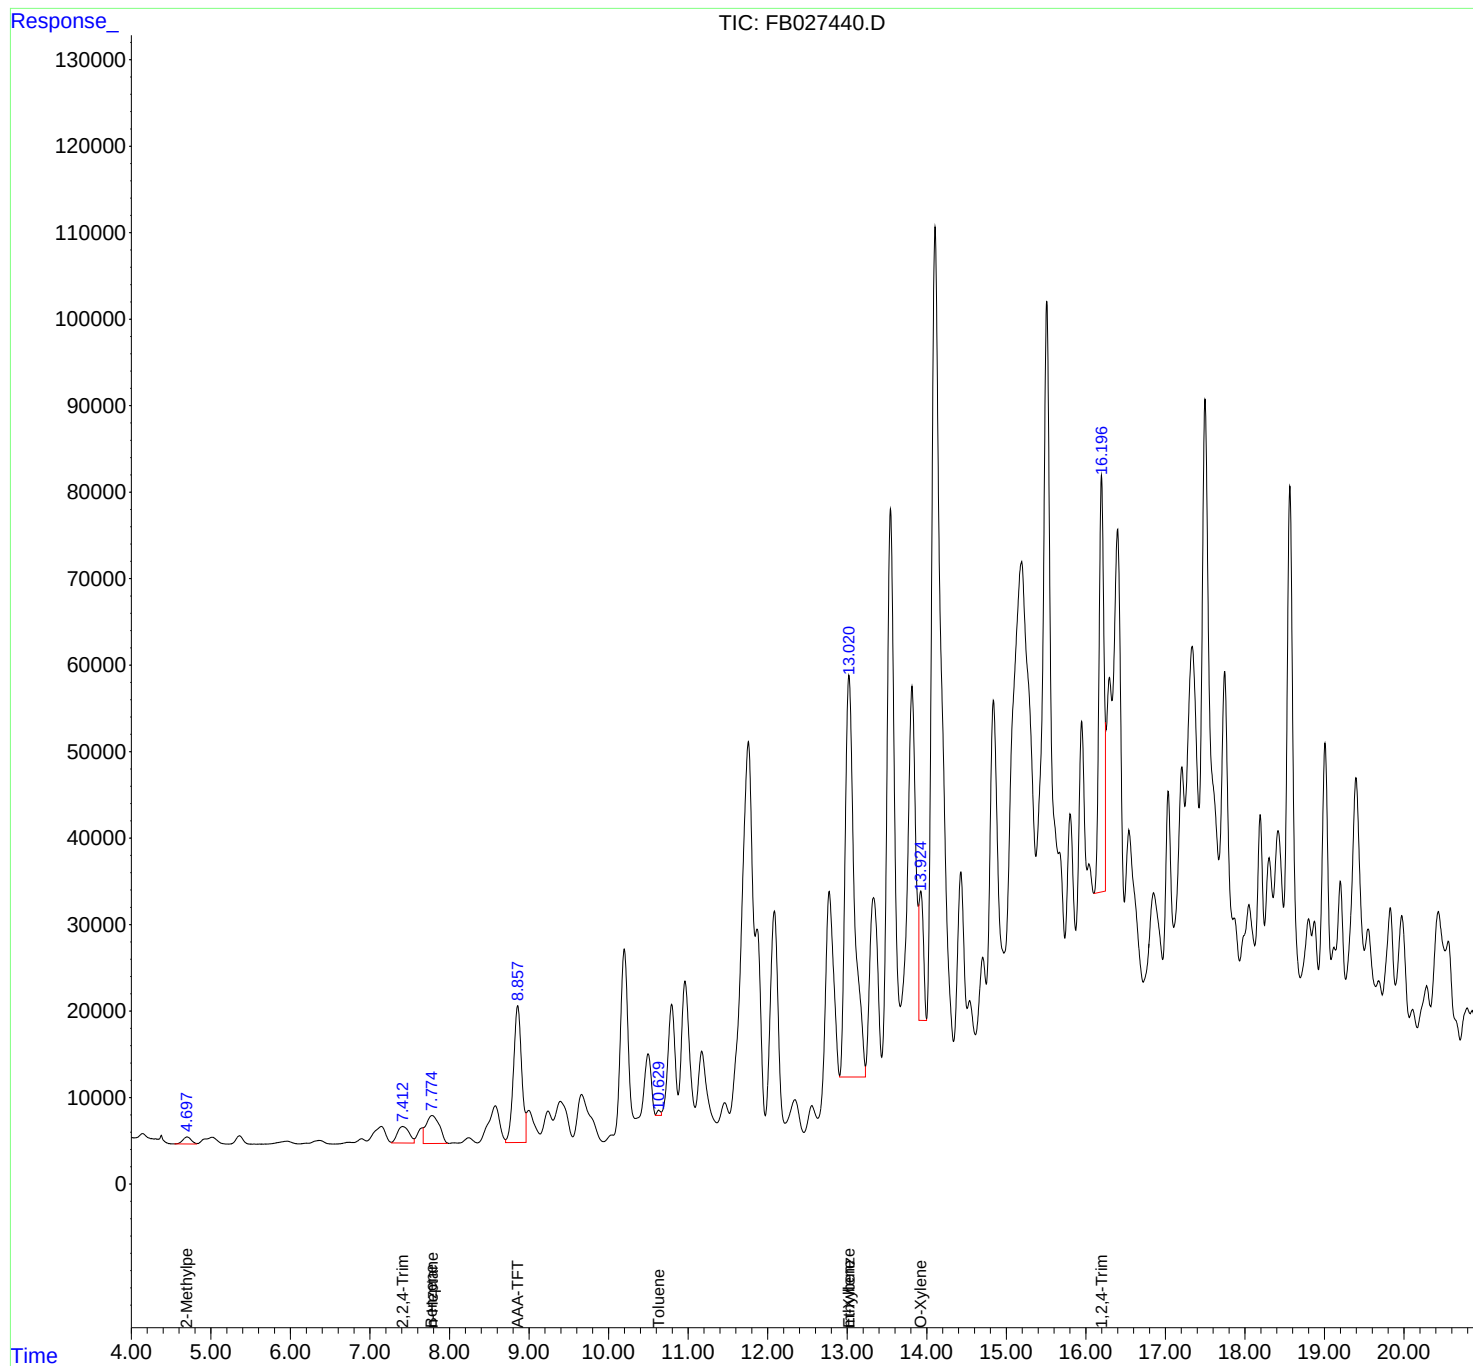

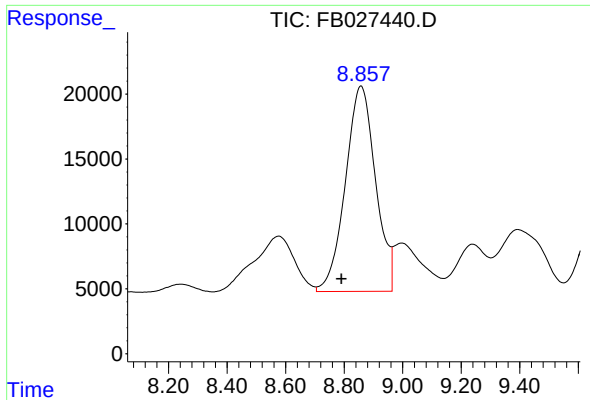


#5 AAA-TFT

R.T.: 8.858 min
Delta R.T.: 0.068 min
Response: 1131353
Conc: 100.86 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14A-1A-5-GRMSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2022
Supervised By :Ankita Jodhani 06/15/2022

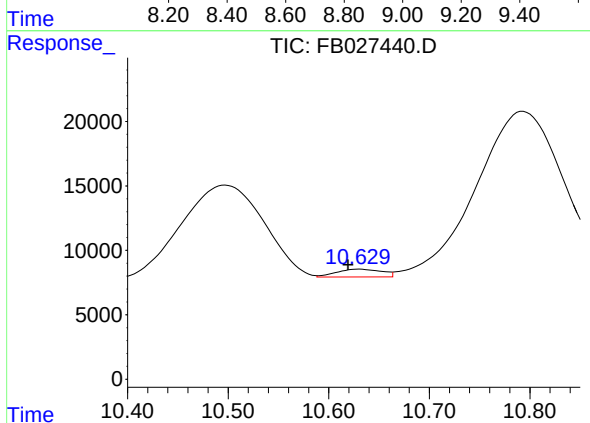


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.010 min
Response: 19556
Conc: 1.01 ng/ml m

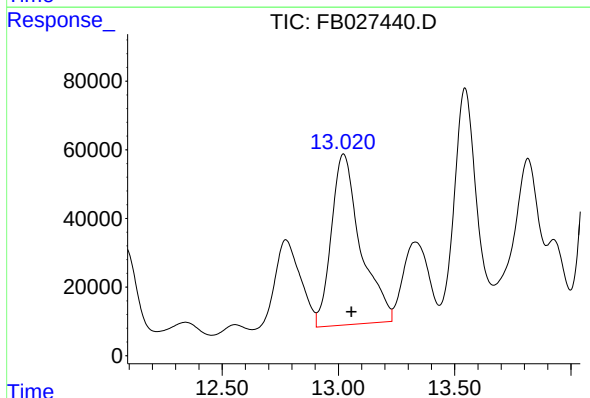


#7 Ethylbenzene

R.T.: 13.022 min
Delta R.T.: -0.034 min
Response: 4346565
Conc: 240.02 ng/ml

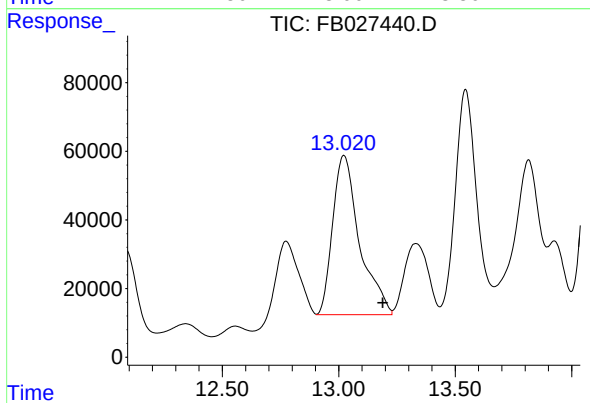

#8 m-Xylene

R.T.: 13.020 min
Delta R.T.: -0.169 min
Response: 3721982
Conc: 208.79 ng/ml m

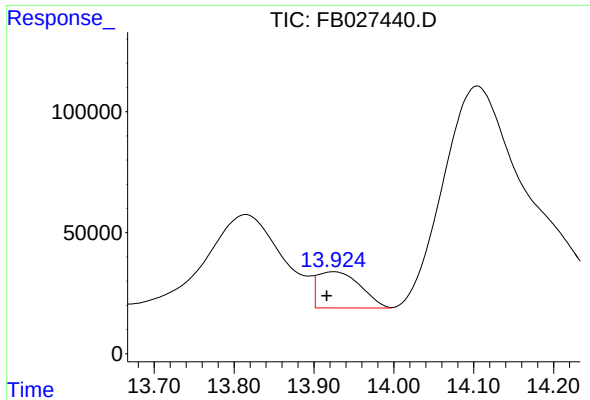


#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.008 min
Response: 543946
Conc: 31.30 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14A-1A-5-GRMSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2022
Supervised By :Ankita Jodhani 06/15/2022

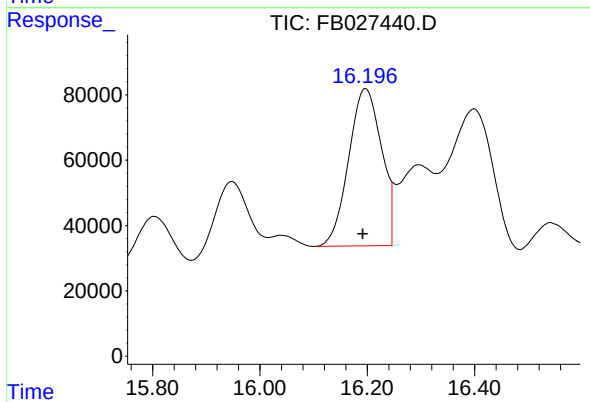

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 2031613
Conc: 118.27 ng/ml m