

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061520\
 Data File : FB024455.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jun 2020 10:57
 Operator : DD/AJ
 Sample : BSF0615S1
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 16 00:50:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	460270	19.024 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	923062	28.879 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	987327	29.451 ng/ml
3) t n-Heptane	7.753	326756	9.662 ng/ml
4) t Benzene	7.888	381712	9.442 ng/ml
6) t Toluene	10.624	1109202	28.225 ng/ml
7) t Ethylbenzene	13.063	348957	9.944 ng/ml
8) t m-Xylene	13.197	680291	19.865 ng/ml
9) t O-Xylene	13.924	656501	19.582 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	549529	19.792 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061520\
Data File : FB024455.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2020 10:57
Operator : DD/AJ
Sample : BSF0615S1
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 16 00:50:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

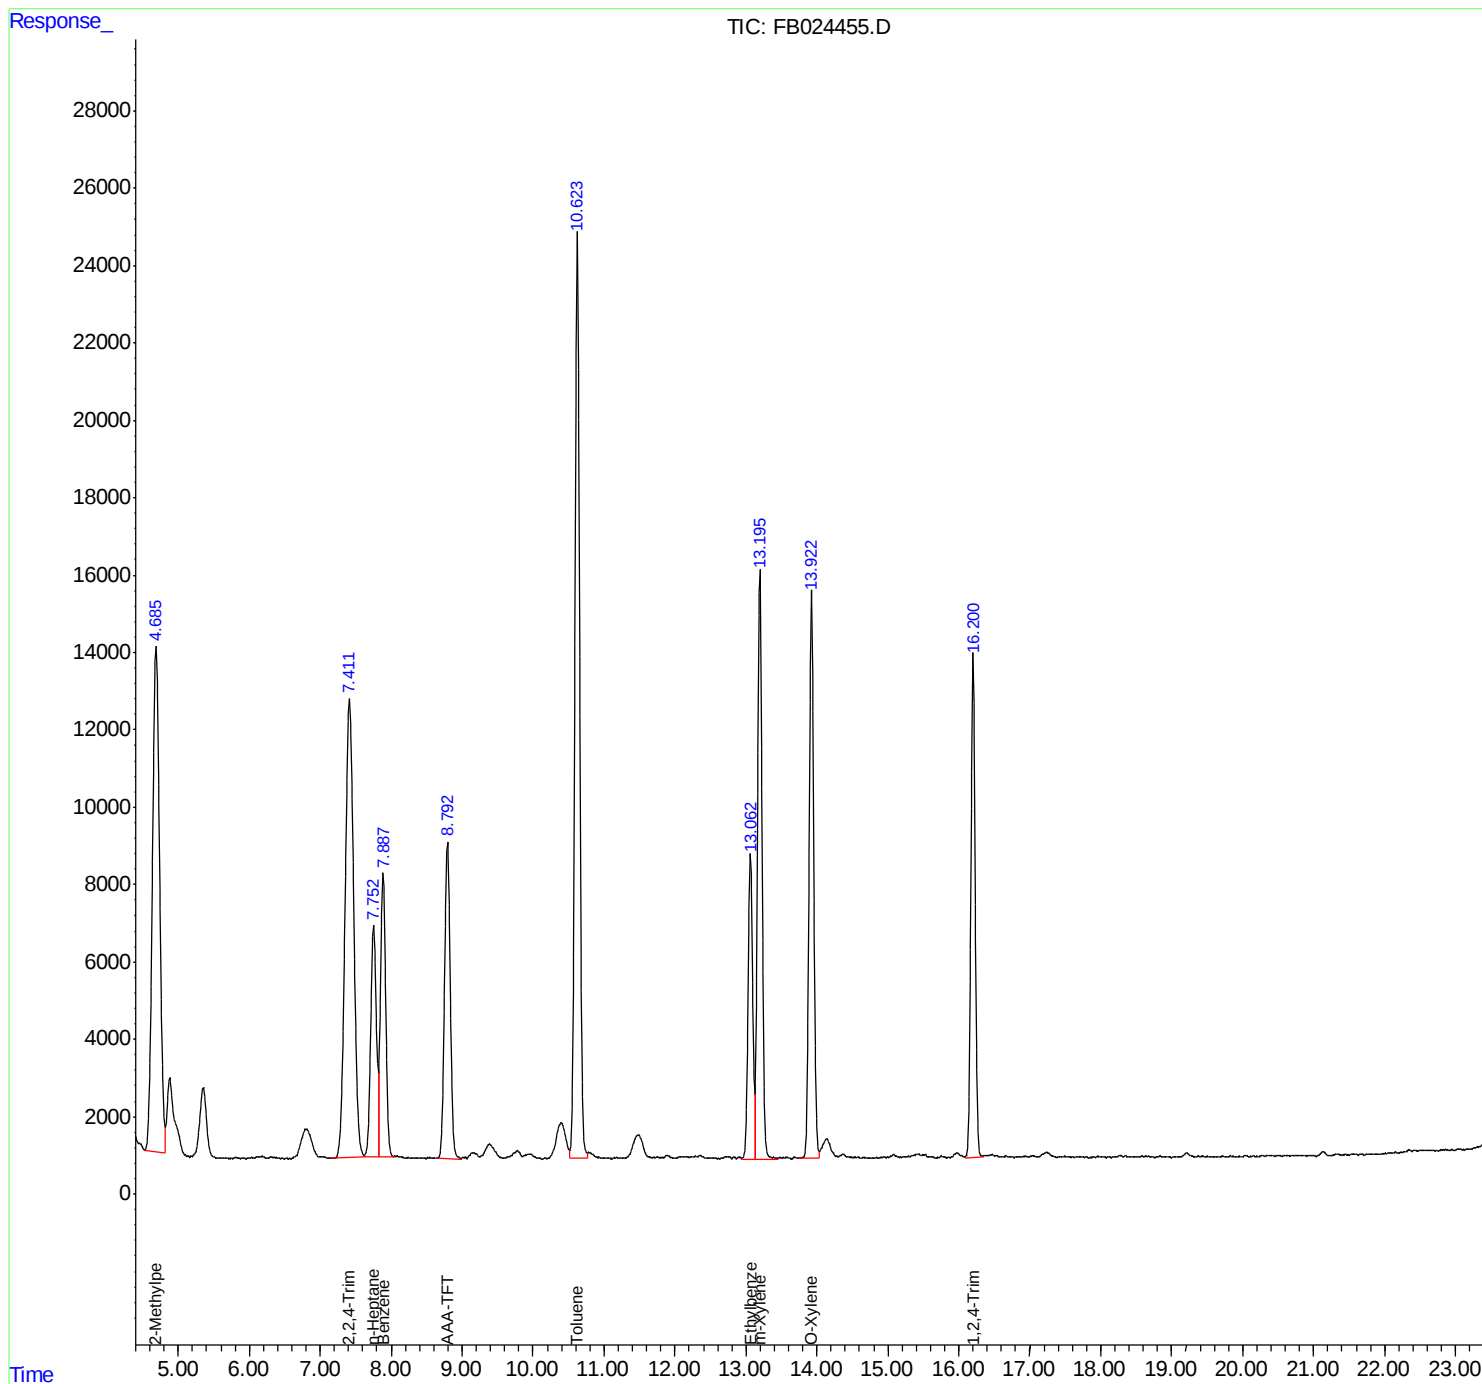

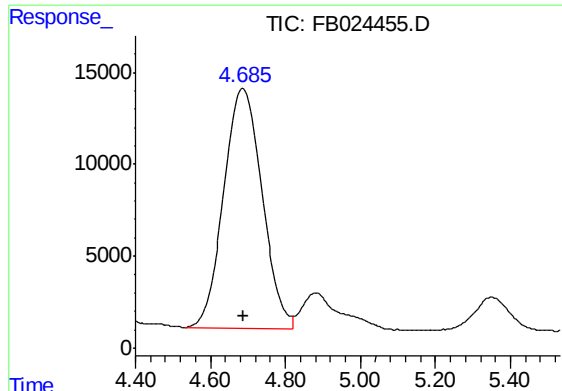


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 923062
Conc: 28.88 ng/ml

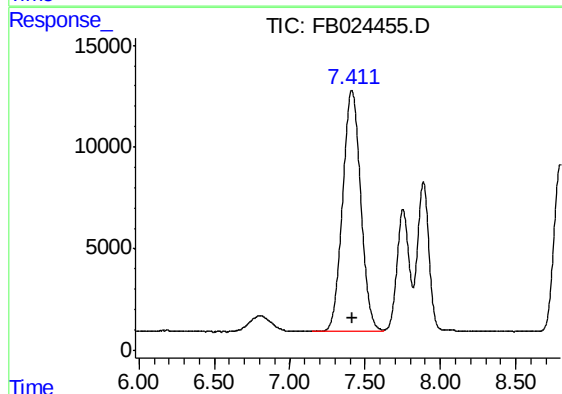


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.003 min
Response: 987327
Conc: 29.45 ng/ml

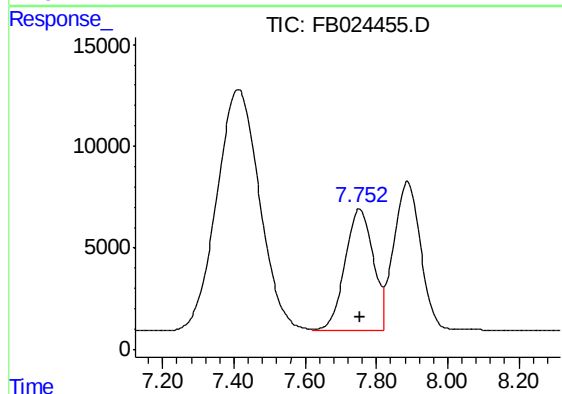


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 326756
Conc: 9.66 ng/ml

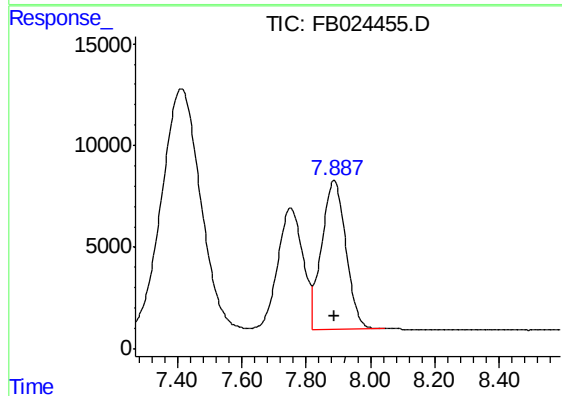


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 381712
Conc: 9.44 ng/ml

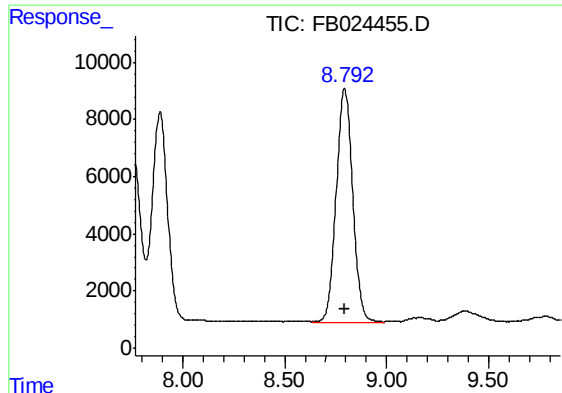


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.003 min
Response: 460270
Conc: 19.02 ng/ml

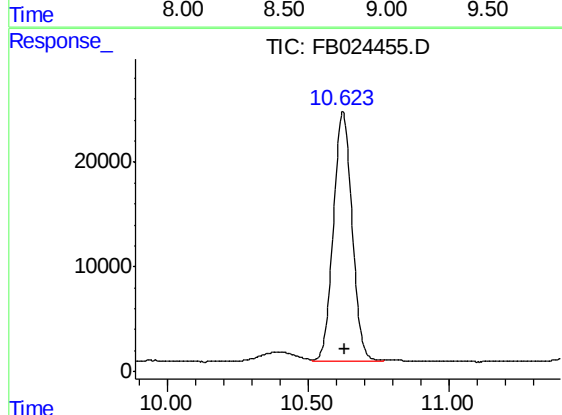


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.004 min
Response: 1109202
Conc: 28.23 ng/ml

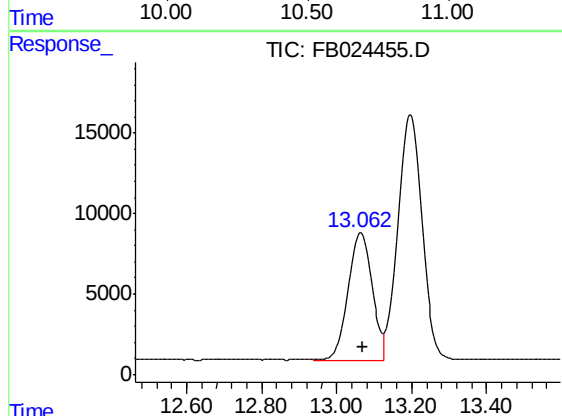


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.004 min
Response: 348957
Conc: 9.94 ng/ml

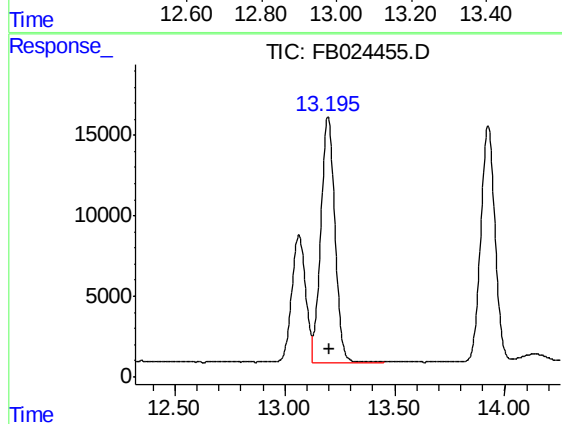


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.005 min
Response: 680291
Conc: 19.86 ng/ml

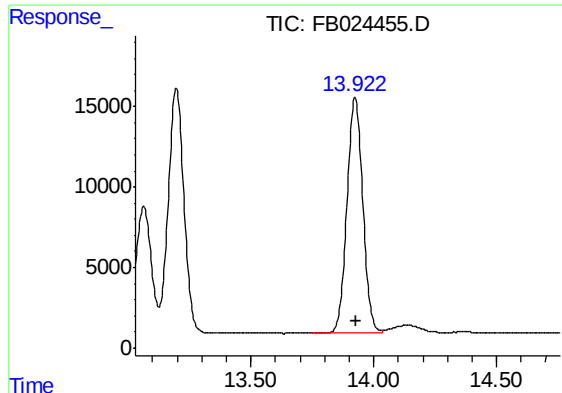

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.005 min
Response: 656501
Conc: 19.58 ng/ml

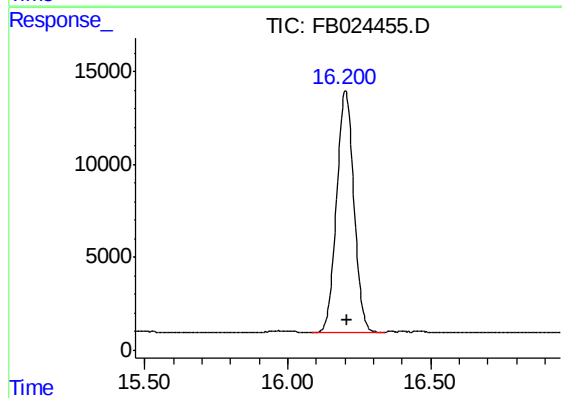

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 549529
Conc: 19.79 ng/ml