

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061520\
Data File : FB024456.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2020 11:57
Operator : DD/AJ
Sample : L2808-02
Misc : 5.04gm/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 16 00:50:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	470008	19.427 ng/ml
Target Compounds			
6) t Toluene	10.626	10023	0.255 ng/ml
7) t Ethylbenzene	13.022	239800	6.834 ng/ml
9) t O-Xylene	13.934	57346	1.710 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061520\
Data File : FB024456.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2020 11:57
Operator : DD/AJ
Sample : L2808-02
Misc : 5.04gm/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 16 00:50:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

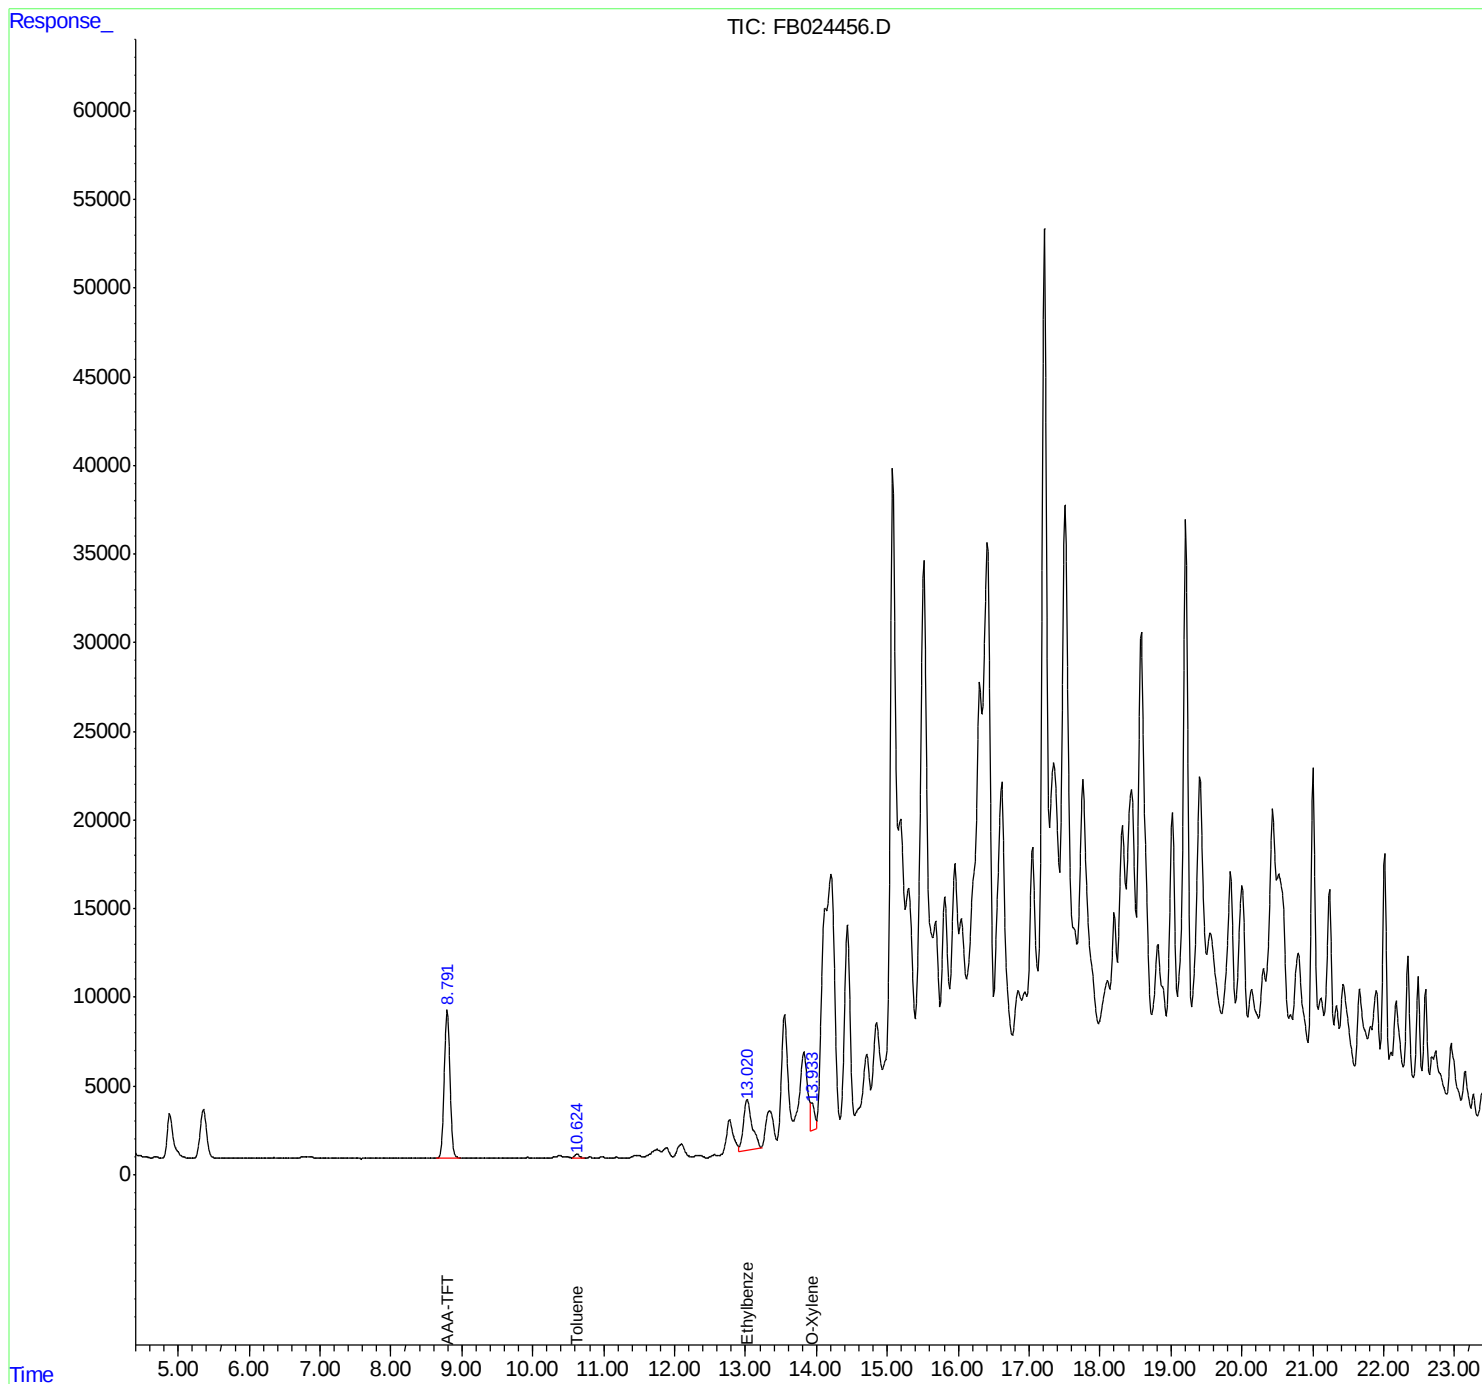

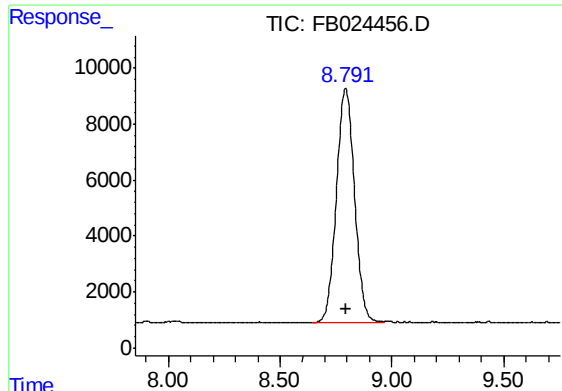


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.004 min
Response: 470008
Conc: 19.43 ng/ml

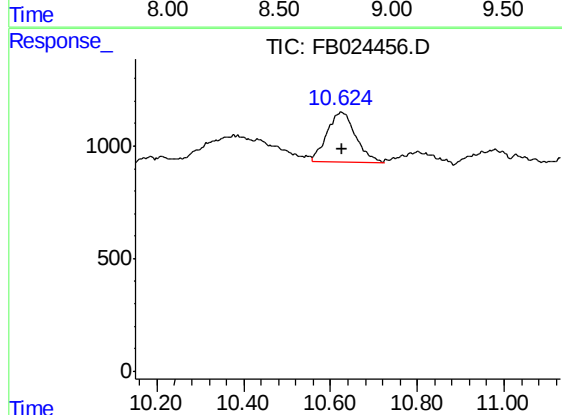


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 10023
Conc: 0.26 ng/ml

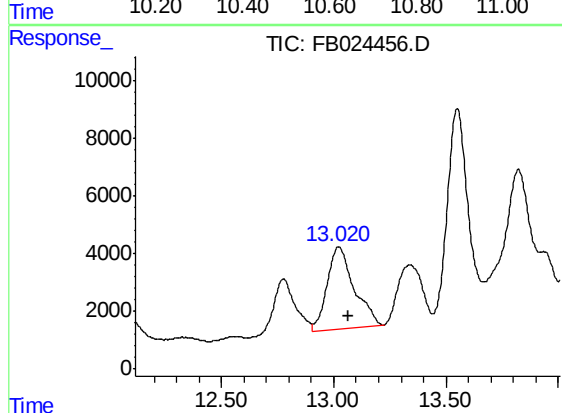

#7 Ethylbenzene

R.T.: 13.022 min
Delta R.T.: -0.046 min
Response: 239800
Conc: 6.83 ng/ml

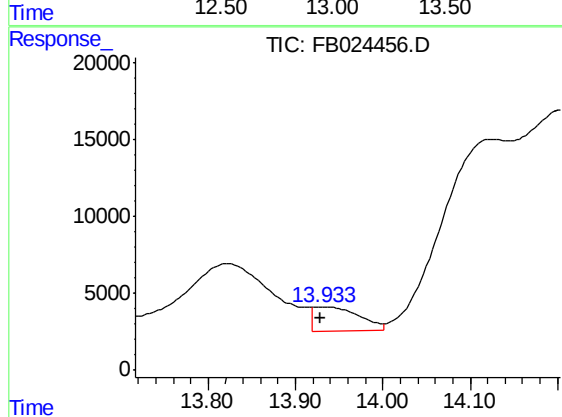

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.005 min
Response: 57346
Conc: 1.71 ng/ml