

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061520\
 Data File : FB024458.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jun 2020 12:57
 Operator : DD/AJ
 Sample : L2997-01MS
 Misc : 5.03gm/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 16 00:51:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	514376	21.260 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	831167	26.004 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	864604	25.791 ng/ml
3) t n-Heptane	7.754	267853	7.921 ng/ml
4) t Benzene	7.888	369772	9.147 ng/ml
6) t Toluene	10.626	1037864	26.410 ng/ml
7) t Ethylbenzene	13.065	315048	8.978 ng/ml
8) t m-Xylene	13.198	613827	17.924 ng/ml
9) t O-Xylene	13.925	602112	17.959 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	489627	17.634 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061520\
Data File : FB024458.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2020 12:57
Operator : DD/AJ
Sample : L2997-01MS
Misc : 5.03gm/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 16 00:51:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

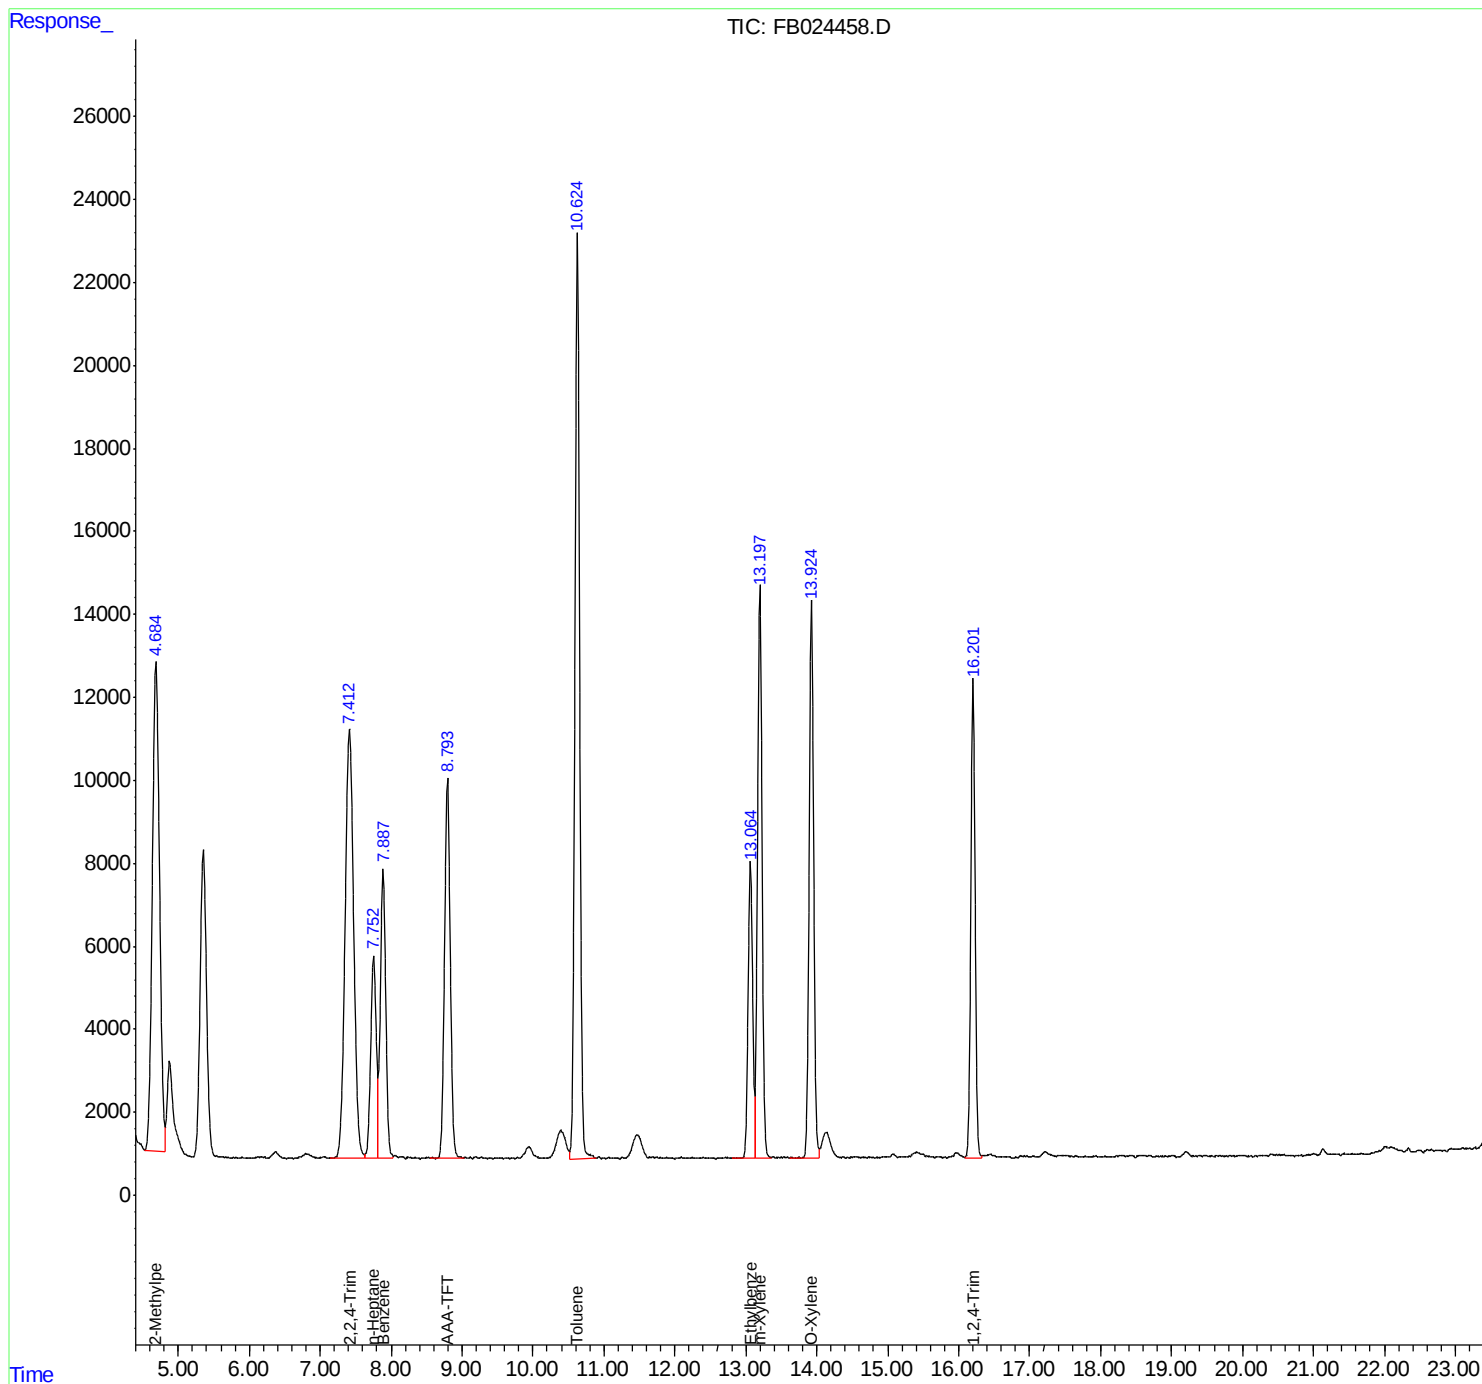

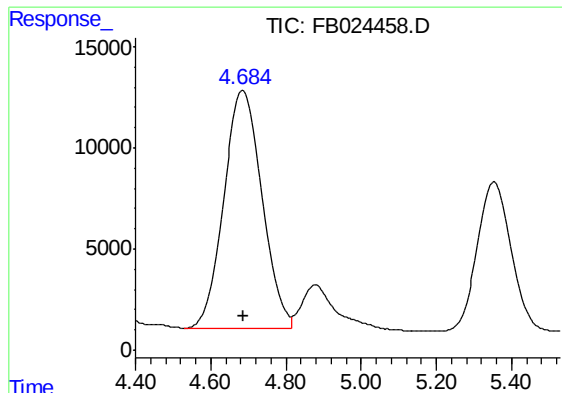


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.001 min
Response: 831167
Conc: 26.00 ng/ml

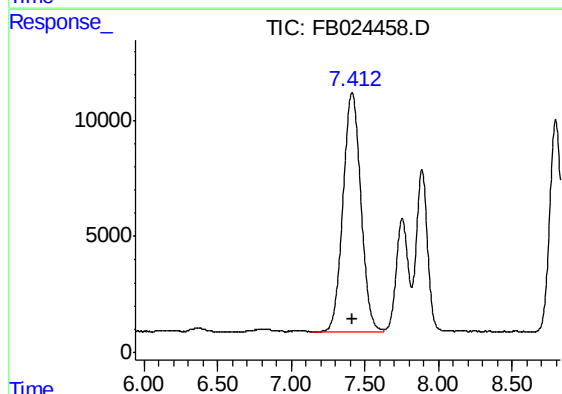


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.003 min
Response: 864604
Conc: 25.79 ng/ml

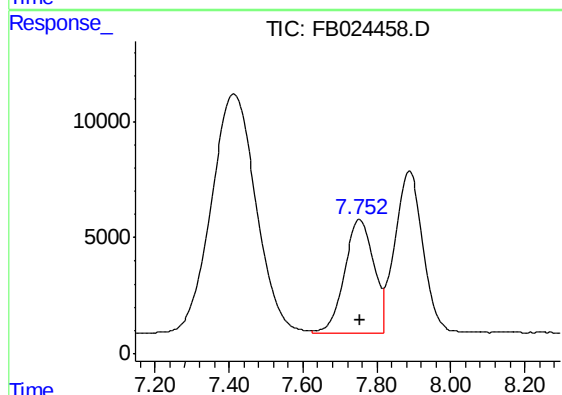


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.001 min
Response: 267853
Conc: 7.92 ng/ml

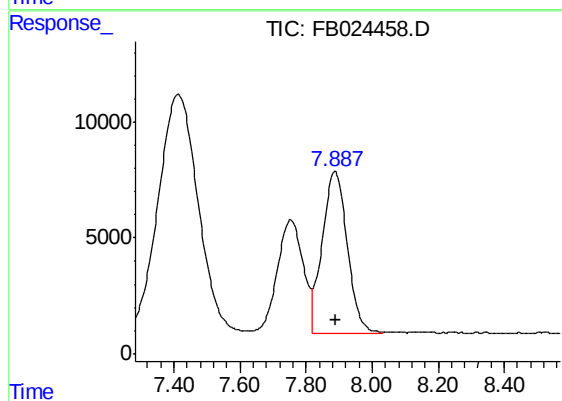


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 369772
Conc: 9.15 ng/ml

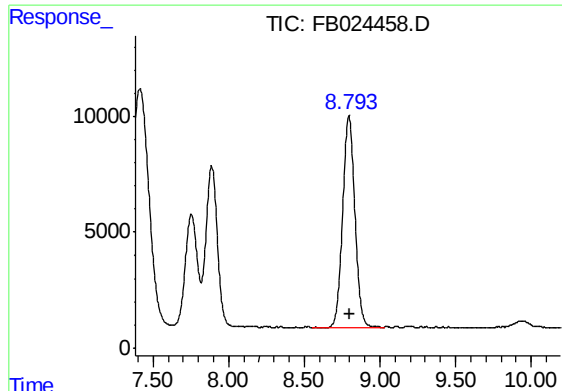


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.002 min
Response: 514376
Conc: 21.26 ng/ml

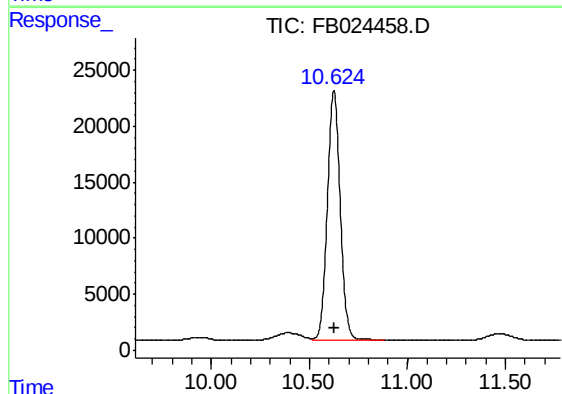


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.003 min
Response: 1037864
Conc: 26.41 ng/ml

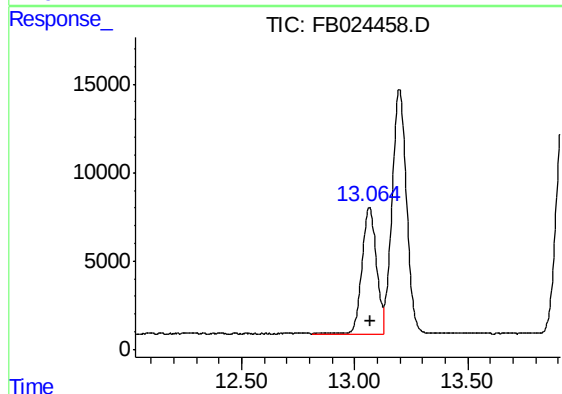


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 315048
Conc: 8.98 ng/ml

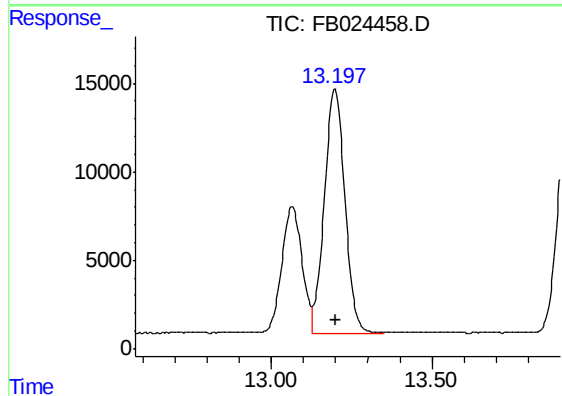


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.003 min
Response: 613827
Conc: 17.92 ng/ml

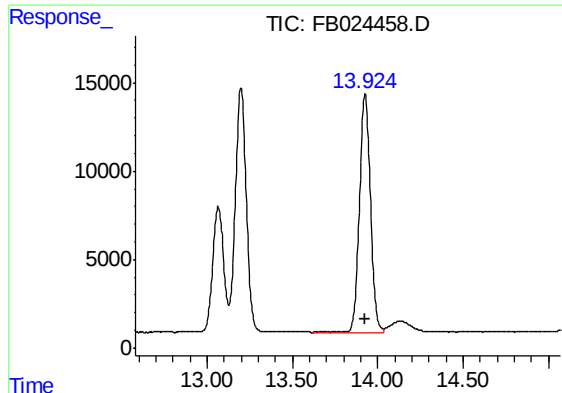

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.004 min
Response: 602112
Conc: 17.96 ng/ml

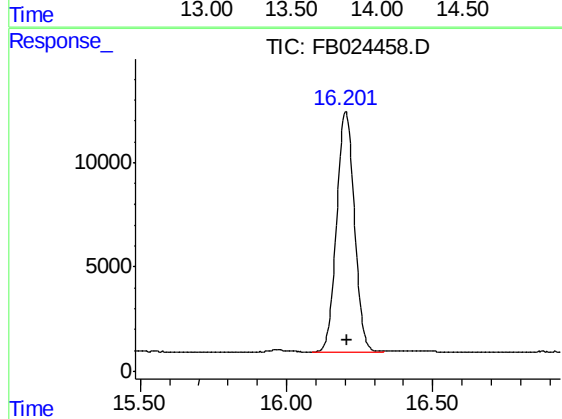

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.004 min
Response: 489627
Conc: 17.63 ng/ml