

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
Data File : FB025874.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2021 11:13
Operator : DD/AJ
Sample : VBF0615S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 16 01:20:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.221	460249	19.045 ng/ml
Target Compounds			
8) t m-Xylene	13.577	23557	0.599 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
Data File : FB025874.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2021 11:13
Operator : DD/AJ
Sample : VBF0615S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 16 01:20:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

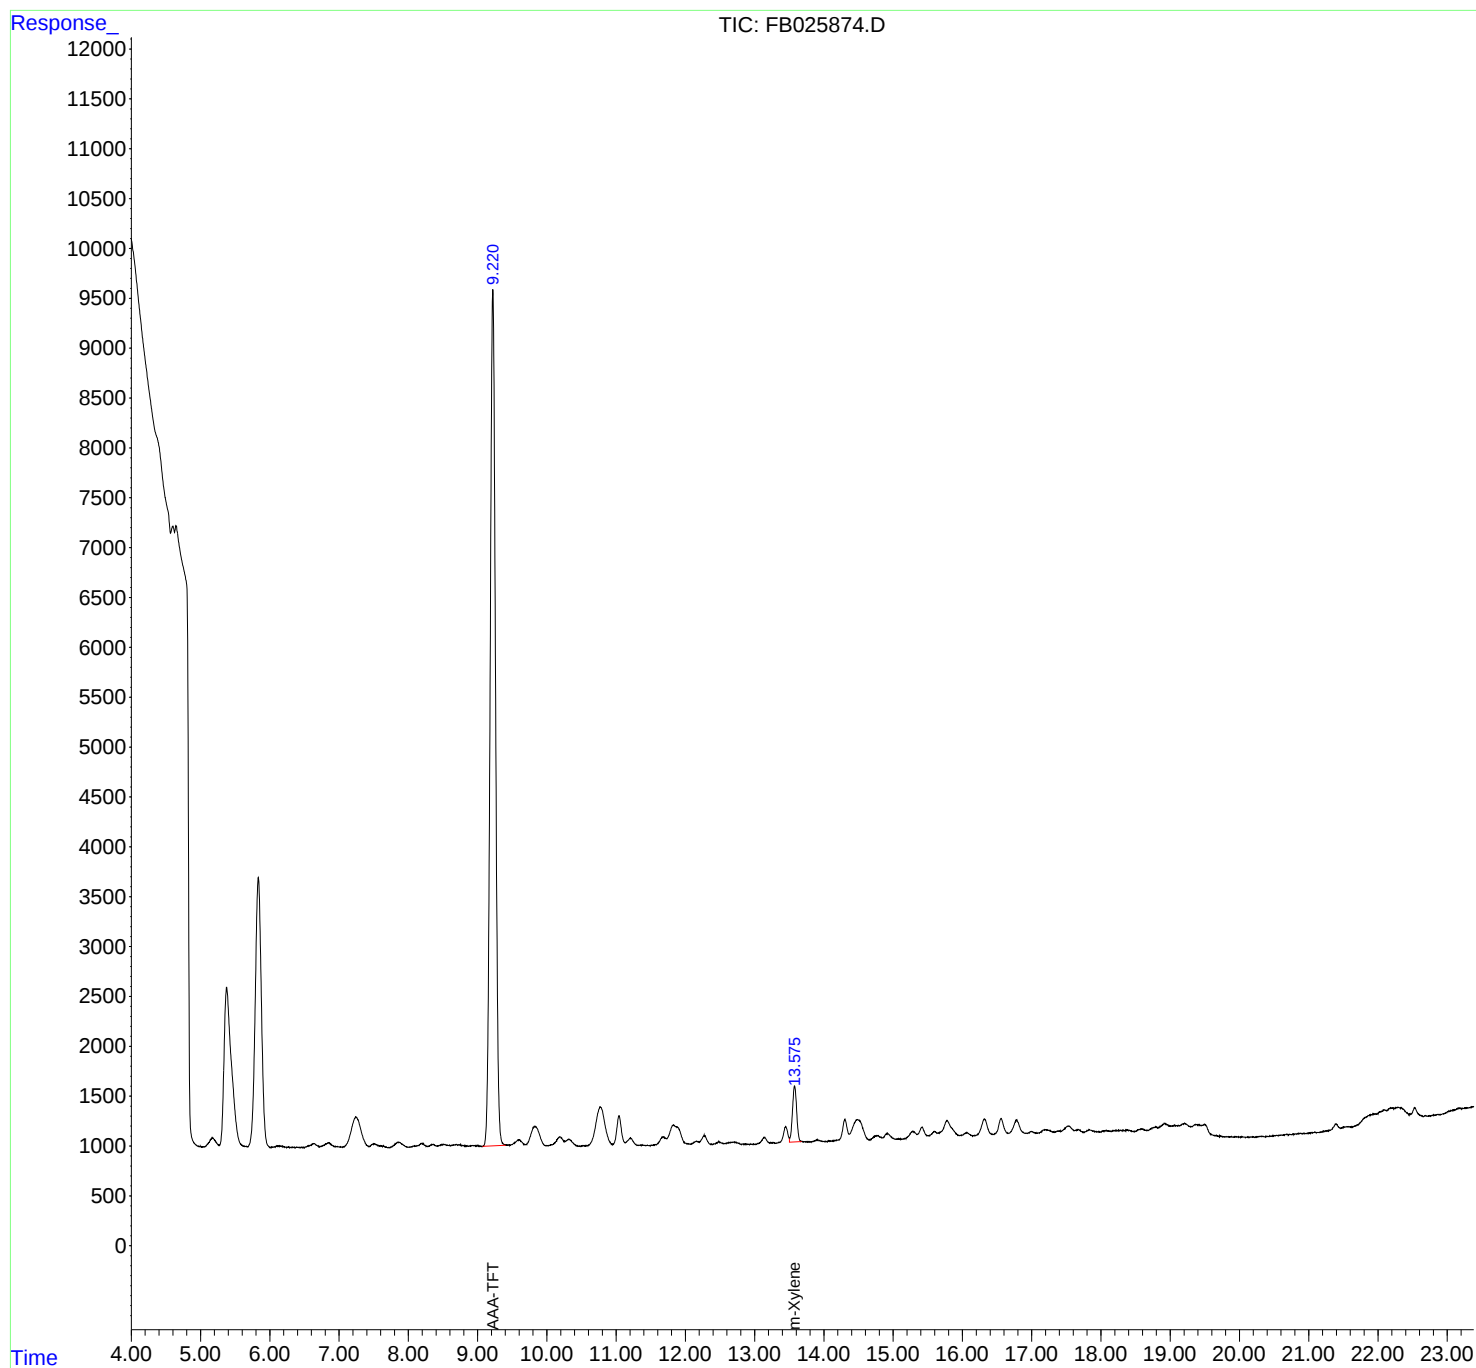


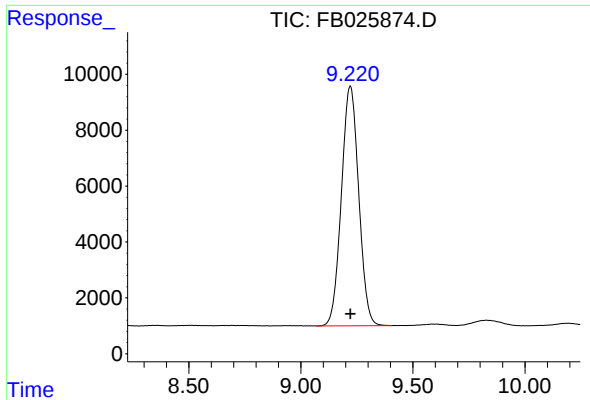

#5 AAA-TFT

R.T.: 9.221 min
Delta R.T.: 0.000 min
Response: 460249
Conc: 19.04 ng/ml

Instrument :
FID_B
ClientSampleId :

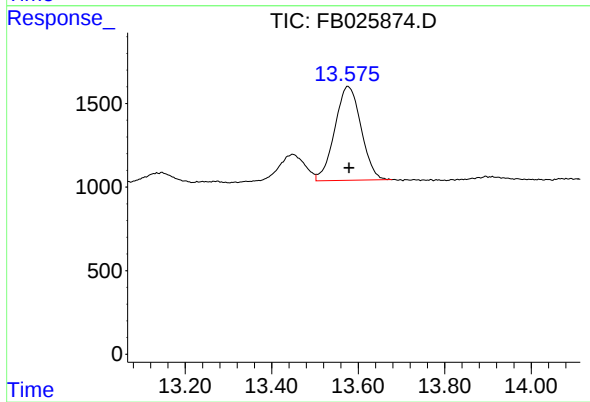

#8 m-Xylene

R.T.: 13.577 min
Delta R.T.: -0.002 min
Response: 23557
Conc: 0.60 ng/ml