

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
Data File : FB025876.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2021 12:32
Operator : DD/AJ
Sample : M2639-01
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 16 01:20:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.231	423441	17.522 ng/ml
Target Compounds			
6) t Toluene	11.048	20936	0.509 ng/ml
8) t m-Xylene	13.581	17075	0.434 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
Data File : FB025876.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2021 12:32
Operator : DD/AJ
Sample : M2639-01
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 16 01:20:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

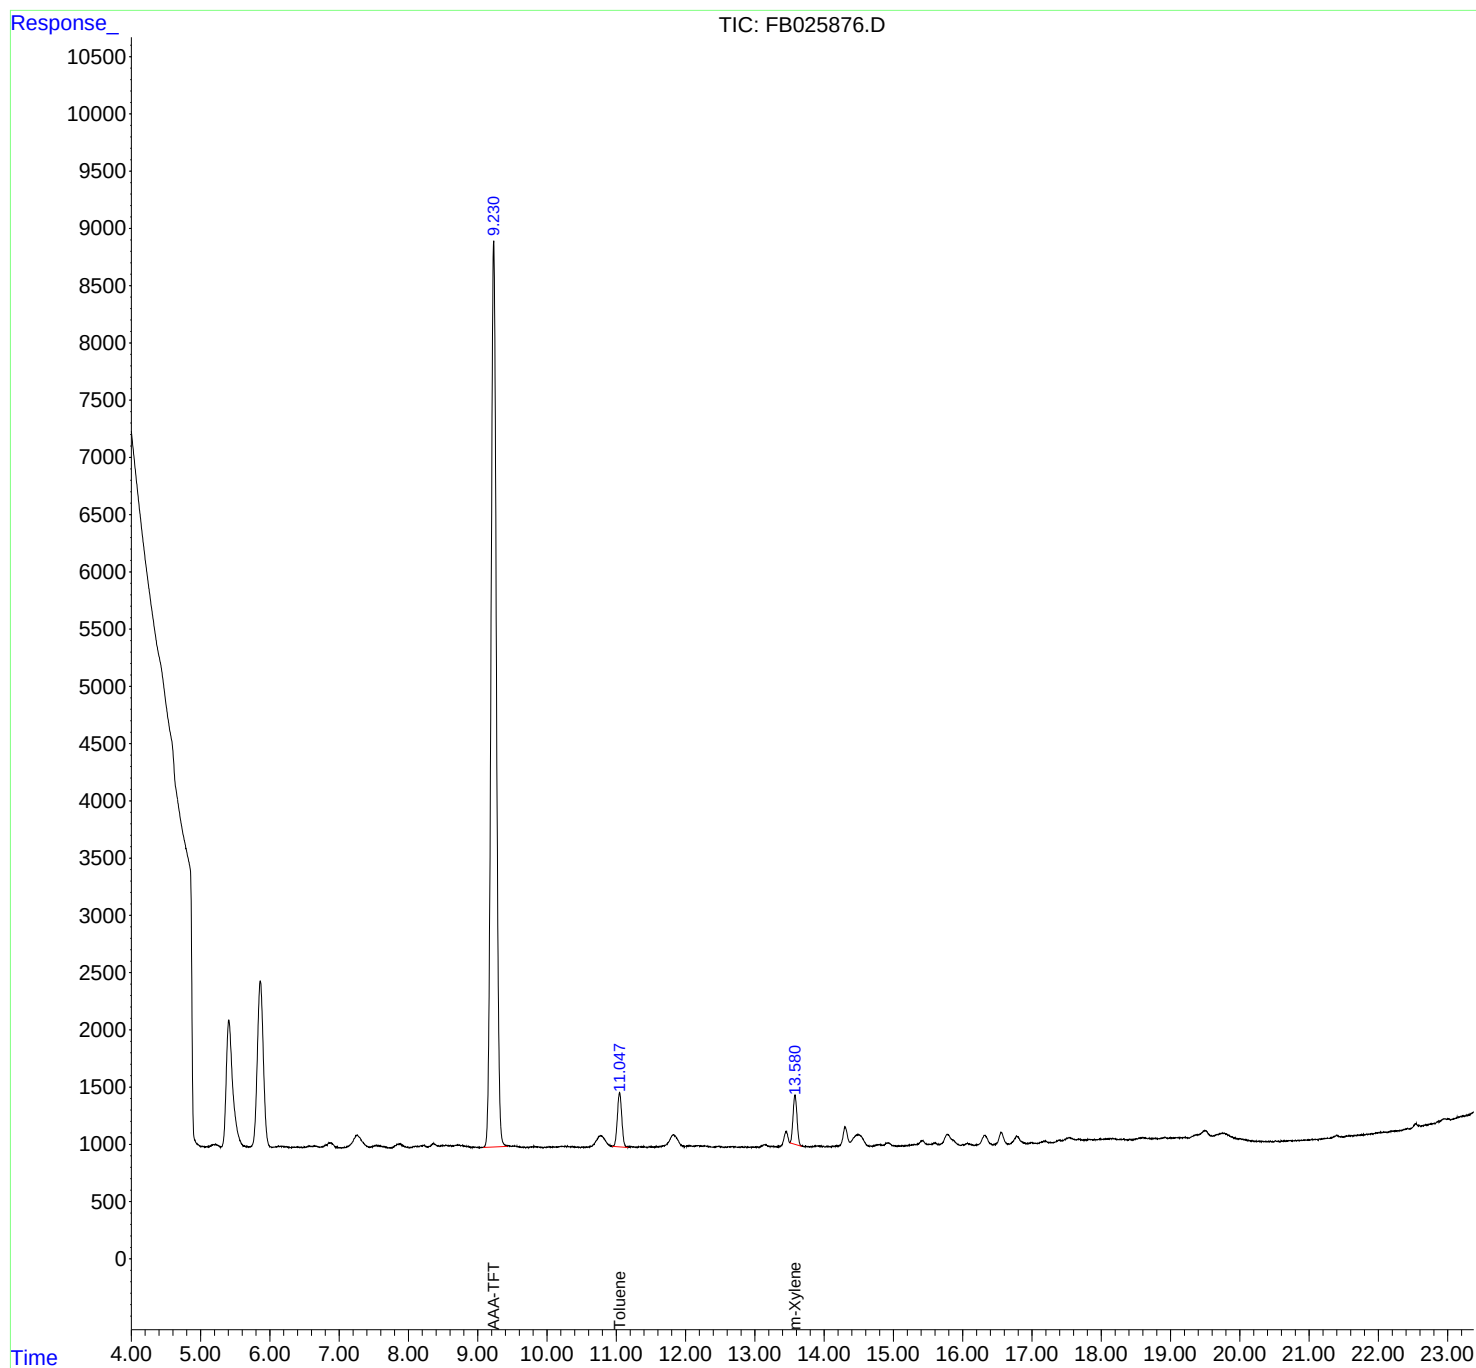


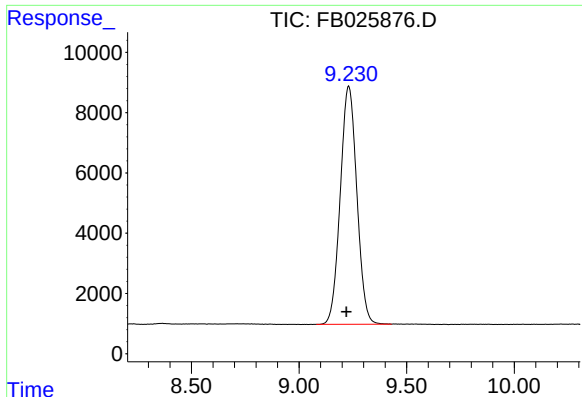

#5 AAA-TFT


R.T.: 9.231 min
Delta R.T.: 0.010 min
Response: 423441
Conc: 17.52 ng/ml

Instrument :
FID_B
ClientSampleId :

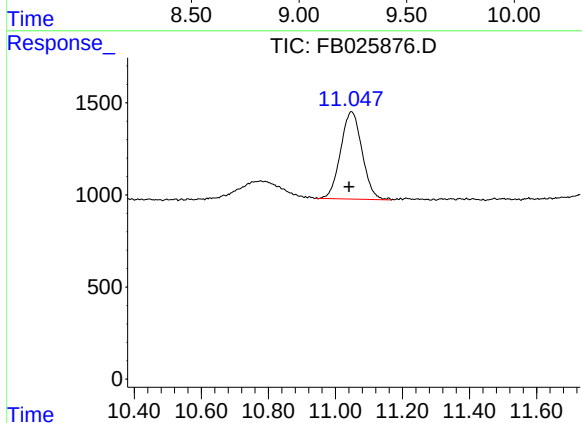

#6 Toluene

R.T.: 11.048 min
Delta R.T.: 0.007 min
Response: 20936
Conc: 0.51 ng/ml

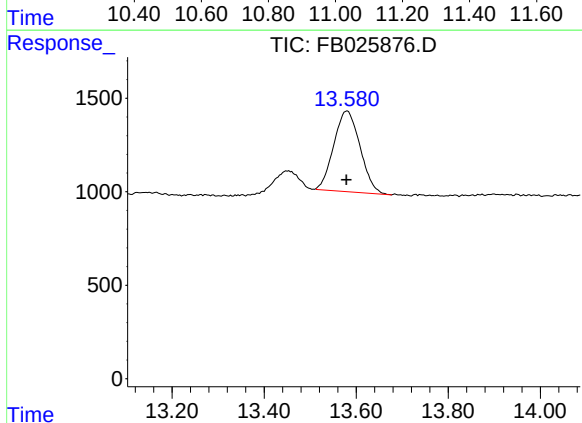

#8 m-Xylene

R.T.: 13.581 min
Delta R.T.: 0.002 min
Response: 17075
Conc: 0.43 ng/ml