

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
 Data File : FB025878.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jun 2021 13:56
 Operator : DD/AJ
 Sample : M2639-01MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 16 01:20:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.224	456960	18.909 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.185	685171	26.035 ng/ml
2) t 2,2,4-Trimethylpentane	7.881	494390	24.542 ng/ml
3) t n-Heptane	8.200	271803	7.562 ng/ml
4) t Benzene	8.350	397454	9.521 ng/ml
6) t Toluene	11.042	1076707	26.165 ng/ml
7) t Ethylbenzene	13.449	322365	8.458 ng/ml
8) t m-Xylene	13.580	629868	16.022 ng/ml
9) t O-Xylene	14.302	572802	17.965 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	325386	16.532 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
Data File : FB025878.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2021 13:56
Operator : DD/AJ
Sample : M2639-01MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 16 01:20:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

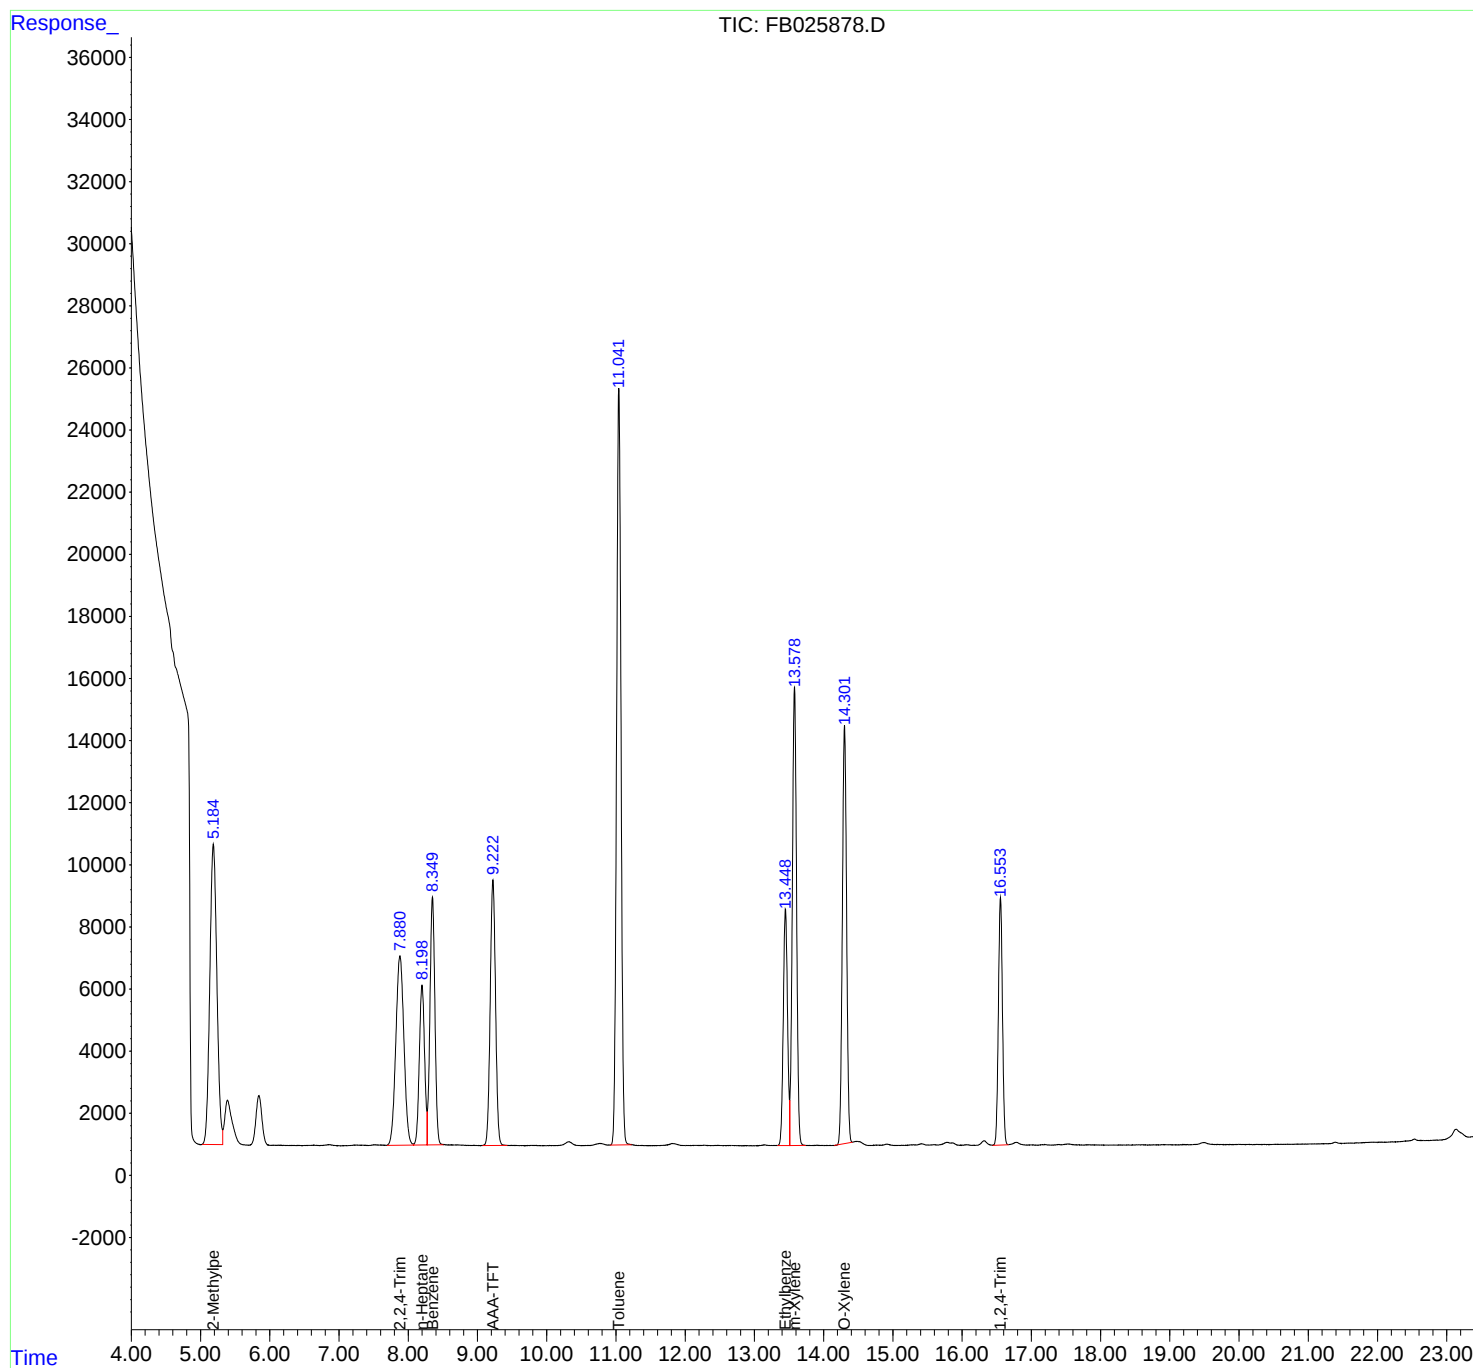


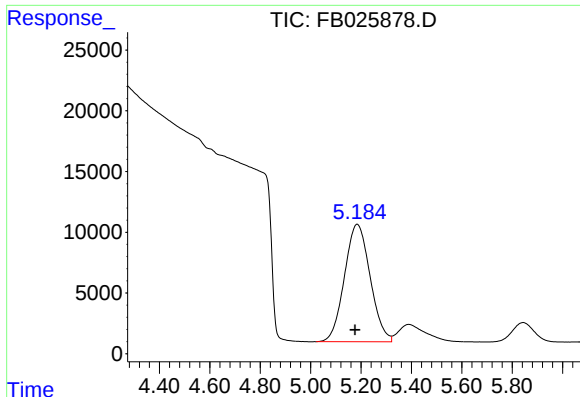

#1 2-Methylpentane


R.T.: 5.185 min
Delta R.T.: 0.008 min
Response: 685171
Conc: 26.04 ng/ml

Instrument :
FID_B
ClientSampleId :

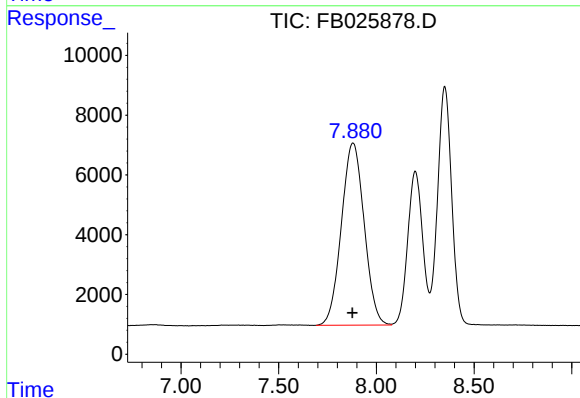


#2 2,2,4-Trimethylpentane

R.T.: 7.881 min
Delta R.T.: 0.003 min
Response: 494390
Conc: 24.54 ng/ml

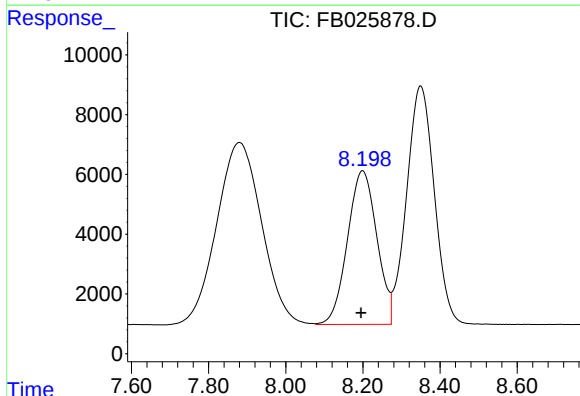


#3 n-Heptane

R.T.: 8.200 min
Delta R.T.: 0.004 min
Response: 271803
Conc: 7.56 ng/ml

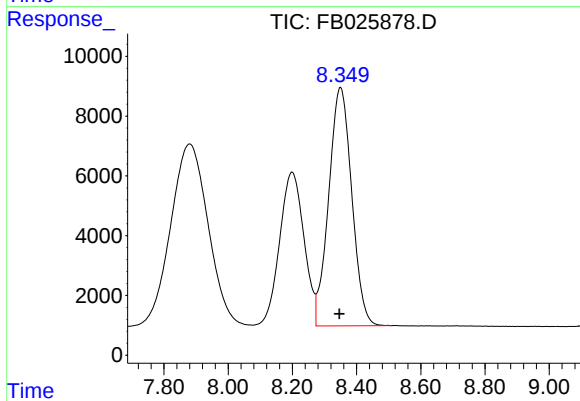

#4 Benzene


R.T.: 8.350 min
Delta R.T.: 0.004 min
Response: 397454
Conc: 9.52 ng/ml

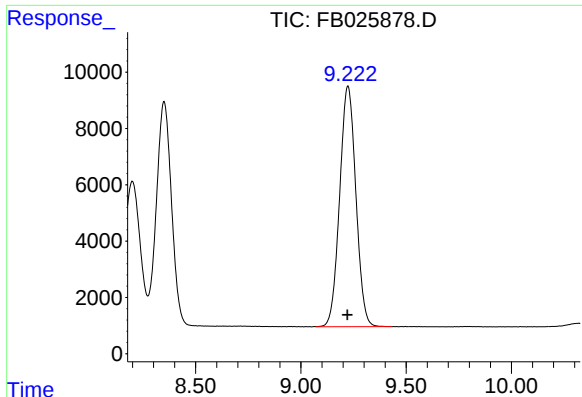

#5 AAA-TFT


R.T.: 9.224 min
Delta R.T.: 0.003 min
Response: 456960
Conc: 18.91 ng/ml

Instrument :
FID_B
ClientSampleId :

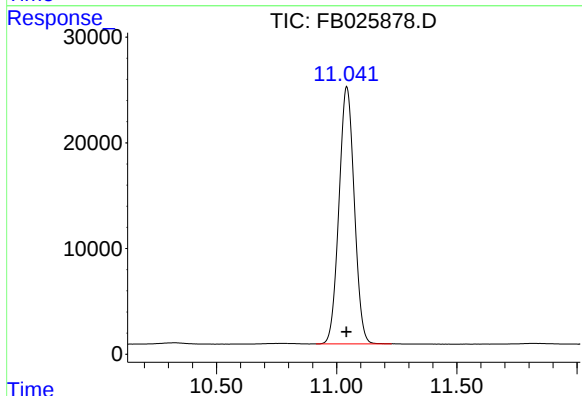


#6 Toluene

R.T.: 11.042 min
Delta R.T.: 0.001 min
Response: 1076707
Conc: 26.16 ng/ml

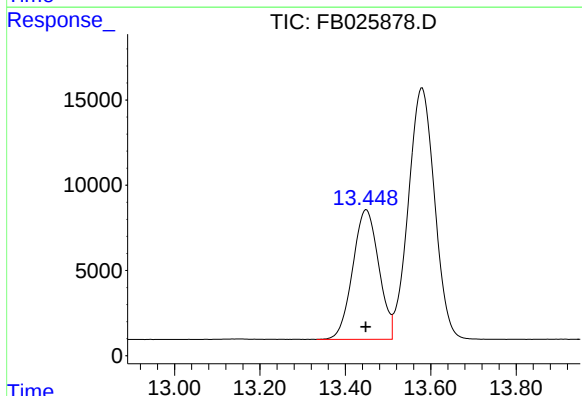


#7 Ethylbenzene

R.T.: 13.449 min
Delta R.T.: 0.001 min
Response: 322365
Conc: 8.46 ng/ml

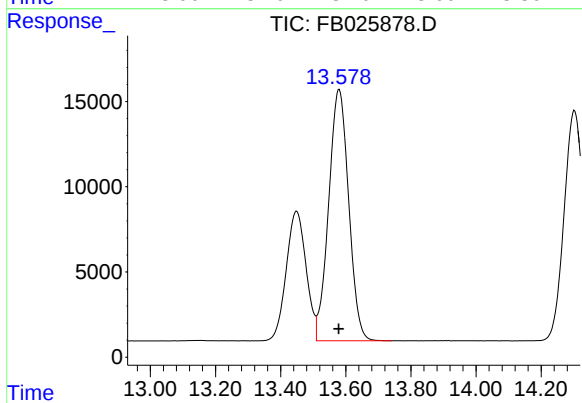

#8 m-Xylene


R.T.: 13.580 min
Delta R.T.: 0.001 min
Response: 629868
Conc: 16.02 ng/ml

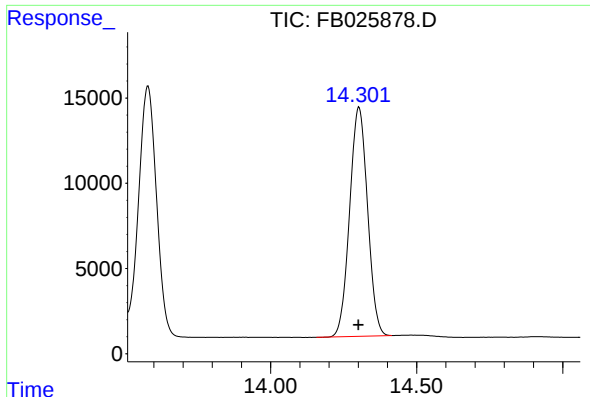

#9 O-Xylene

R.T.: 14.302 min
Delta R.T.: 0.001 min
Response: 572802
Conc: 17.96 ng/ml

Instrument :
FID_B
ClientSampleId :

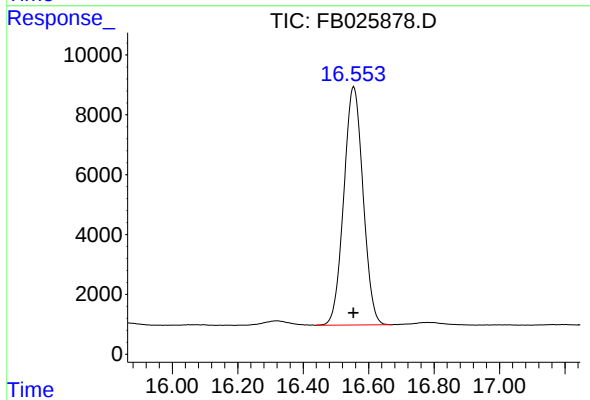

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: 0.001 min
Response: 325386
Conc: 16.53 ng/ml