

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
 Data File : FB025875.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jun 2021 11:56
 Operator : DD/AJ
 Sample : BSF0615S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0615S1

Integration File: Calibration.e
 Quant Time: Jun 16 01:20:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.226	470876	19.484 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.193	809914	30.775 ng/ml
2) t 2,2,4-Trimethylpentane	7.885	661489	32.836 ng/ml
3) t n-Heptane	8.203	370938	10.319 ng/ml
4) t Benzene	8.354	410095	9.824 ng/ml
6) t Toluene	11.044	1155576	28.081 ng/ml
7) t Ethylbenzene	13.449	350922	9.208 ng/ml
8) t m-Xylene	13.579	688312	17.509 ng/ml
9) t O-Xylene	14.302	610868	19.158 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	364982	18.543 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
Data File : FB025875.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2021 11:56
Operator : DD/AJ
Sample : BSF0615S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0615S1

Integration File: Calibration.e
Quant Time: Jun 16 01:20:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

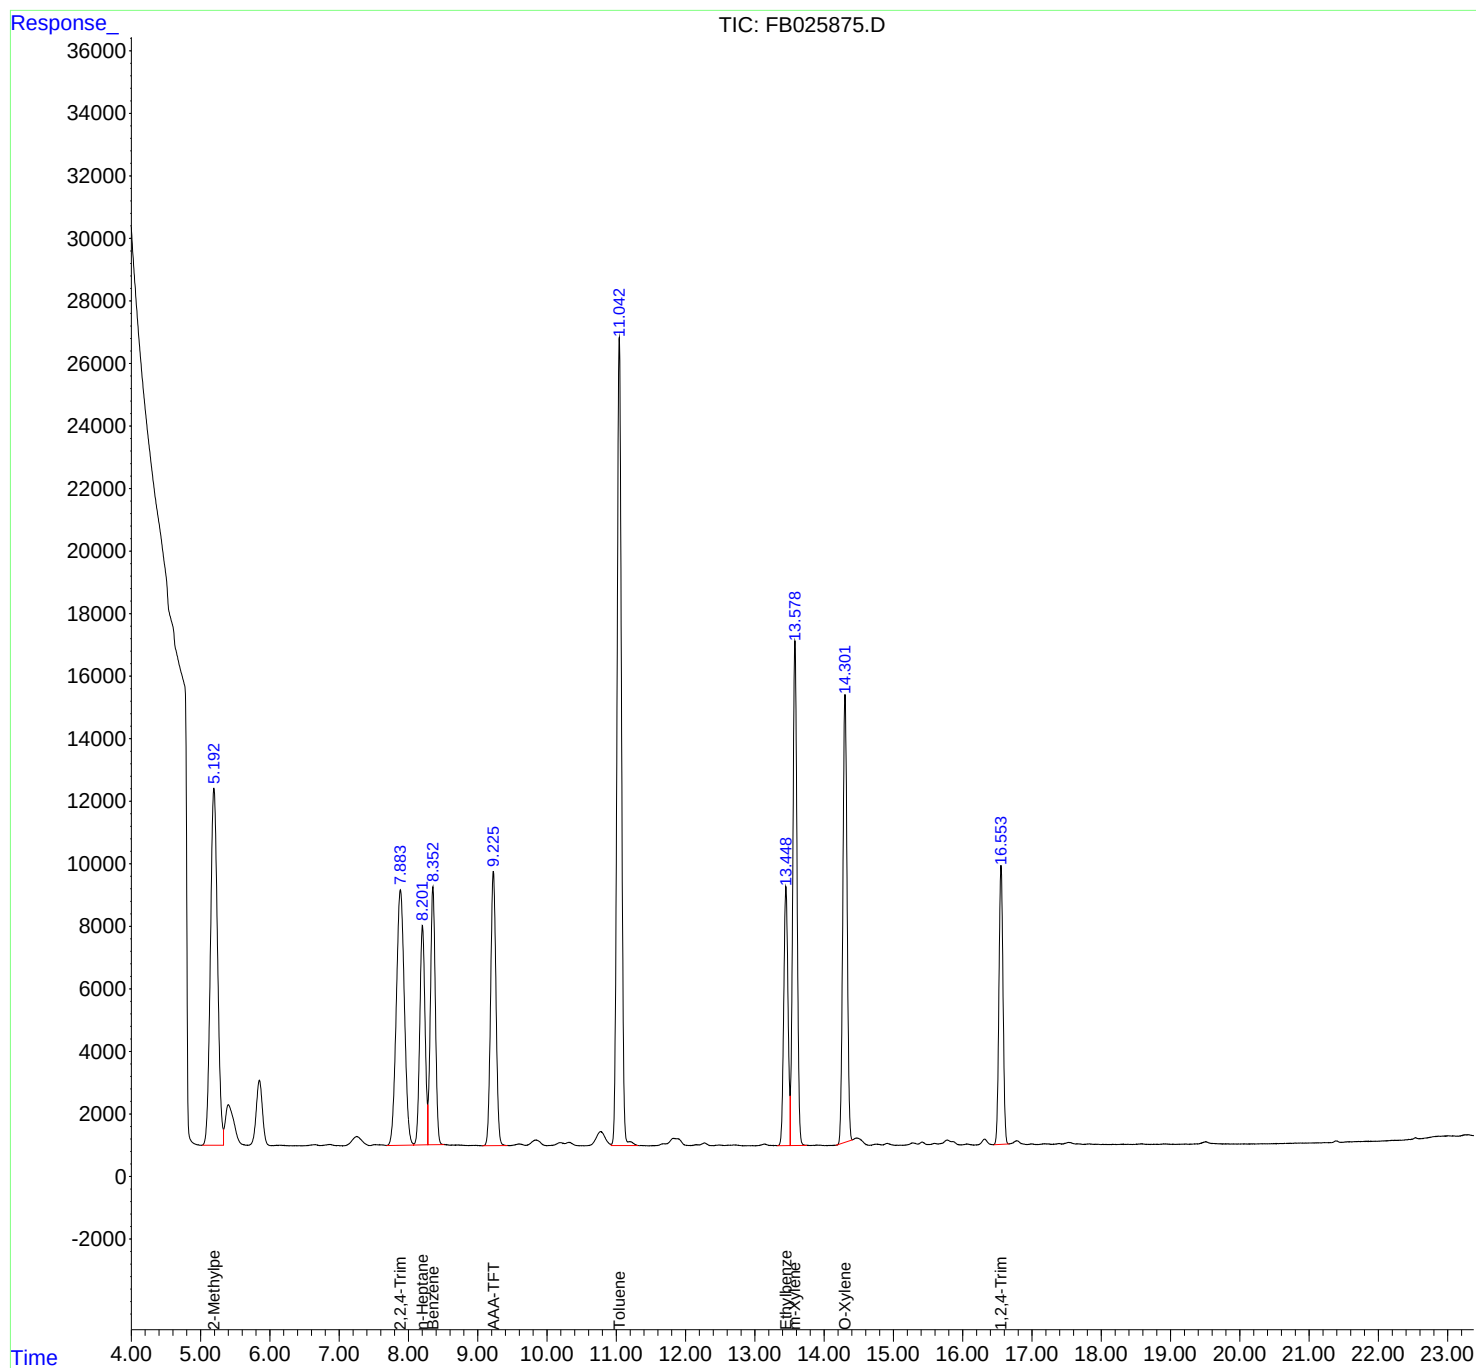


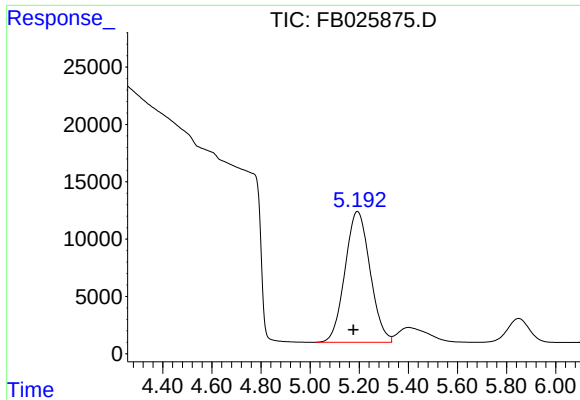

#1 2-Methylpentane


R.T.: 5.193 min
Delta R.T.: 0.016 min
Response: 809914
Conc: 30.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0615S1

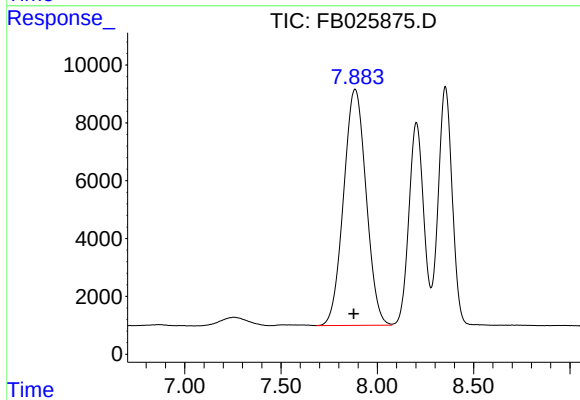


#2 2,2,4-Trimethylpentane

R.T.: 7.885 min
Delta R.T.: 0.006 min
Response: 661489
Conc: 32.84 ng/ml

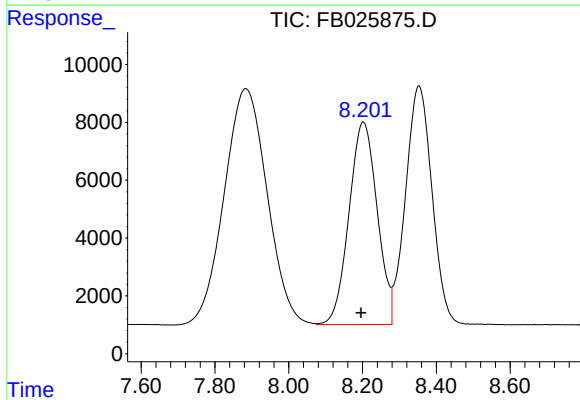


#3 n-Heptane

R.T.: 8.203 min
Delta R.T.: 0.007 min
Response: 370938
Conc: 10.32 ng/ml

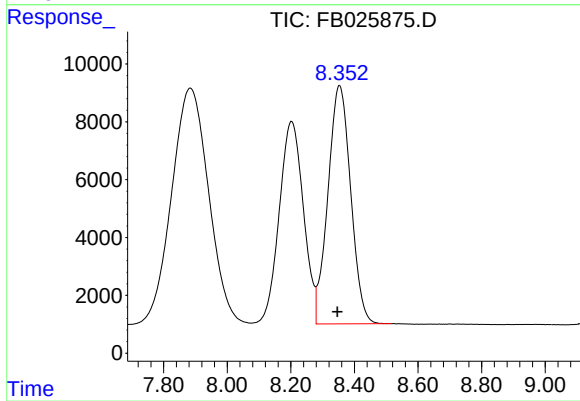

#4 Benzene


R.T.: 8.354 min
Delta R.T.: 0.007 min
Response: 410095
Conc: 9.82 ng/ml

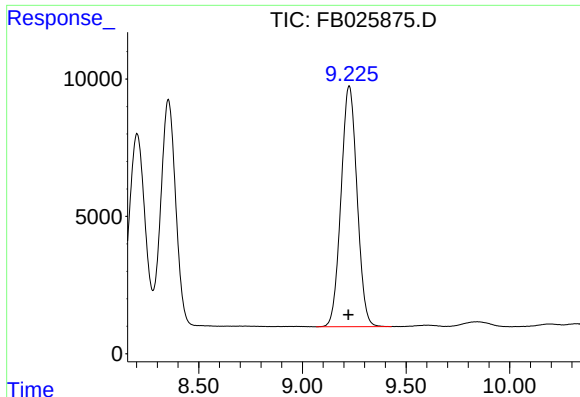

#5 AAA-TFT


R.T.: 9.226 min
Delta R.T.: 0.005 min
Response: 470876
Conc: 19.48 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0615S1

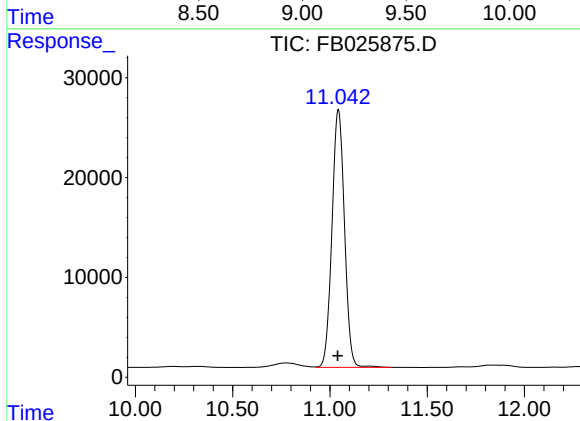


#6 Toluene

R.T.: 11.044 min
Delta R.T.: 0.003 min
Response: 1155576
Conc: 28.08 ng/ml

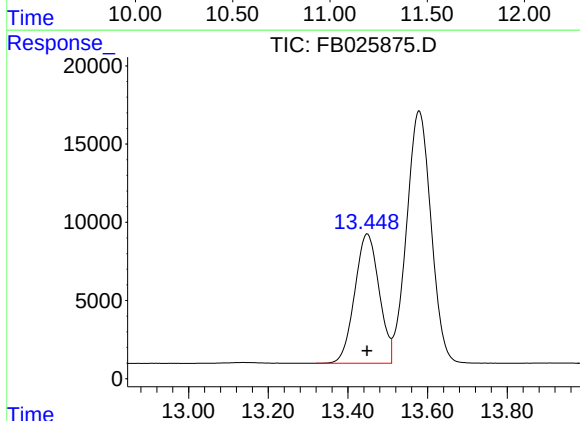


#7 Ethylbenzene

R.T.: 13.449 min
Delta R.T.: 0.000 min
Response: 350922
Conc: 9.21 ng/ml

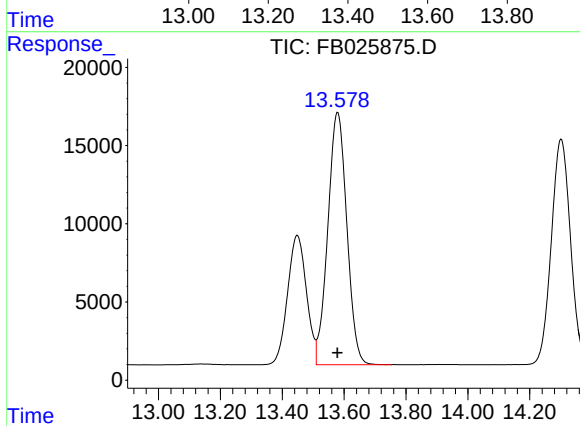

#8 m-Xylene


R.T.: 13.579 min
Delta R.T.: 0.000 min
Response: 688312
Conc: 17.51 ng/ml

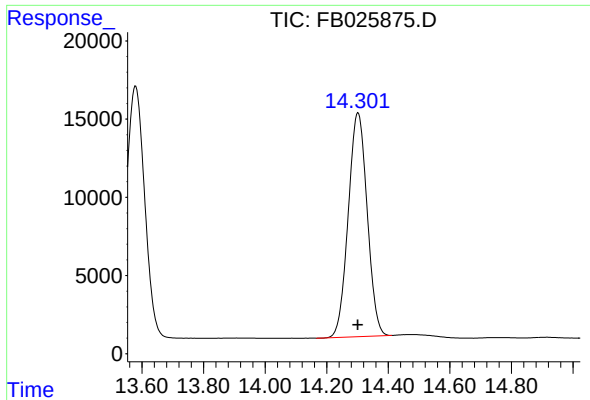

#9 O-Xylene

R.T.: 14.302 min
Delta R.T.: 0.000 min
Response: 610868
Conc: 19.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0615S1

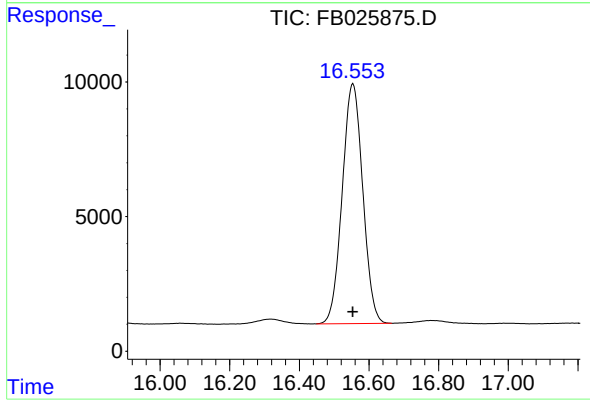

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: 0.000 min
Response: 364982
Conc: 18.54 ng/ml