

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
 Data File : FB025877.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jun 2021 13:11
 Operator : DD/AJ
 Sample : M2639-01MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 B67MS

Integration File: Calibration.e
 Quant Time: Jun 16 01:20:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.218	488705	20.222 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.168	763714	29.020 ng/ml
2) t 2,2,4-Trimethylpentane	7.871	592969	29.435 ng/ml
3) t n-Heptane	8.191	324312	9.022 ng/ml
4) t Benzene	8.342	411870	9.866 ng/ml
6) t Toluene	11.039	1138809	27.674 ng/ml
7) t Ethylbenzene	13.447	344549	9.041 ng/ml
8) t m-Xylene	13.577	673064	17.121 ng/ml
9) t O-Xylene	14.301	598049	18.756 ng/ml
10) t 1,2,4-Trimethylbenzene	16.553	343440	17.449 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061521\
Data File : FB025877.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2021 13:11
Operator : DD/AJ
Sample : M2639-01MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B67MS

Integration File: Calibration.e
Quant Time: Jun 16 01:20:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

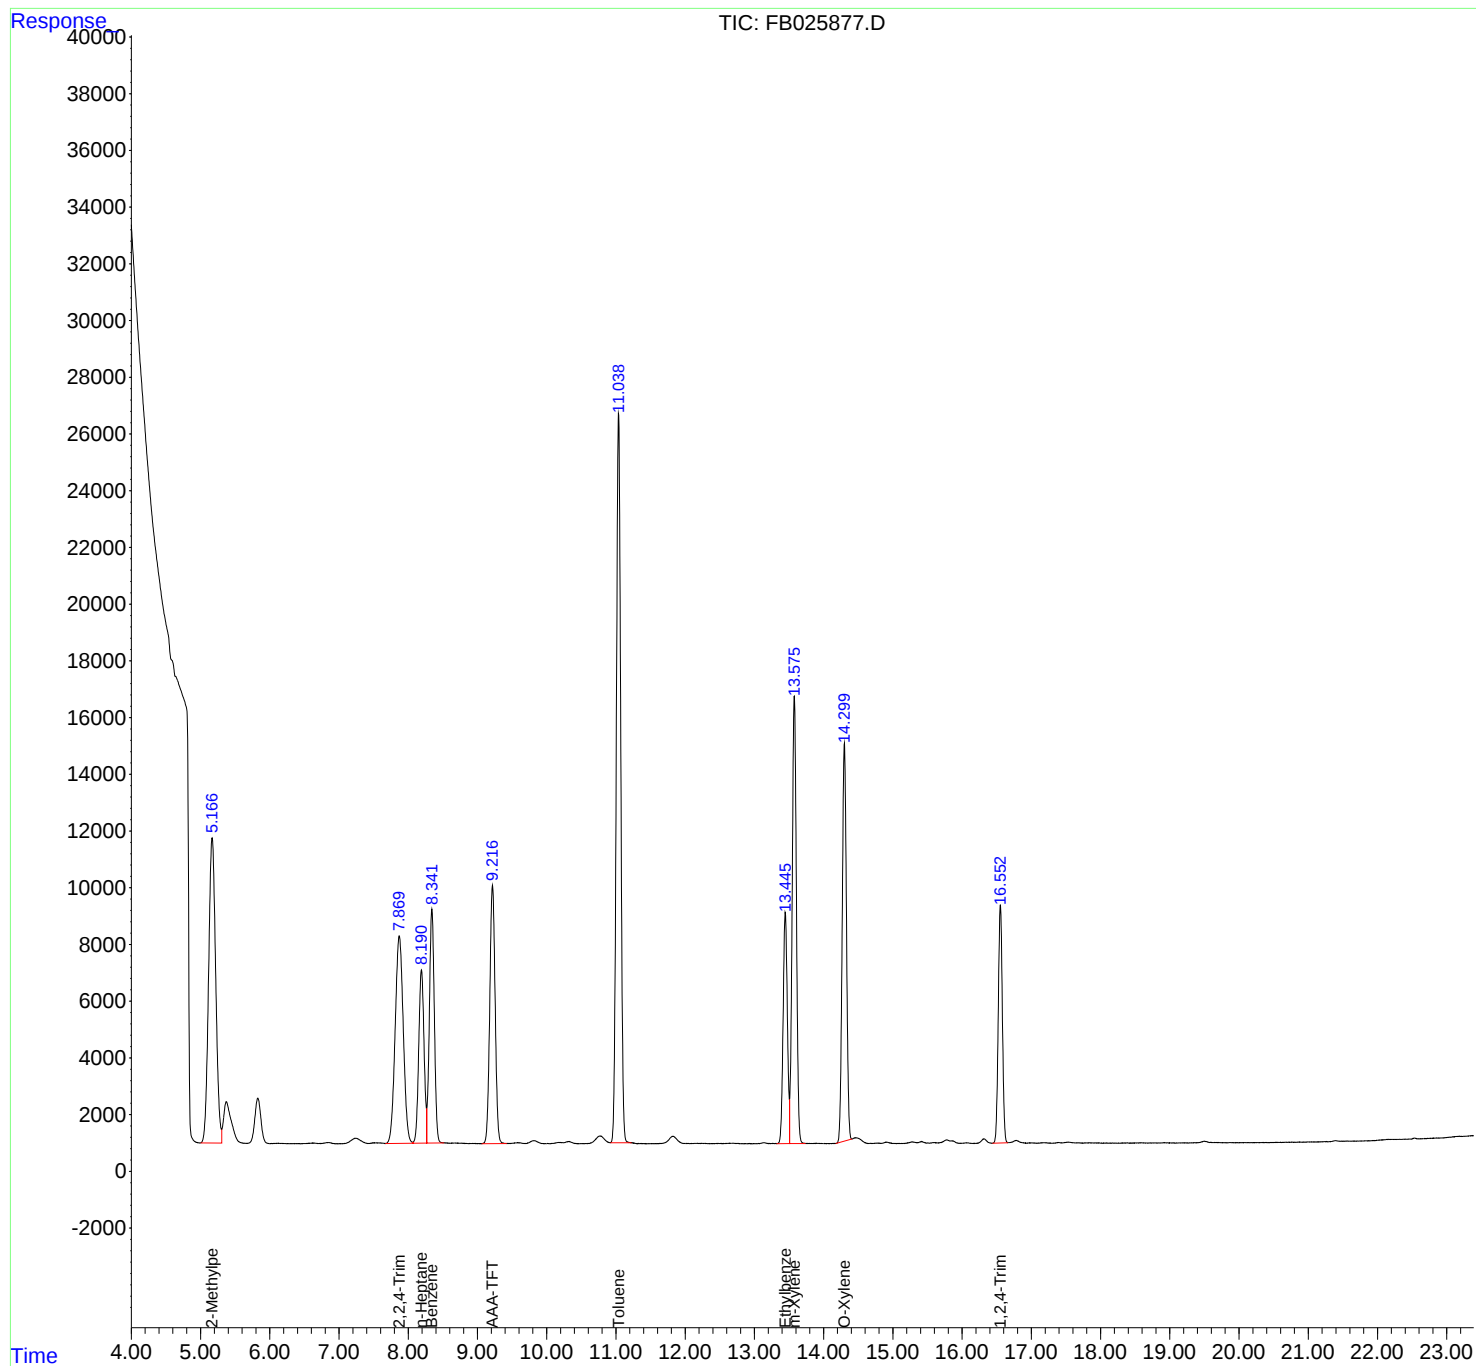


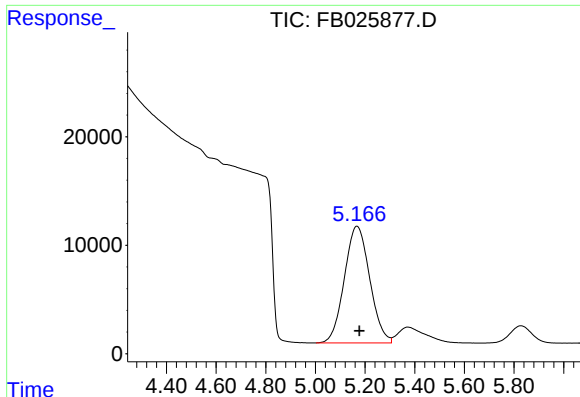

#1 2-Methylpentane


R.T.: 5.168 min
Delta R.T.: -0.009 min
Response: 763714
Conc: 29.02 ng/ml

Instrument :
FID_B
ClientSampleId :
B67MS

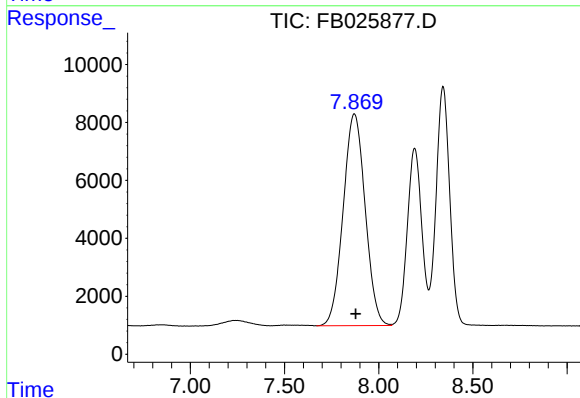


#2 2,2,4-Trimethylpentane

R.T.: 7.871 min
Delta R.T.: -0.008 min
Response: 592969
Conc: 29.44 ng/ml

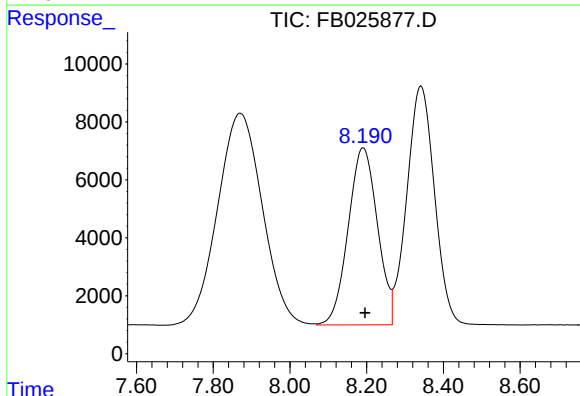


#3 n-Heptane

R.T.: 8.191 min
Delta R.T.: -0.005 min
Response: 324312
Conc: 9.02 ng/ml

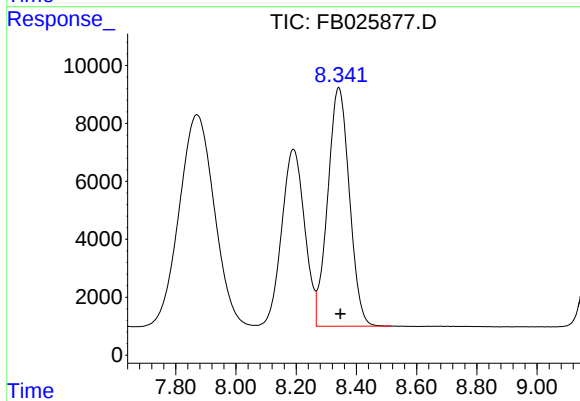

#4 Benzene


R.T.: 8.342 min
Delta R.T.: -0.005 min
Response: 411870
Conc: 9.87 ng/ml

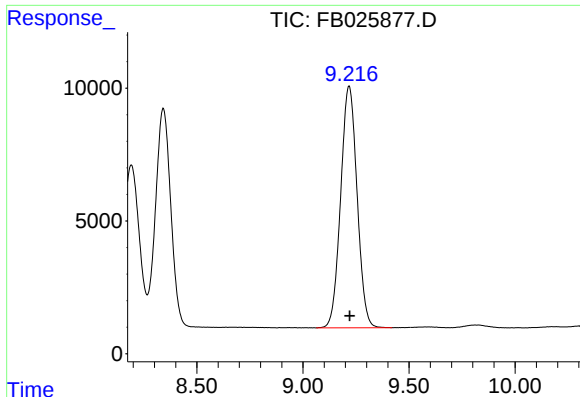

#5 AAA-TFT


R.T.: 9.218 min
Delta R.T.: -0.004 min
Response: 488705
Conc: 20.22 ng/ml

Instrument :
FID_B
ClientSampleId :
B67MS

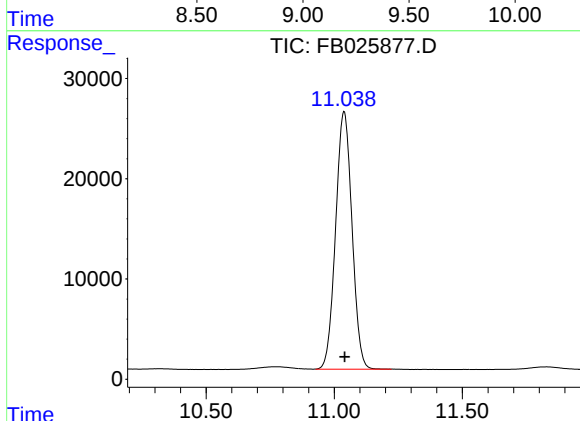


#6 Toluene

R.T.: 11.039 min
Delta R.T.: -0.002 min
Response: 1138809
Conc: 27.67 ng/ml

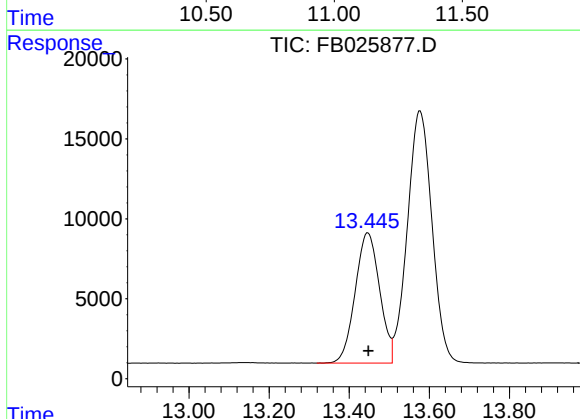


#7 Ethylbenzene

R.T.: 13.447 min
Delta R.T.: -0.001 min
Response: 344549
Conc: 9.04 ng/ml

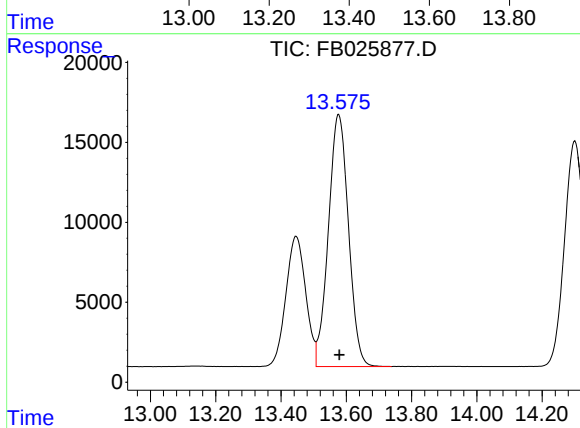

#8 m-Xylene


R.T.: 13.577 min
Delta R.T.: -0.002 min
Response: 673064
Conc: 17.12 ng/ml

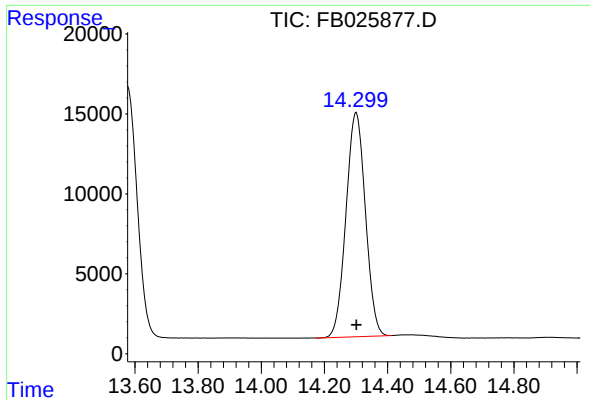

#9 O-Xylene

R.T.: 14.301 min
Delta R.T.: 0.000 min
Response: 598049
Conc: 18.76 ng/ml

Instrument :
FID_B
ClientSampleId :
B67MS

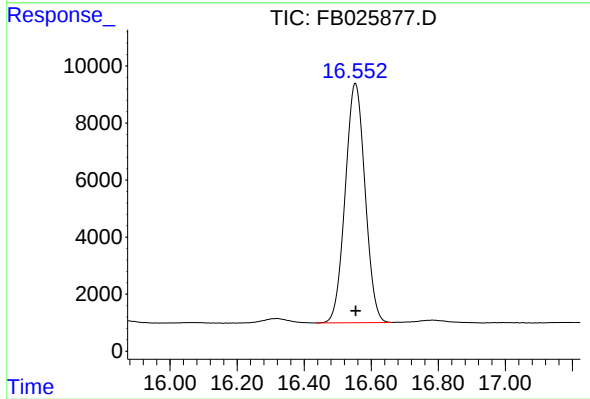

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min
Delta R.T.: 0.000 min
Response: 343440
Conc: 17.45 ng/ml