

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061522\
Data File : FB027446.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2022 9:17
Operator : AJ/MA
Sample : VBF0615S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 16 01:19:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	245534	21.890 ng/ml
Target Compounds			
4) t Benzene	7.884	839	0.041 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061522\
Data File : FB027446.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2022 9:17
Operator : AJ/MA
Sample : VBF0615S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 16 01:19:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

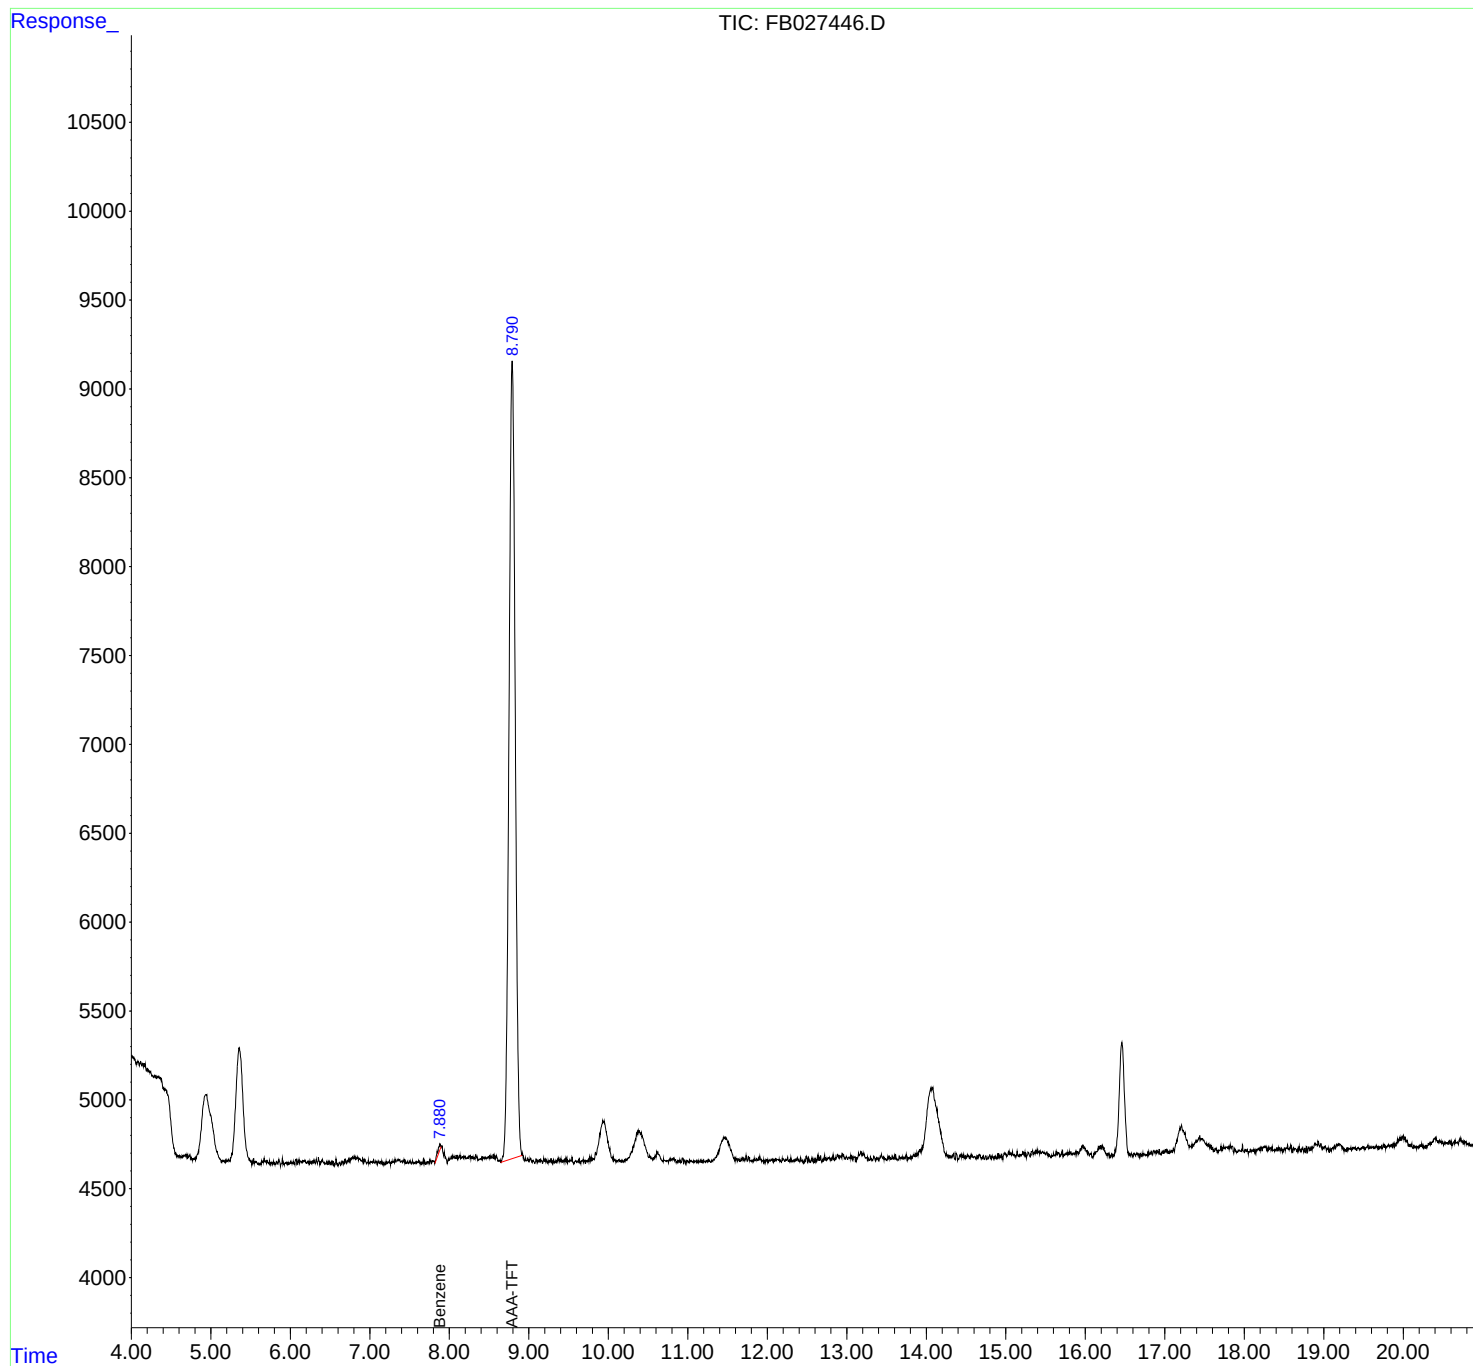


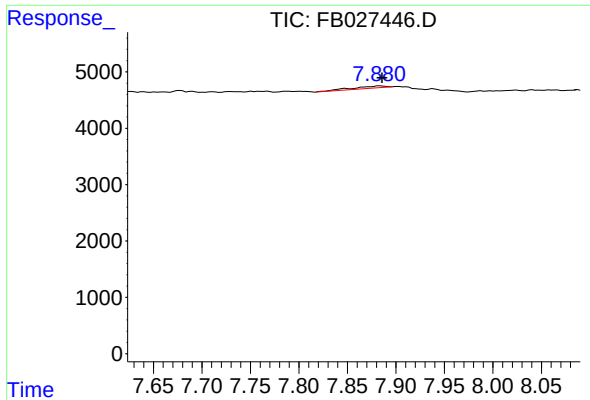

#4 Benzene

R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 839
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :

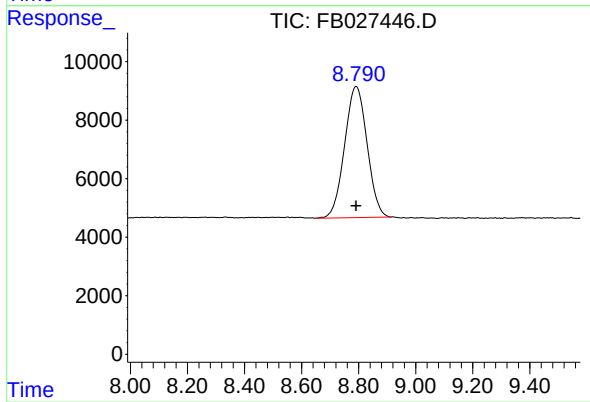

#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.001 min
Response: 245534
Conc: 21.89 ng/ml