

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061522\
 Data File : FB027448.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jun 2022 10:30
 Operator : AJ/MA
 Sample : BSF0615S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0615S1

Integration File: SAMPLE.e
 Quant Time: Jun 16 01:20:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	222041	19.796 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	528445	31.367 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	553427	31.519 ng/ml
3) t n-Heptane	7.750	179280	10.234 ng/ml
4) t Benzene	7.886	209657	10.281 ng/ml
6) t Toluene	10.619	589905	30.467 ng/ml
7) t Ethylbenzene	13.056	183654	10.141 ng/ml
8) t m-Xylene	13.189	367266	20.603 ng/ml
9) t O-Xylene	13.916	355663	20.469 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	362218	21.086 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061522\
Data File : FB027448.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2022 10:30
Operator : AJ/MA
Sample : BSF0615S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0615S1

Integration File: SAMPLE.e
Quant Time: Jun 16 01:20:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

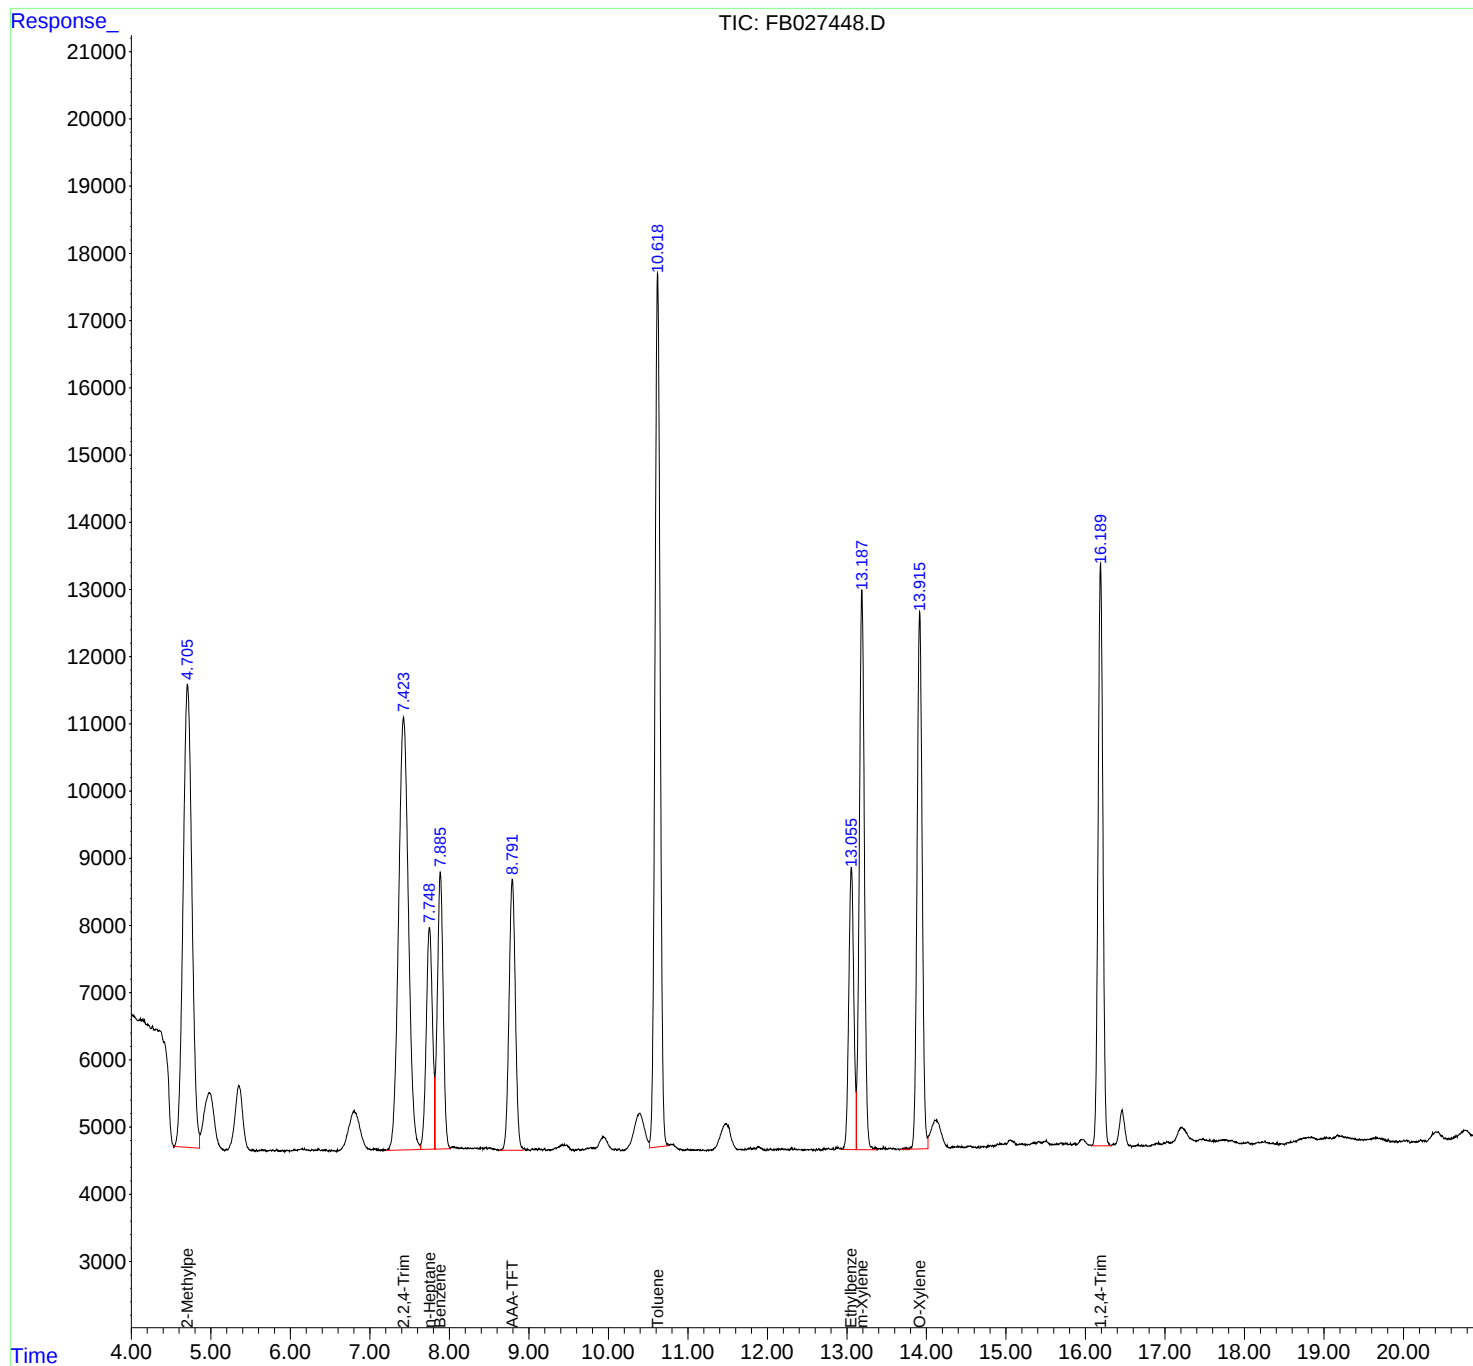


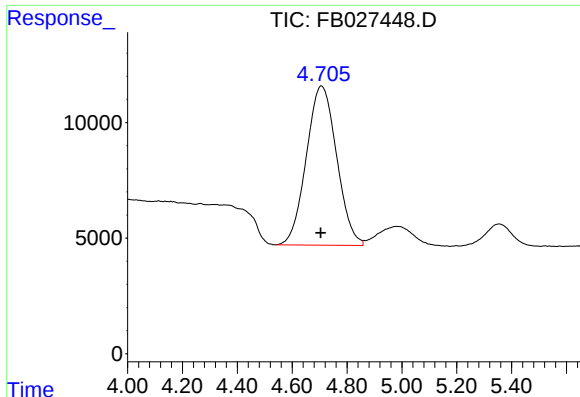

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.003 min
Response: 528445
Conc: 31.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0615S1

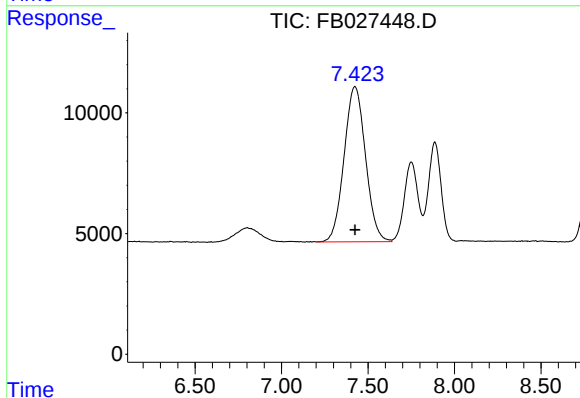


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.002 min
Response: 553427
Conc: 31.52 ng/ml

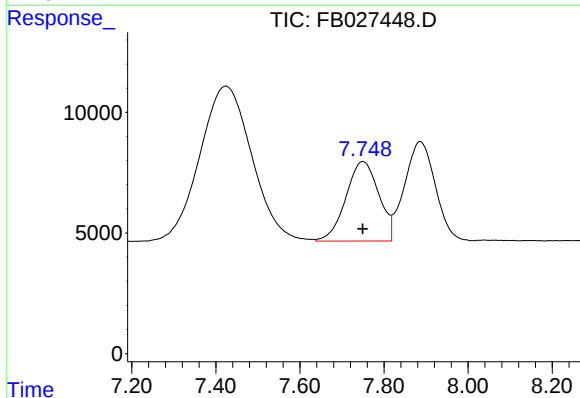


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 179280
Conc: 10.23 ng/ml

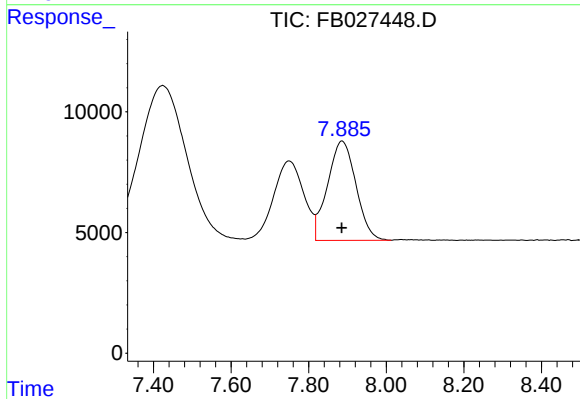

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 209657
Conc: 10.28 ng/ml

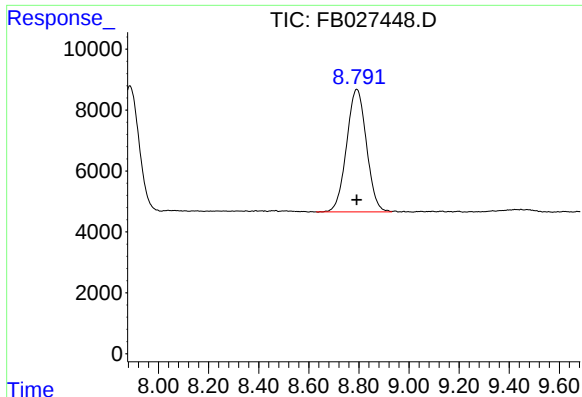

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.001 min
Response: 222041
Conc: 19.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0615S1

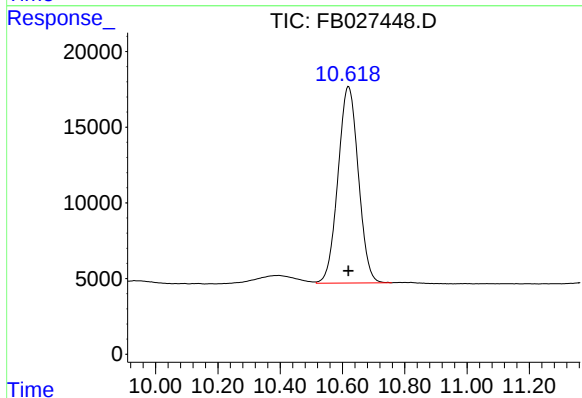


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 589905
Conc: 30.47 ng/ml

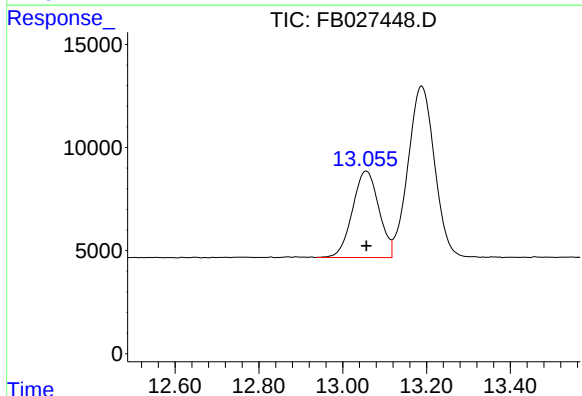


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 183654
Conc: 10.14 ng/ml

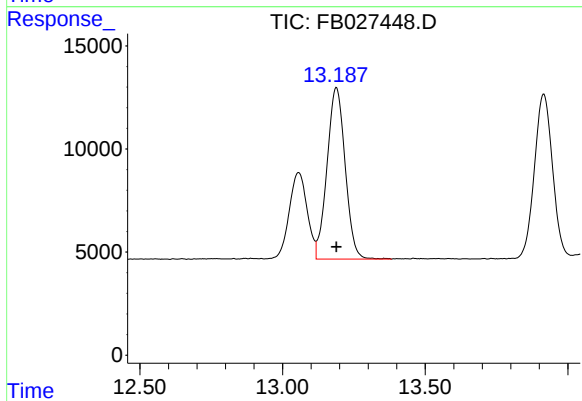

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 367266
Conc: 20.60 ng/ml

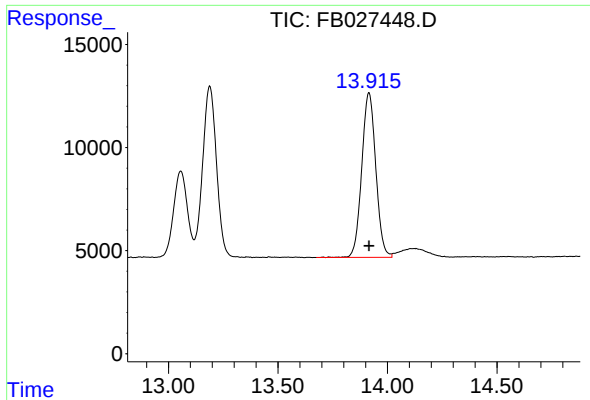

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 355663
Conc: 20.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0615S1

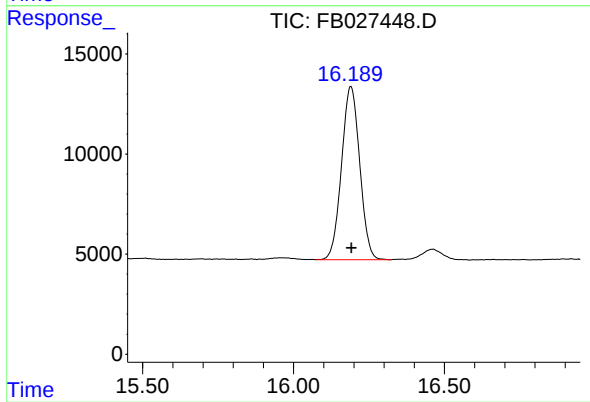

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.001 min
Response: 362218
Conc: 21.09 ng/ml