

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030056.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2023 9:53
Operator : YP/AJ
Sample : 03289-11
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 19 01:41:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	266155	19.131 ng/ml
Target Compounds			
4) t Benzene	7.885	4896	0.219 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030056.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2023 9:53
Operator : YP/AJ
Sample : 03289-11
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 19 01:41:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

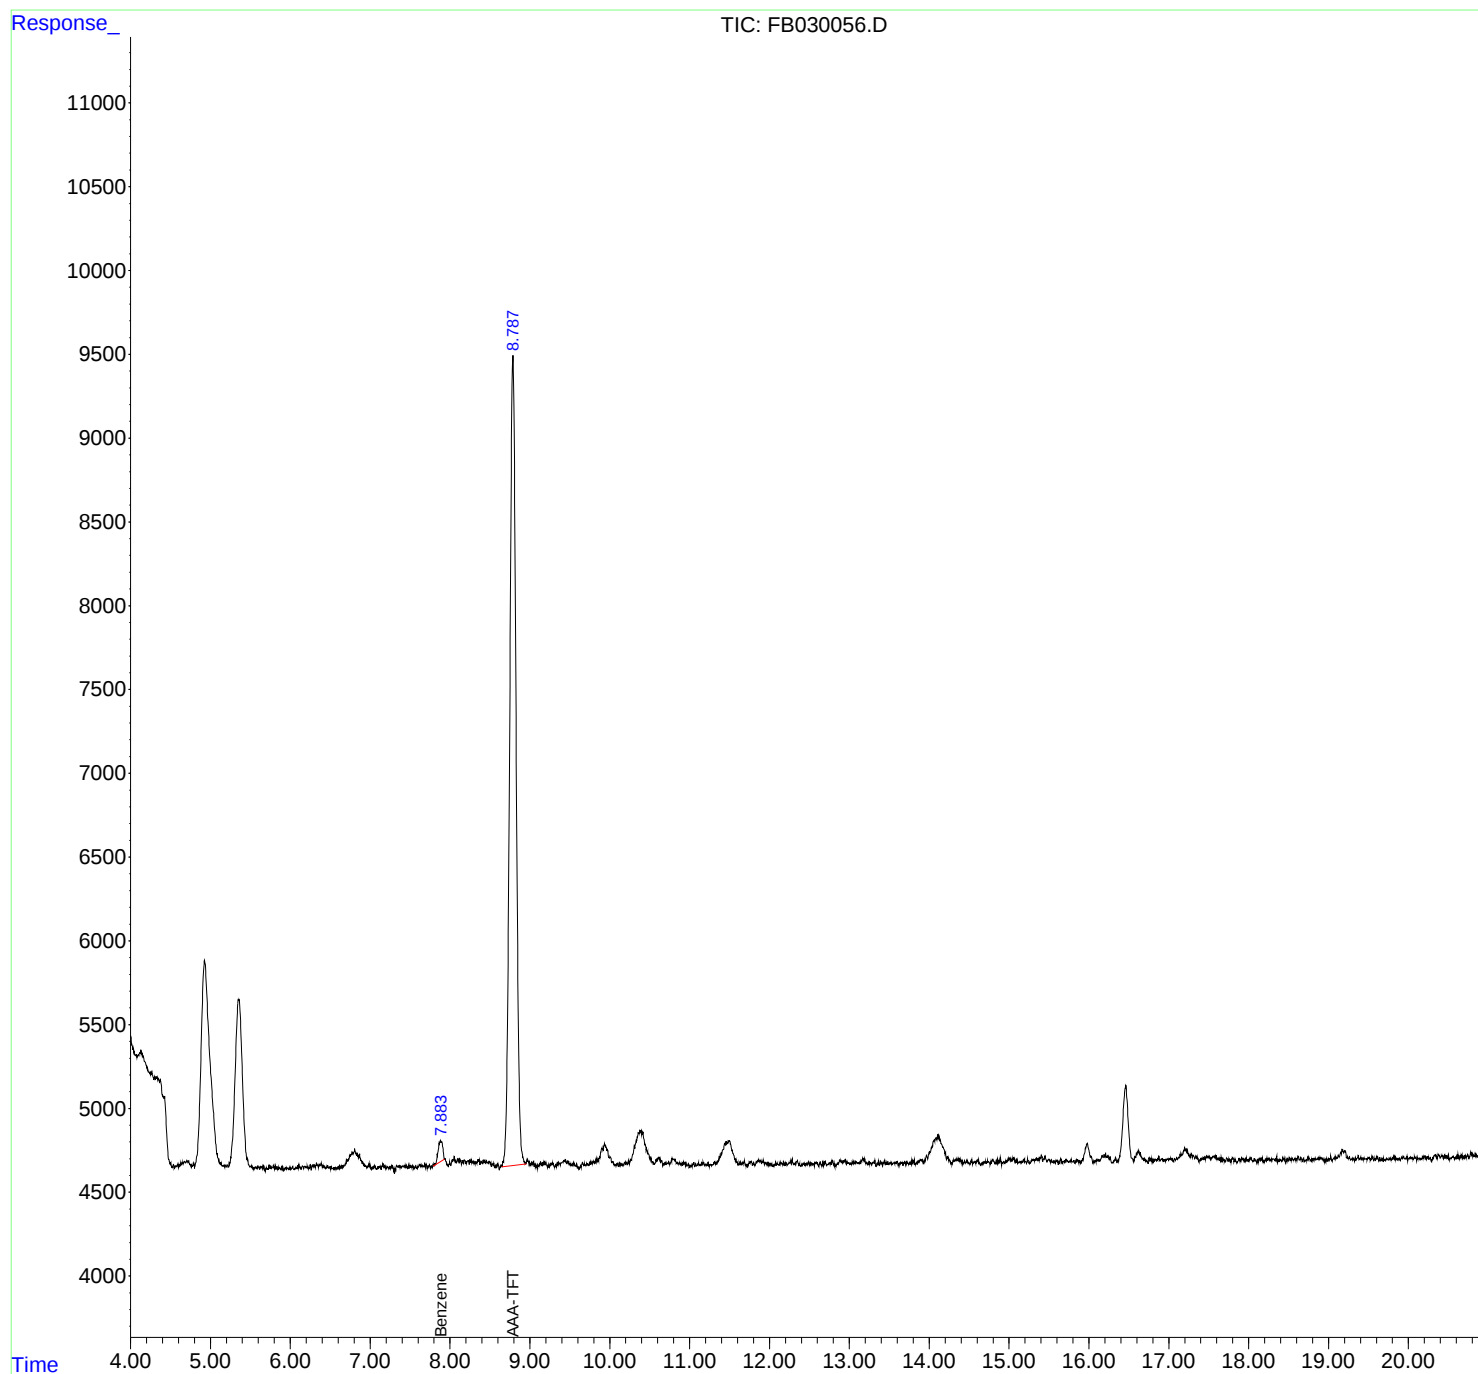


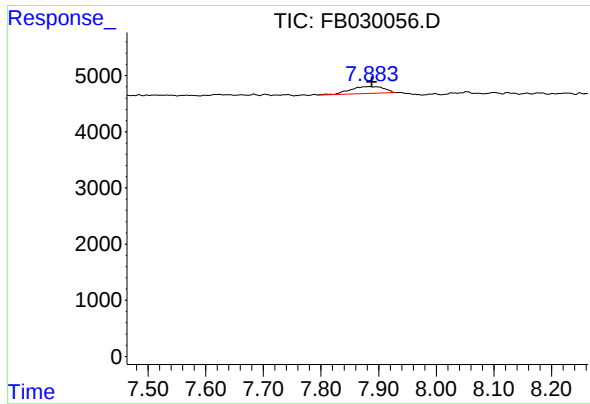

#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.003 min
Response: 4896
Conc: 0.22 ng/ml

Instrument :
FID_B
ClientSampleId :

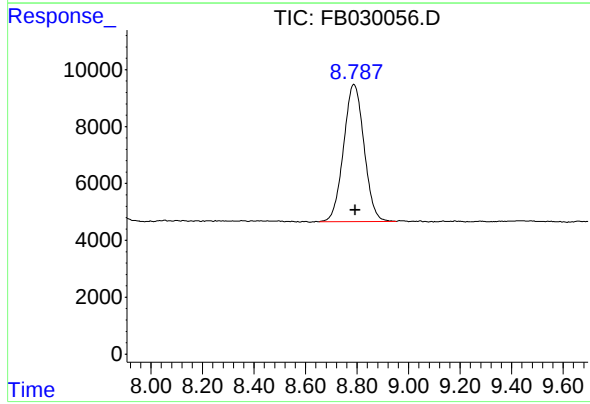

#5 AAA-TFT

R.T.: 8.788 min
Delta R.T.: -0.005 min
Response: 266155
Conc: 19.13 ng/ml