

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
 Data File : FB030024.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jun 2023 10:55
 Operator : YP/AJ
 Sample : BSF0616S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0616S1

Integration File: Calibration.e
 Quant Time: Jun 17 02:27:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	284035	20.416 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	573150	30.335 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	573053	30.370 ng/ml
3) t n-Heptane	7.747	189368	9.783 ng/ml
4) t Benzene	7.883	236991	10.587 ng/ml
6) t Toluene	10.616	671305	30.931 ng/ml
7) t Ethylbenzene	13.052	210711	10.421 ng/ml
8) t m-Xylene	13.186	419954	20.882 ng/ml
9) t O-Xylene	13.912	407752	20.921 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	392635	20.963 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030024.D
Signal(s) : FID2B.CH
Acq On : 16 Jun 2023 10:55
Operator : YP/AJ
Sample : BSF0616S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0616S1

Integration File: Calibration.e
Quant Time: Jun 17 02:27:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

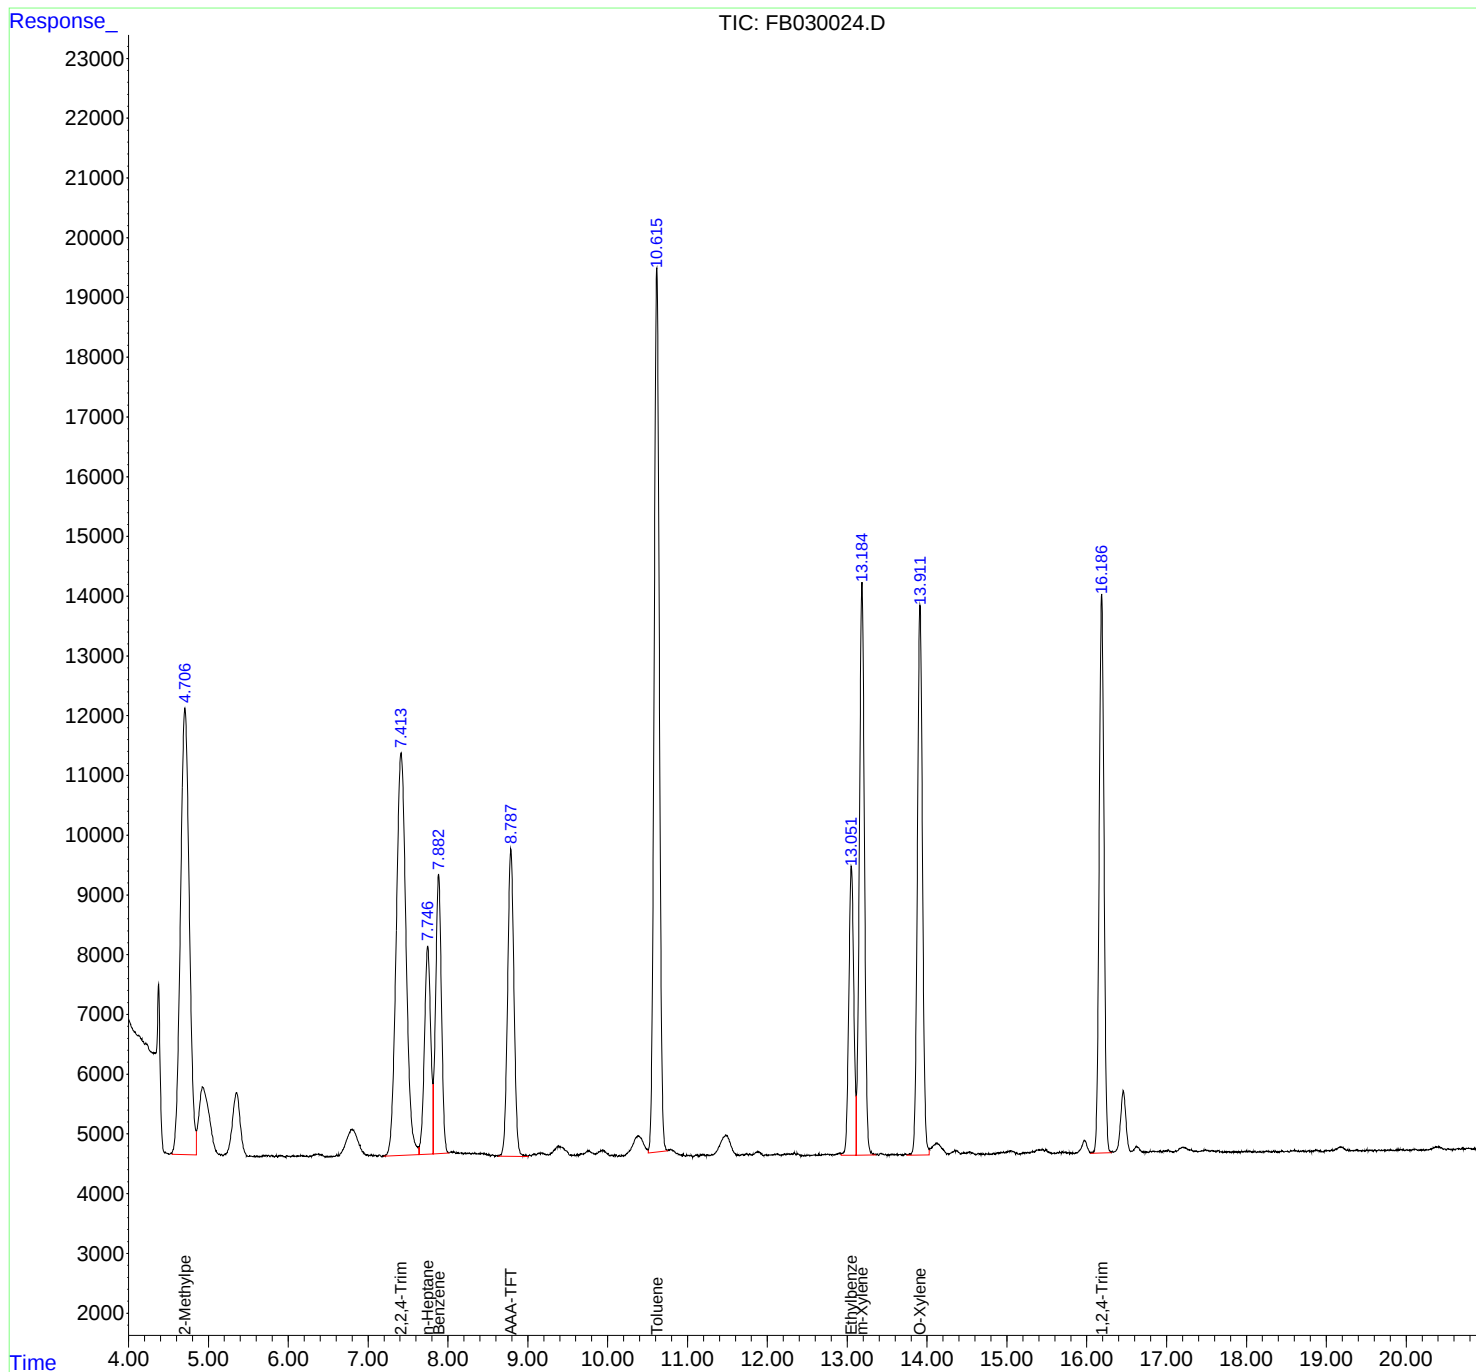


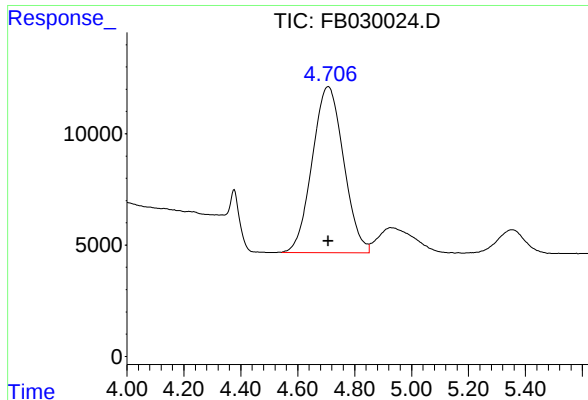

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 573150
Conc: 30.34 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S1

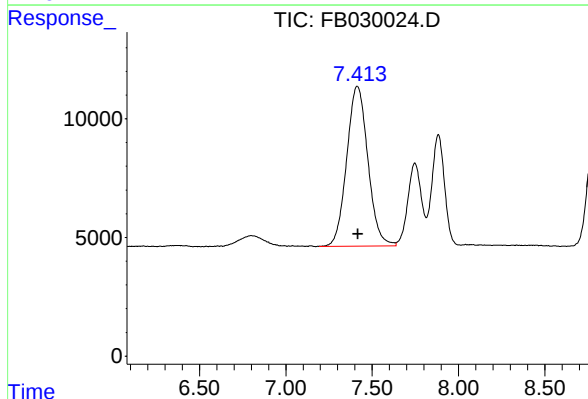


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.005 min
Response: 573053
Conc: 30.37 ng/ml

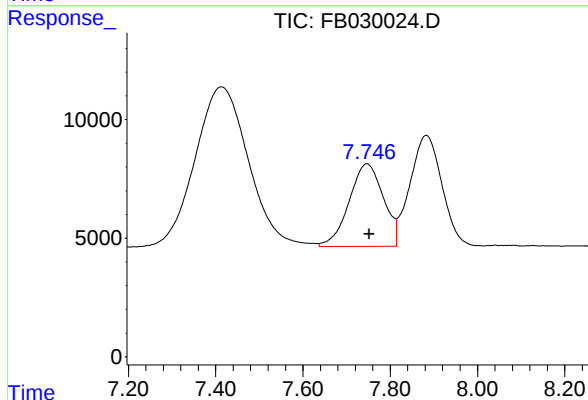


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.005 min
Response: 189368
Conc: 9.78 ng/ml

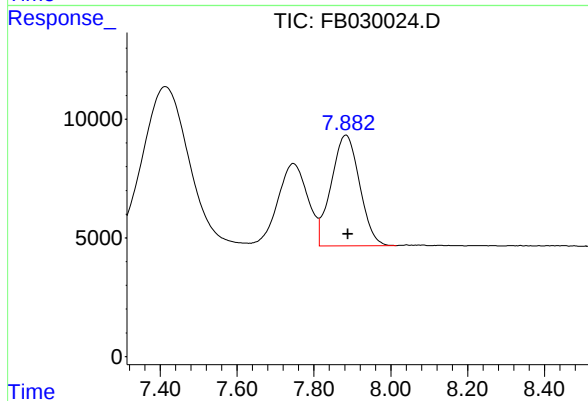

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.005 min
Response: 236991
Conc: 10.59 ng/ml

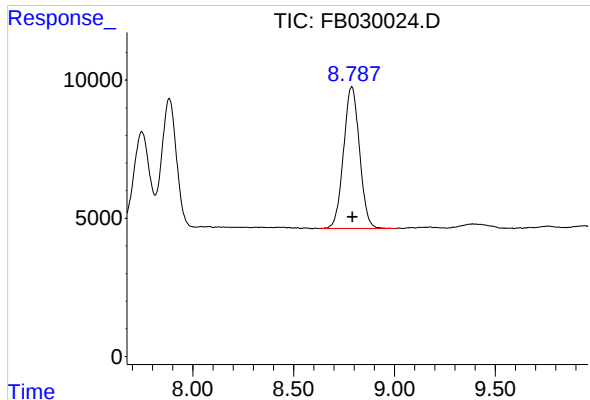

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 284035
Conc: 20.42 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S1

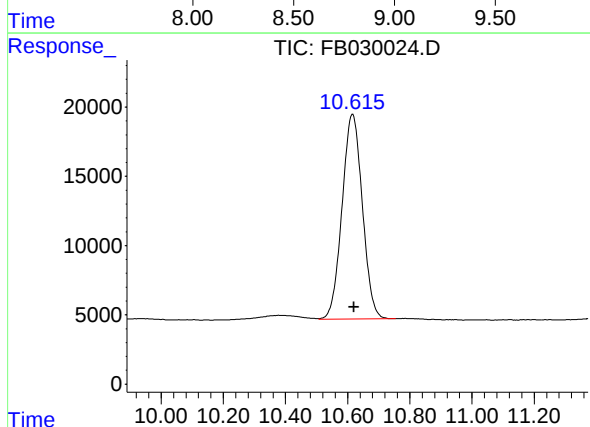


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 671305
Conc: 30.93 ng/ml

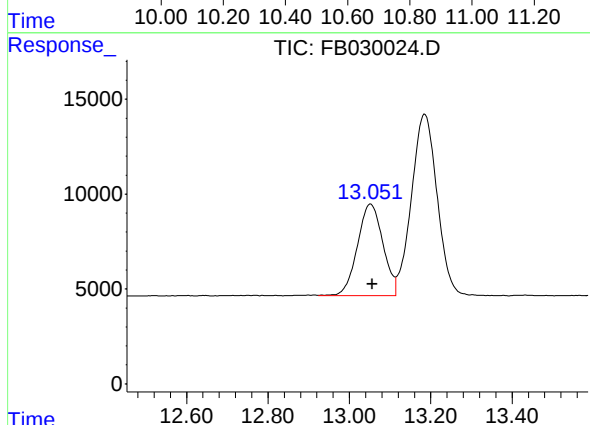


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 210711
Conc: 10.42 ng/ml

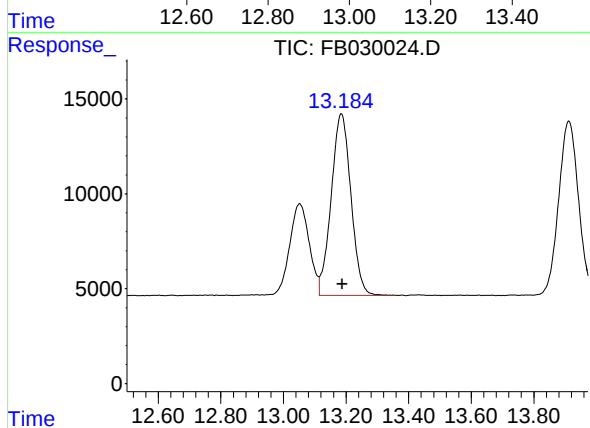

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.004 min
Response: 419954
Conc: 20.88 ng/ml

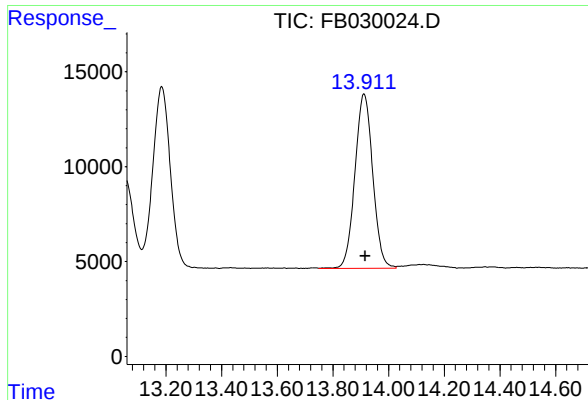

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 407752
Conc: 20.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S1

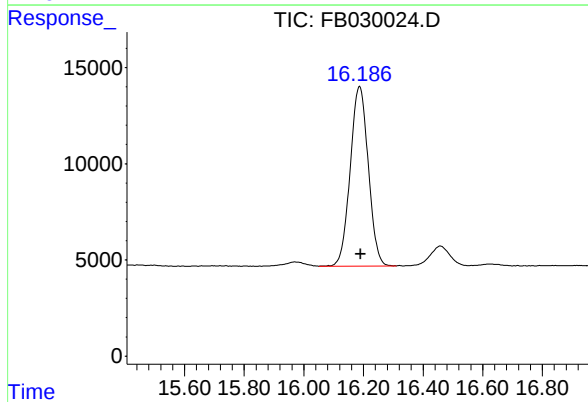

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.003 min
Response: 392635
Conc: 20.96 ng/ml