

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
 Data File : FB030029.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jun 2023 14:06
 Operator : YP/AJ
 Sample : BSF0616S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0616S2

Integration File: Calibration.e
 Quant Time: Jun 17 02:27:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	264659	19.023 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	573072	30.331 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	557714	29.557 ng/ml
3) t n-Heptane	7.750	191710	9.904 ng/ml
4) t Benzene	7.886	236353	10.559 ng/ml
6) t Toluene	10.617	686853	31.648 ng/ml
7) t Ethylbenzene	13.054	214382	10.602 ng/ml
8) t m-Xylene	13.187	426223	21.194 ng/ml
9) t O-Xylene	13.914	408715	20.970 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	387253	20.675 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030029.D
Signal(s) : FID2B.CH
Acq On : 16 Jun 2023 14:06
Operator : YP/AJ
Sample : BSF0616S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0616S2

Integration File: Calibration.e
Quant Time: Jun 17 02:27:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

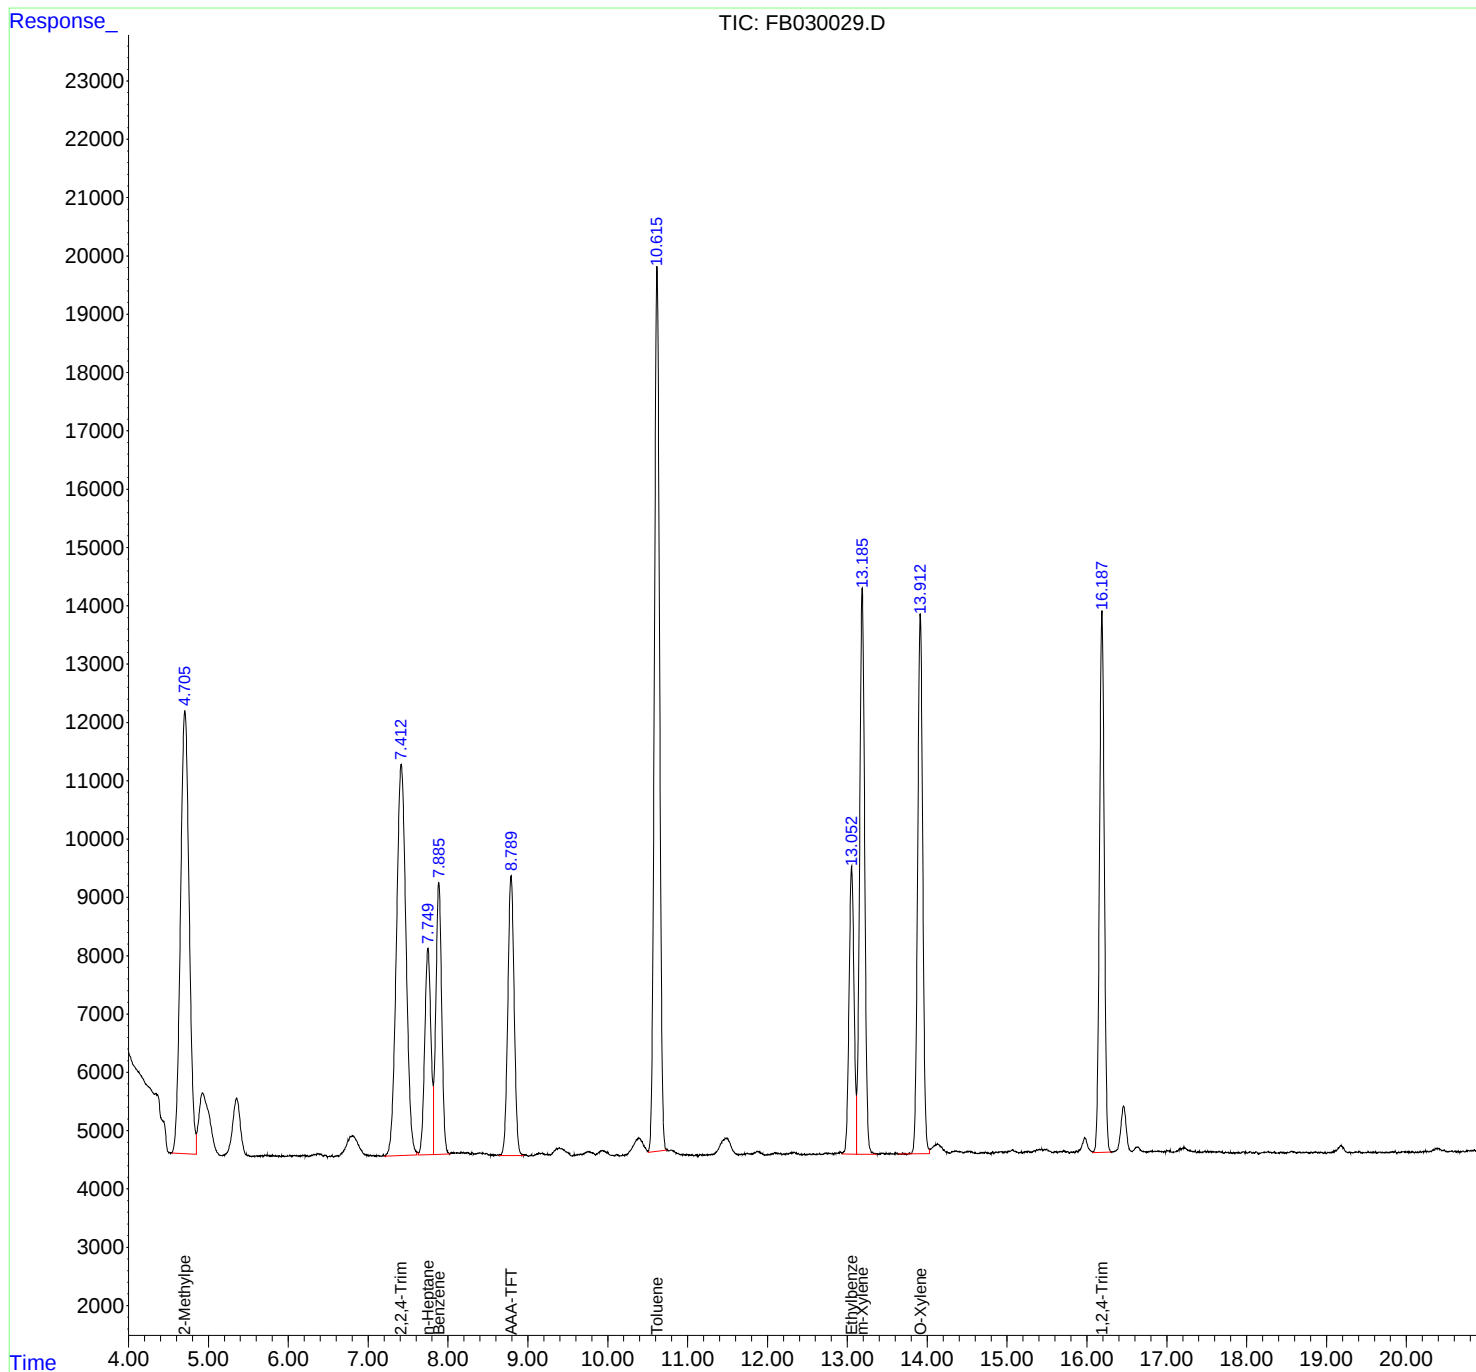


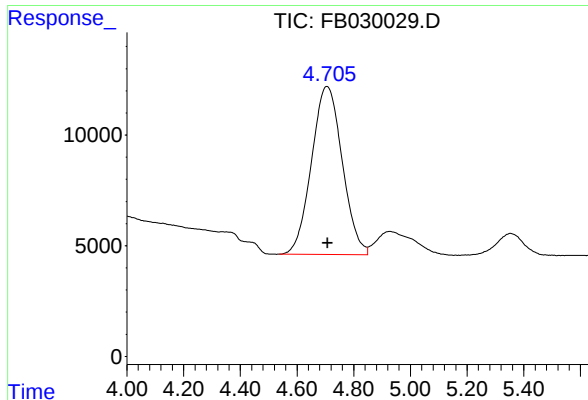

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.002 min
Response: 573072
Conc: 30.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S2

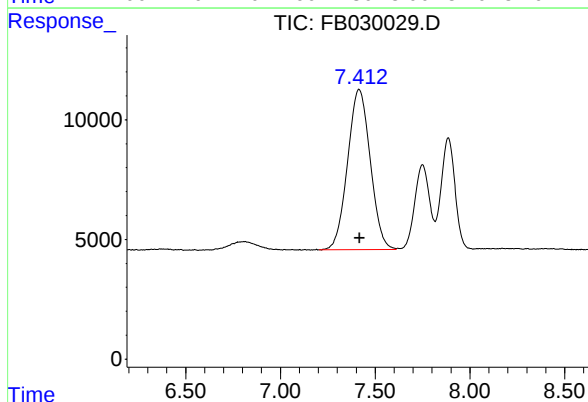


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.005 min
Response: 557714
Conc: 29.56 ng/ml

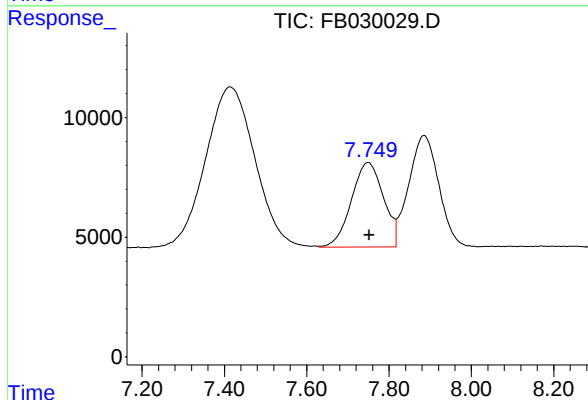


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 191710
Conc: 9.90 ng/ml

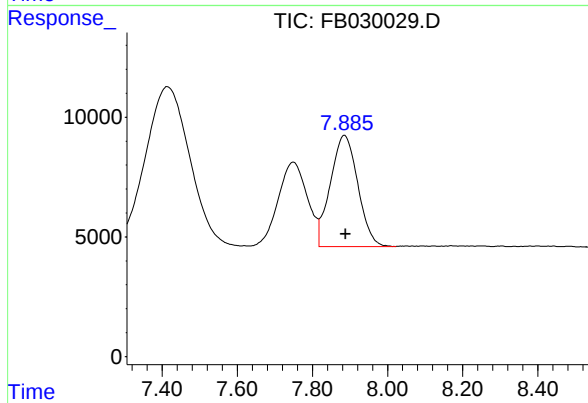

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 236353
Conc: 10.56 ng/ml

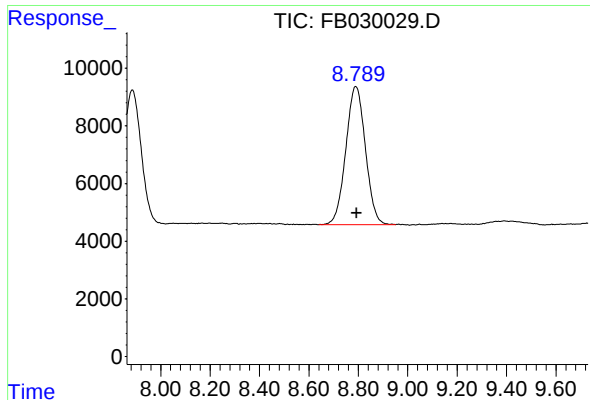

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 264659
Conc: 19.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S2

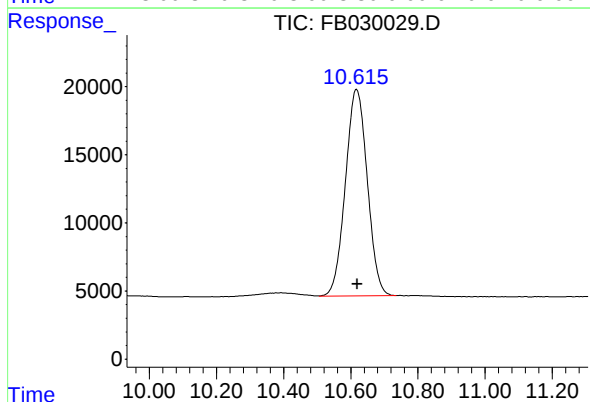


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.003 min
Response: 686853
Conc: 31.65 ng/ml

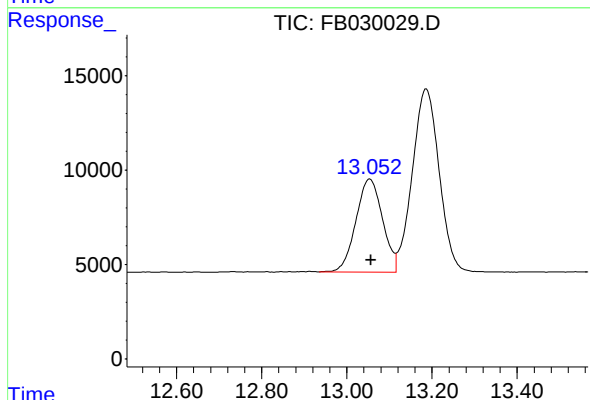


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.003 min
Response: 214382
Conc: 10.60 ng/ml

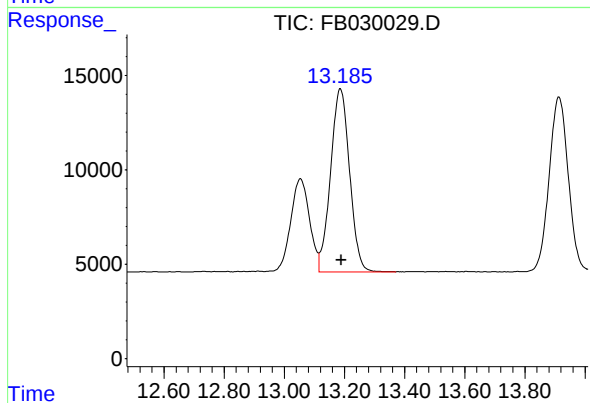

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 426223
Conc: 21.19 ng/ml

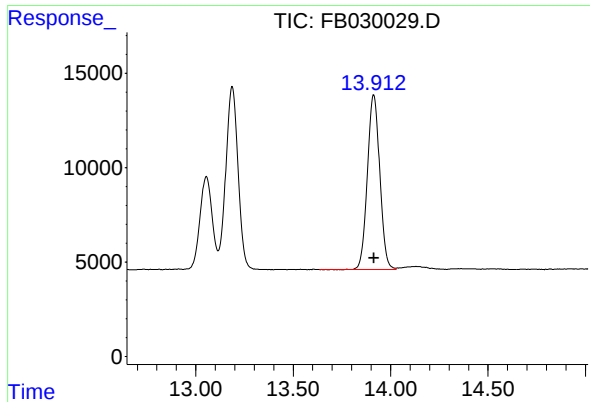

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.002 min
Response: 408715
Conc: 20.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S2

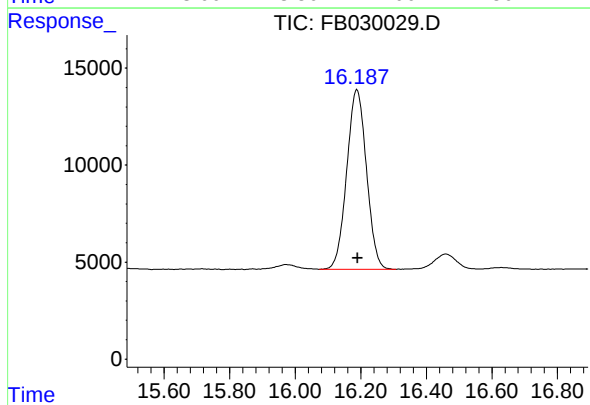

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.002 min
Response: 387253
Conc: 20.68 ng/ml