

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030032.D
Signal(s) : FID2B.CH
Acq On : 16 Jun 2023 16:40
Operator : YP/AJ
Sample : 03289-06
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-02-COMP

Integration File: Calibration.e
Quant Time: Jun 17 02:28:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	220715	15.864 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030032.D
Signal(s) : FID2B.CH
Acq On : 16 Jun 2023 16:40
Operator : YP/AJ
Sample : 03289-06
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-02-COMP

Integration File: Calibration.e
Quant Time: Jun 17 02:28:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

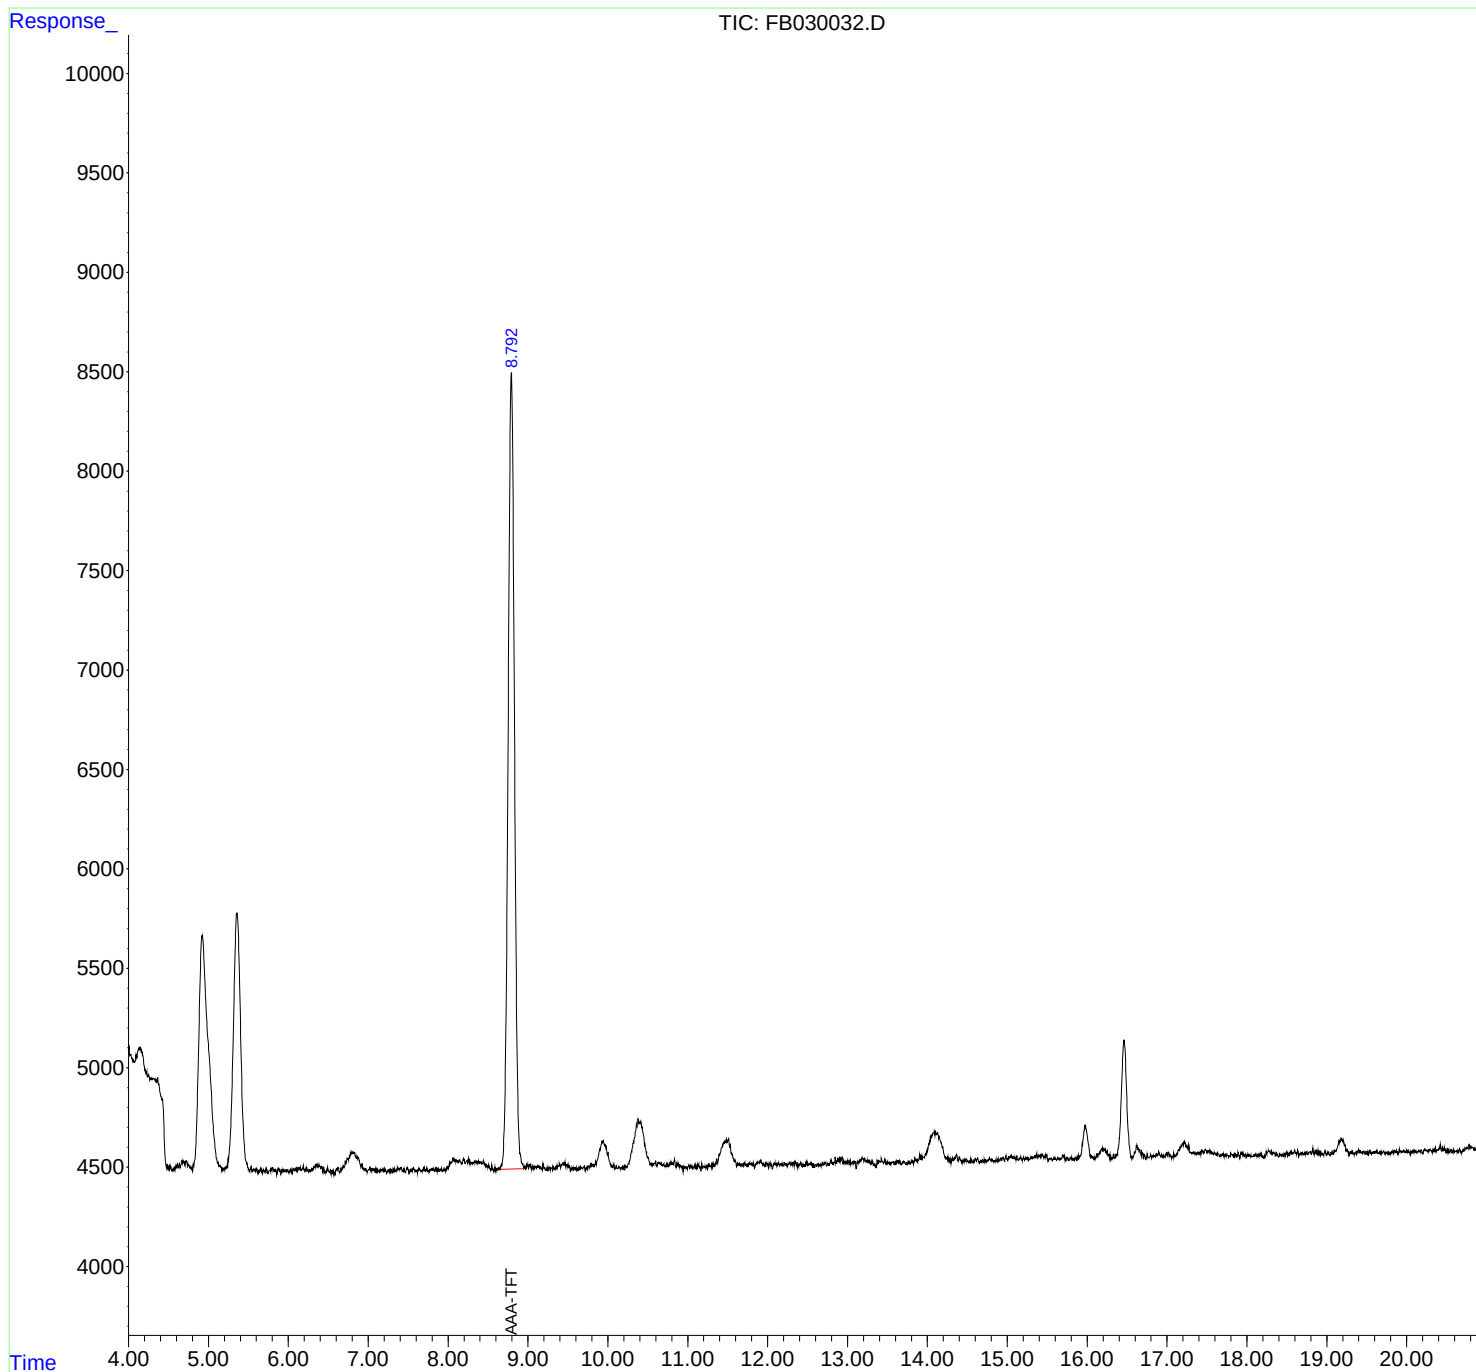

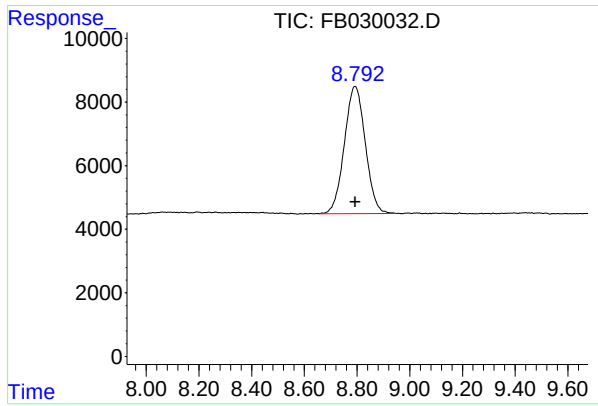

#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 220715
Conc: 15.86 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-02-COMP