

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
 Data File : FB030051.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jun 2023 5:28
 Operator : YP/AJ
 Sample : 03289-24MSD 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-08-COMPMSD

Integration File: Calibration.e
 Quant Time: Jun 17 06:29:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	252067	18.118 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	511280	27.061 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	552541	29.283 ng/ml
3) t n-Heptane	7.744	184005	9.506 ng/ml
4) t Benzene	7.881	251422	11.232 ng/ml
6) t Toluene	10.615	715093	32.949 ng/ml
7) t Ethylbenzene	13.052	220737	10.917 ng/ml
8) t m-Xylene	13.184	440764	21.917 ng/ml
9) t O-Xylene	13.911	429174	22.020 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	398666	21.285 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030051.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2023 5:28
Operator : YP/AJ
Sample : 03289-24MSD 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

Integration File: Calibration.e
Quant Time: Jun 17 06:29:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

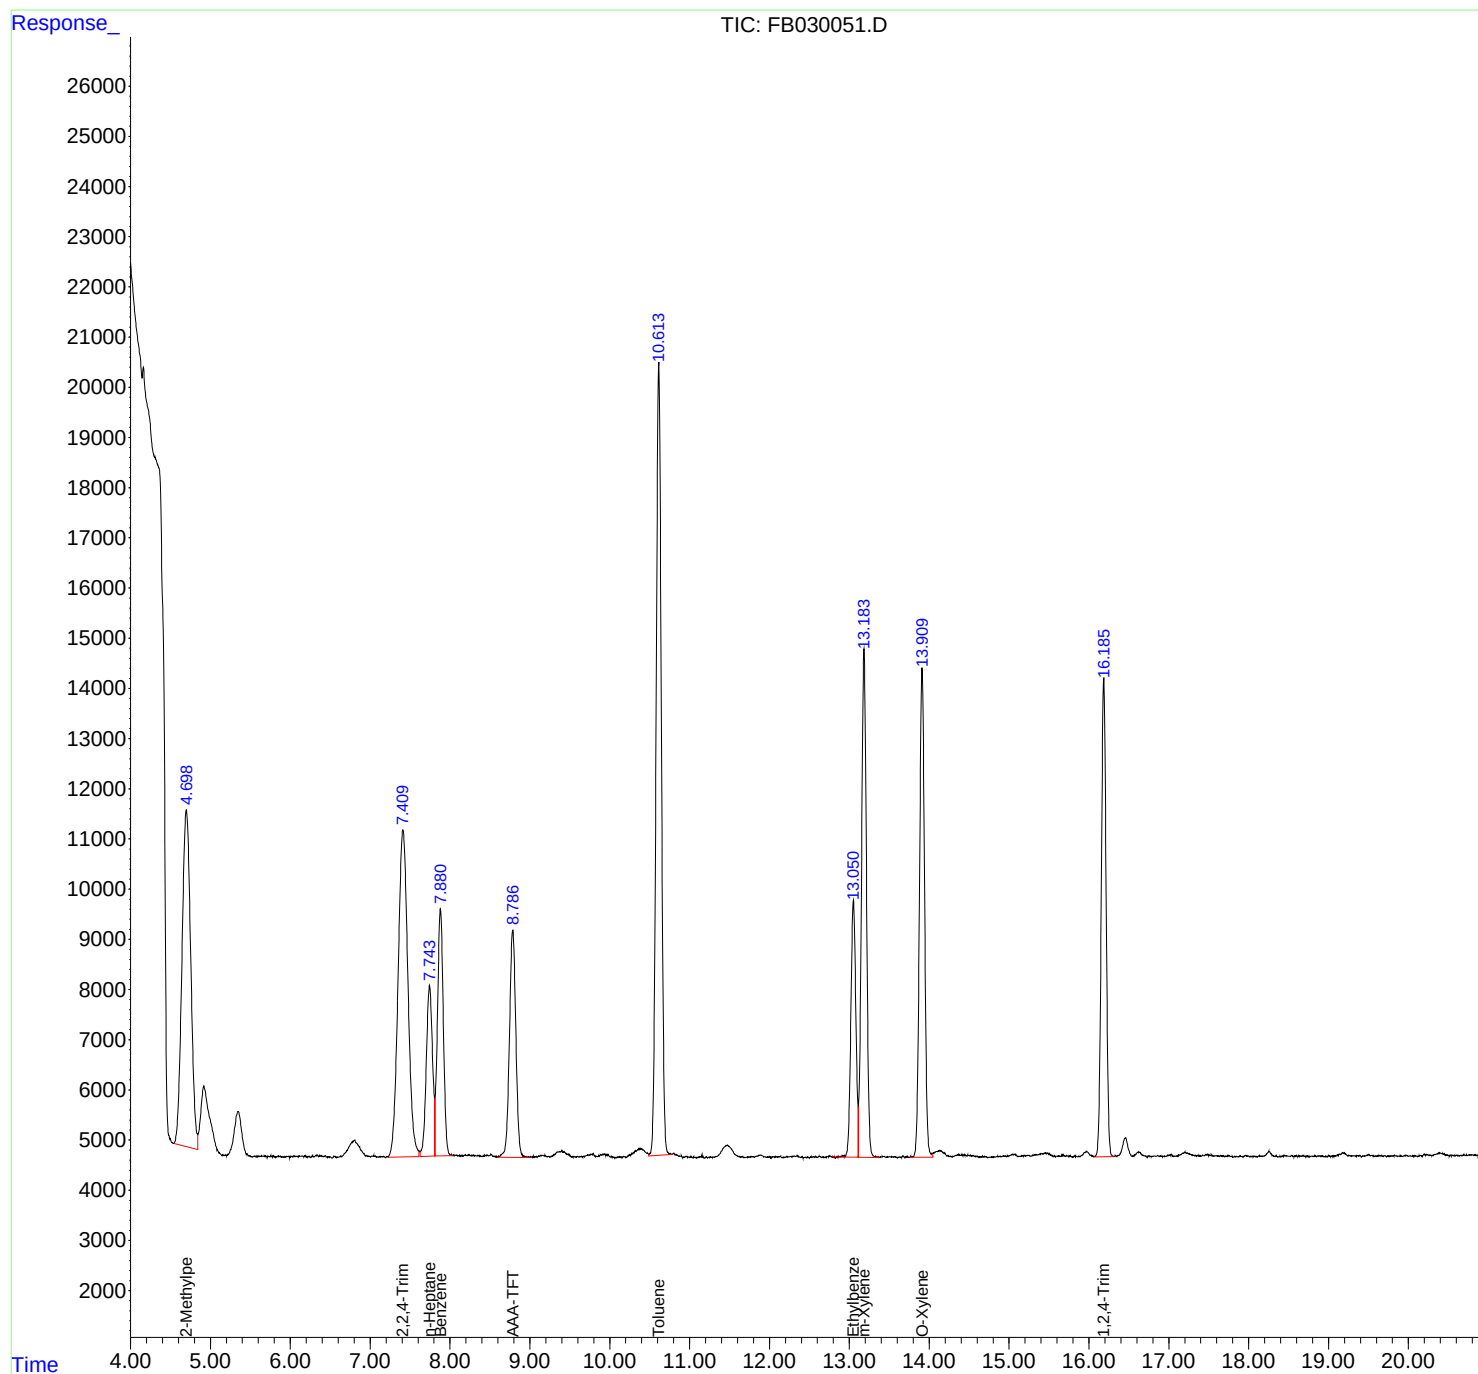


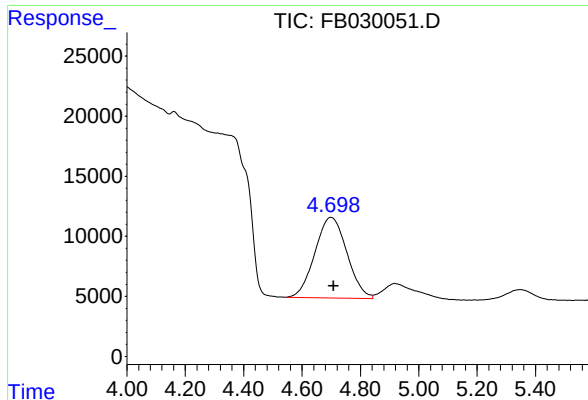

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.009 min
Response: 511280
Conc: 27.06 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

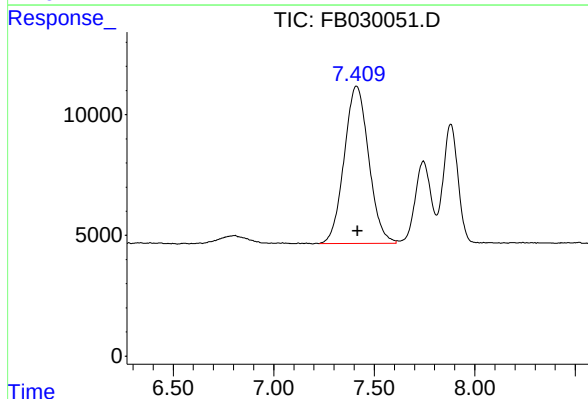


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.008 min
Response: 552541
Conc: 29.28 ng/ml

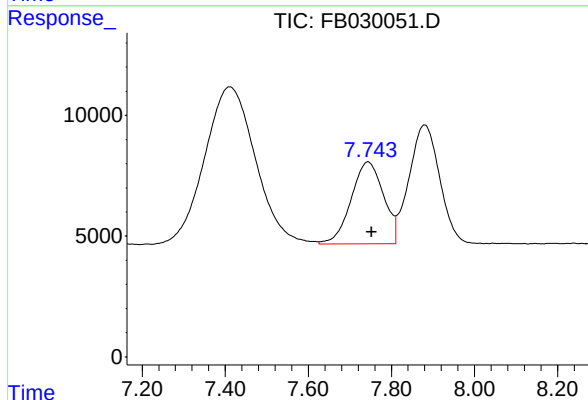


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.008 min
Response: 184005
Conc: 9.51 ng/ml

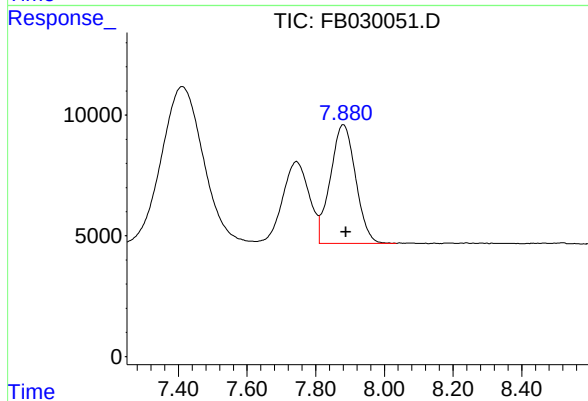

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.008 min
Response: 251422
Conc: 11.23 ng/ml

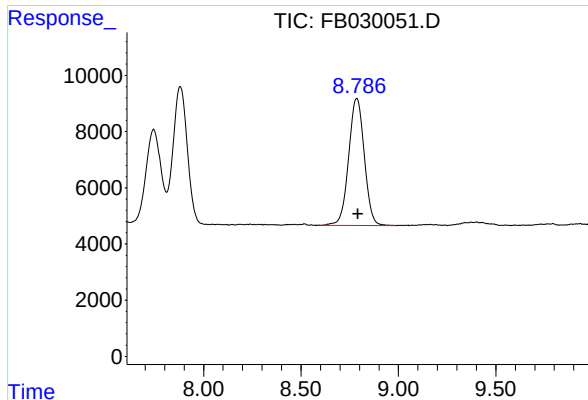

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 252067
Conc: 18.12 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

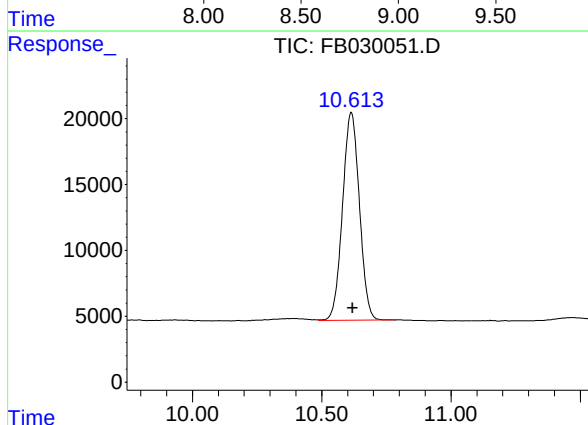


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.006 min
Response: 715093
Conc: 32.95 ng/ml

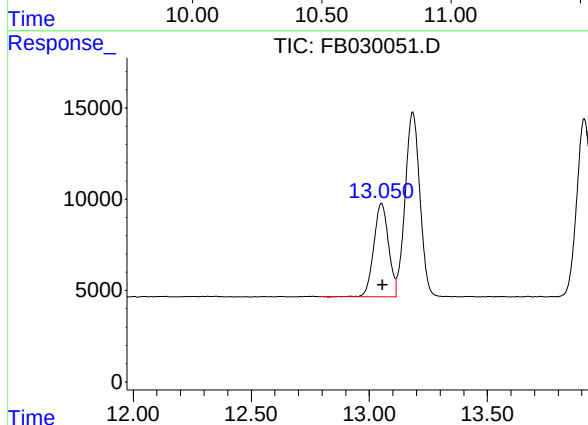


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.005 min
Response: 220737
Conc: 10.92 ng/ml

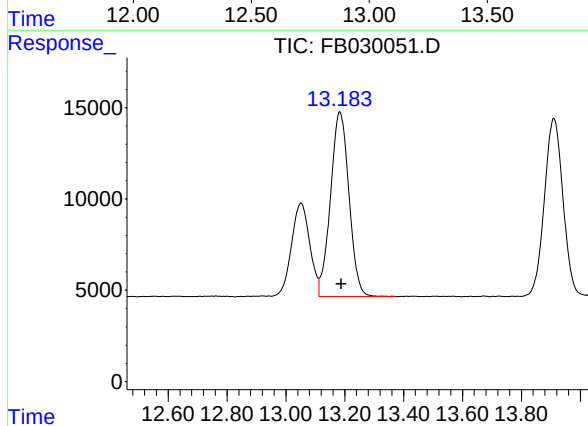

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.005 min
Response: 440764
Conc: 21.92 ng/ml

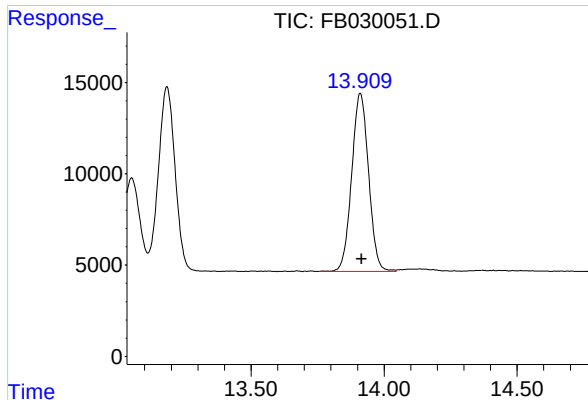

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.005 min
Response: 429174
Conc: 22.02 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

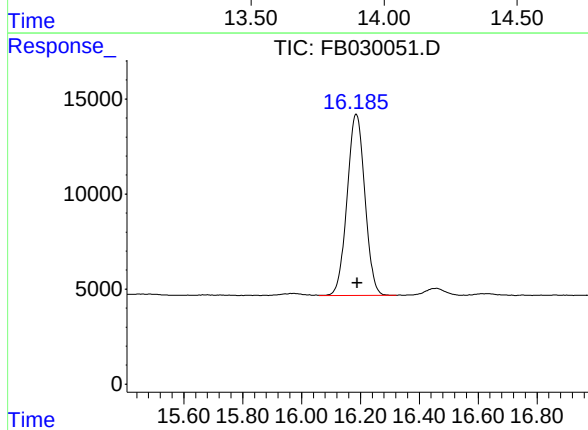

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.004 min
Response: 398666
Conc: 21.28 ng/ml