

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
 Data File : FB030061.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jun 2023 13:02
 Operator : YP/AJ
 Sample : BSF0616S4
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0616S4

Integration File: Calibration.e
 Quant Time: Jun 19 01:41:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	225107	16.180 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	548707	29.042 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	532656	28.229 ng/ml
3) t n-Heptane	7.747	184575	9.536 ng/ml
4) t Benzene	7.883	233233	10.420 ng/ml
6) t Toluene	10.616	677770	31.229 ng/ml
7) t Ethylbenzene	13.052	211998	10.484 ng/ml
8) t m-Xylene	13.185	418047	20.788 ng/ml
9) t O-Xylene	13.912	407337	20.899 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	388723	20.754 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061623\
Data File : FB030061.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2023 13:02
Operator : YP/AJ
Sample : BSF0616S4
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0616S4

Integration File: Calibration.e
Quant Time: Jun 19 01:41:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

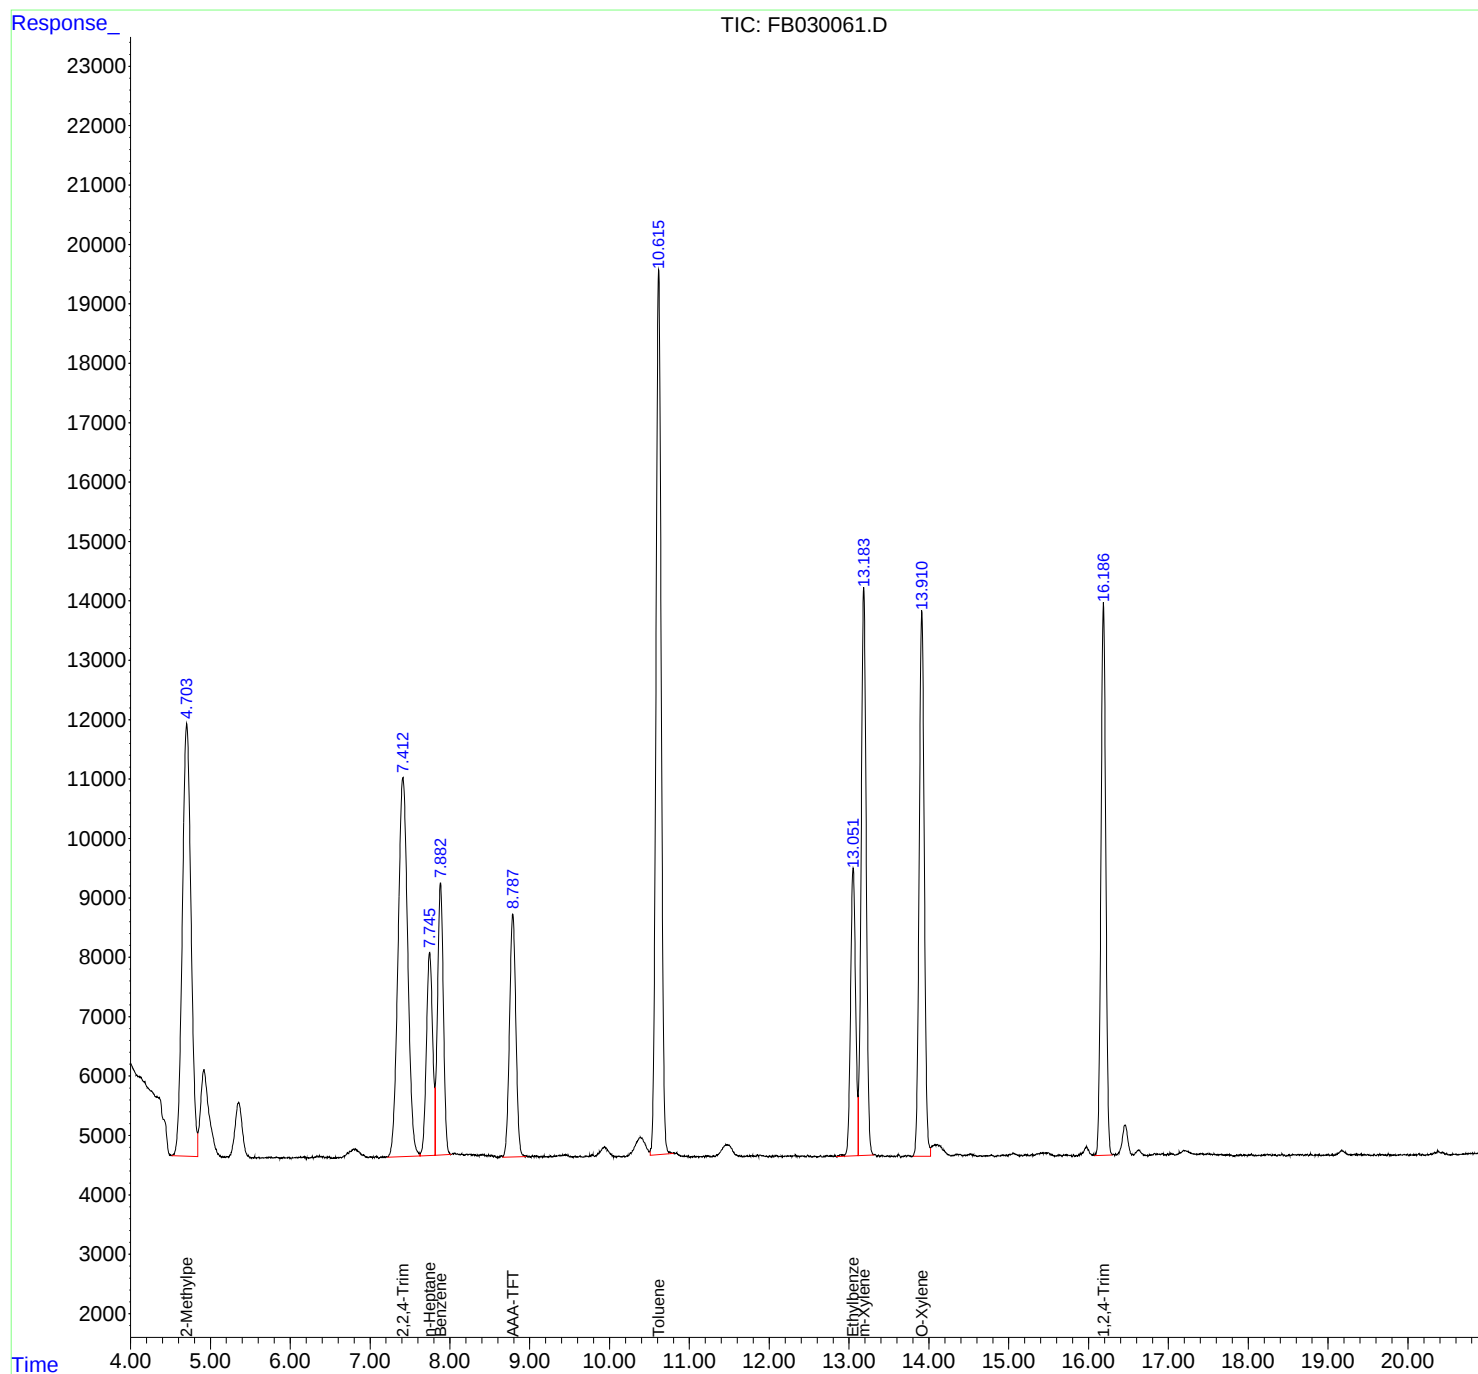


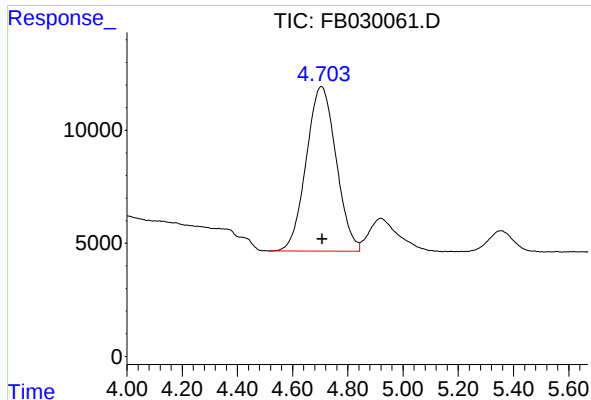

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.004 min
Response: 548707
Conc: 29.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S4

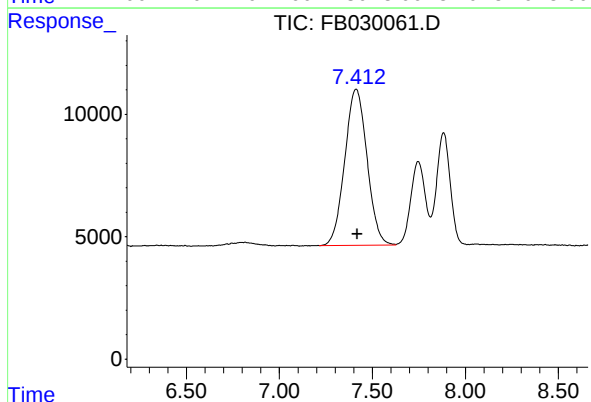


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.005 min
Response: 532656
Conc: 28.23 ng/ml

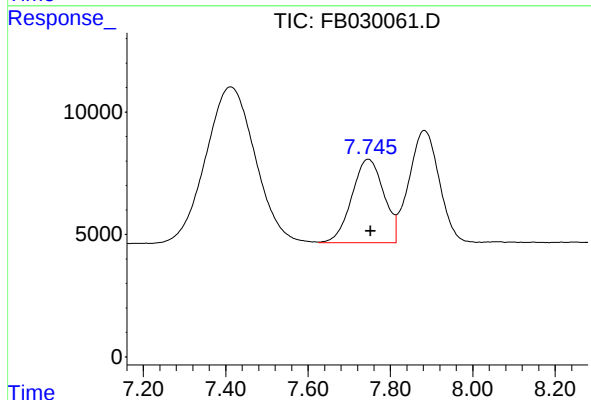


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.005 min
Response: 184575
Conc: 9.54 ng/ml

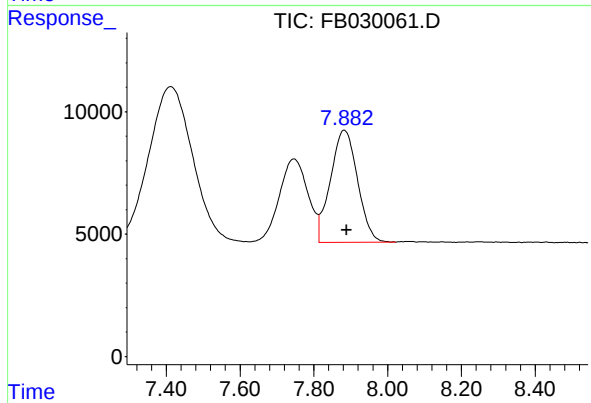

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.006 min
Response: 233233
Conc: 10.42 ng/ml

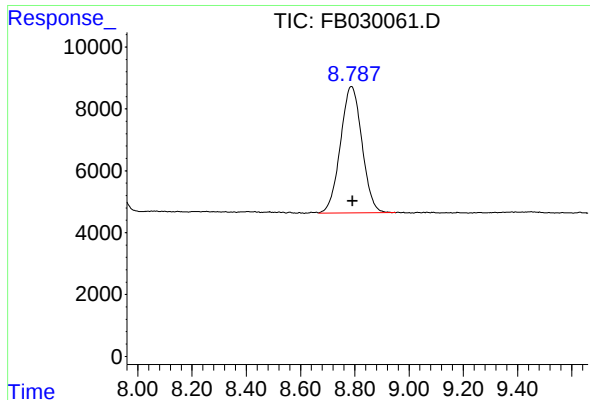

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 225107
Conc: 16.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S4

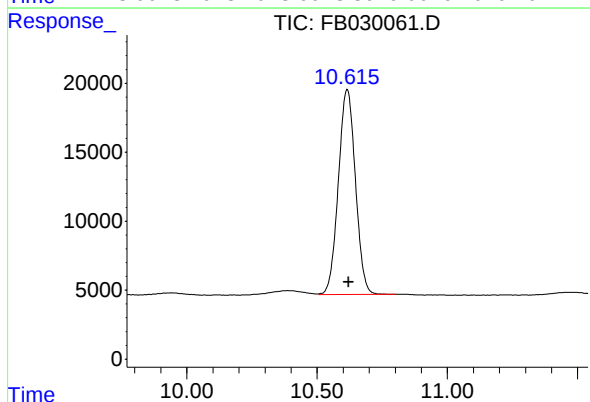


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 677770
Conc: 31.23 ng/ml

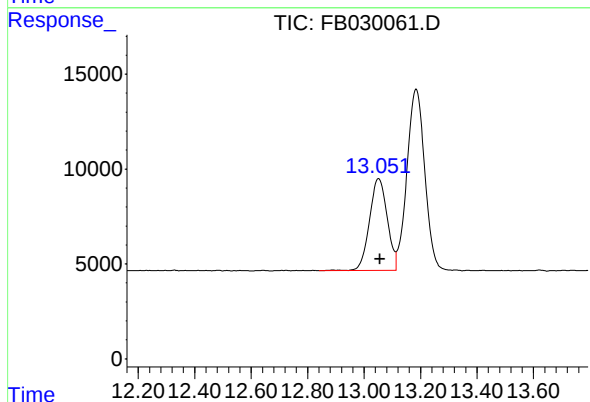


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.005 min
Response: 211998
Conc: 10.48 ng/ml

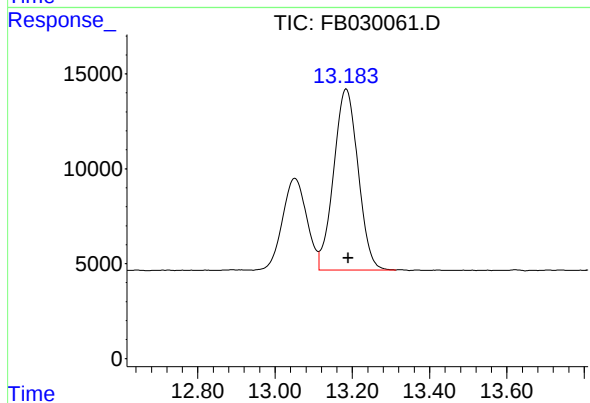

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.004 min
Response: 418047
Conc: 20.79 ng/ml

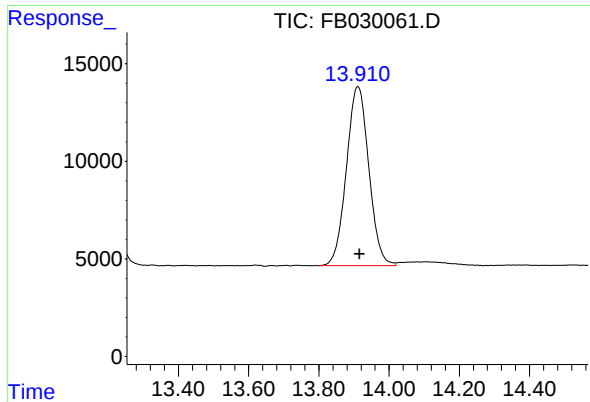

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 407337
Conc: 20.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0616S4

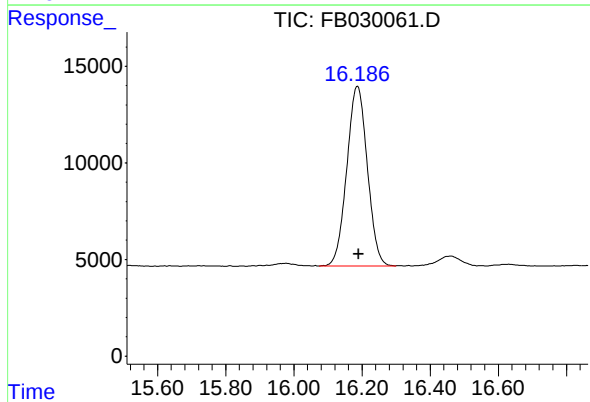

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.003 min
Response: 388723
Conc: 20.75 ng/ml