

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061720\
Data File : FB024472.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2020 16:16
Operator : DD/AJ
Sample : L2812-07
Misc : 5.05gm/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 18 03:22:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	501443	20.726 ng/ml
Target Compounds				
7) t	Ethylbenzene	13.061	2435	0.069 ng/ml
8) t	m-Xylene	13.202	2265	0.066 ng/ml
9) t	O-Xylene	13.922	5027	0.150 ng/ml
10) t	1,2,4-Trimethylbenzene	16.202	4885	0.176 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061720\
Data File : FB024472.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2020 16:16
Operator : DD/AJ
Sample : L2812-07
Misc : 5.05gm/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 18 03:22:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

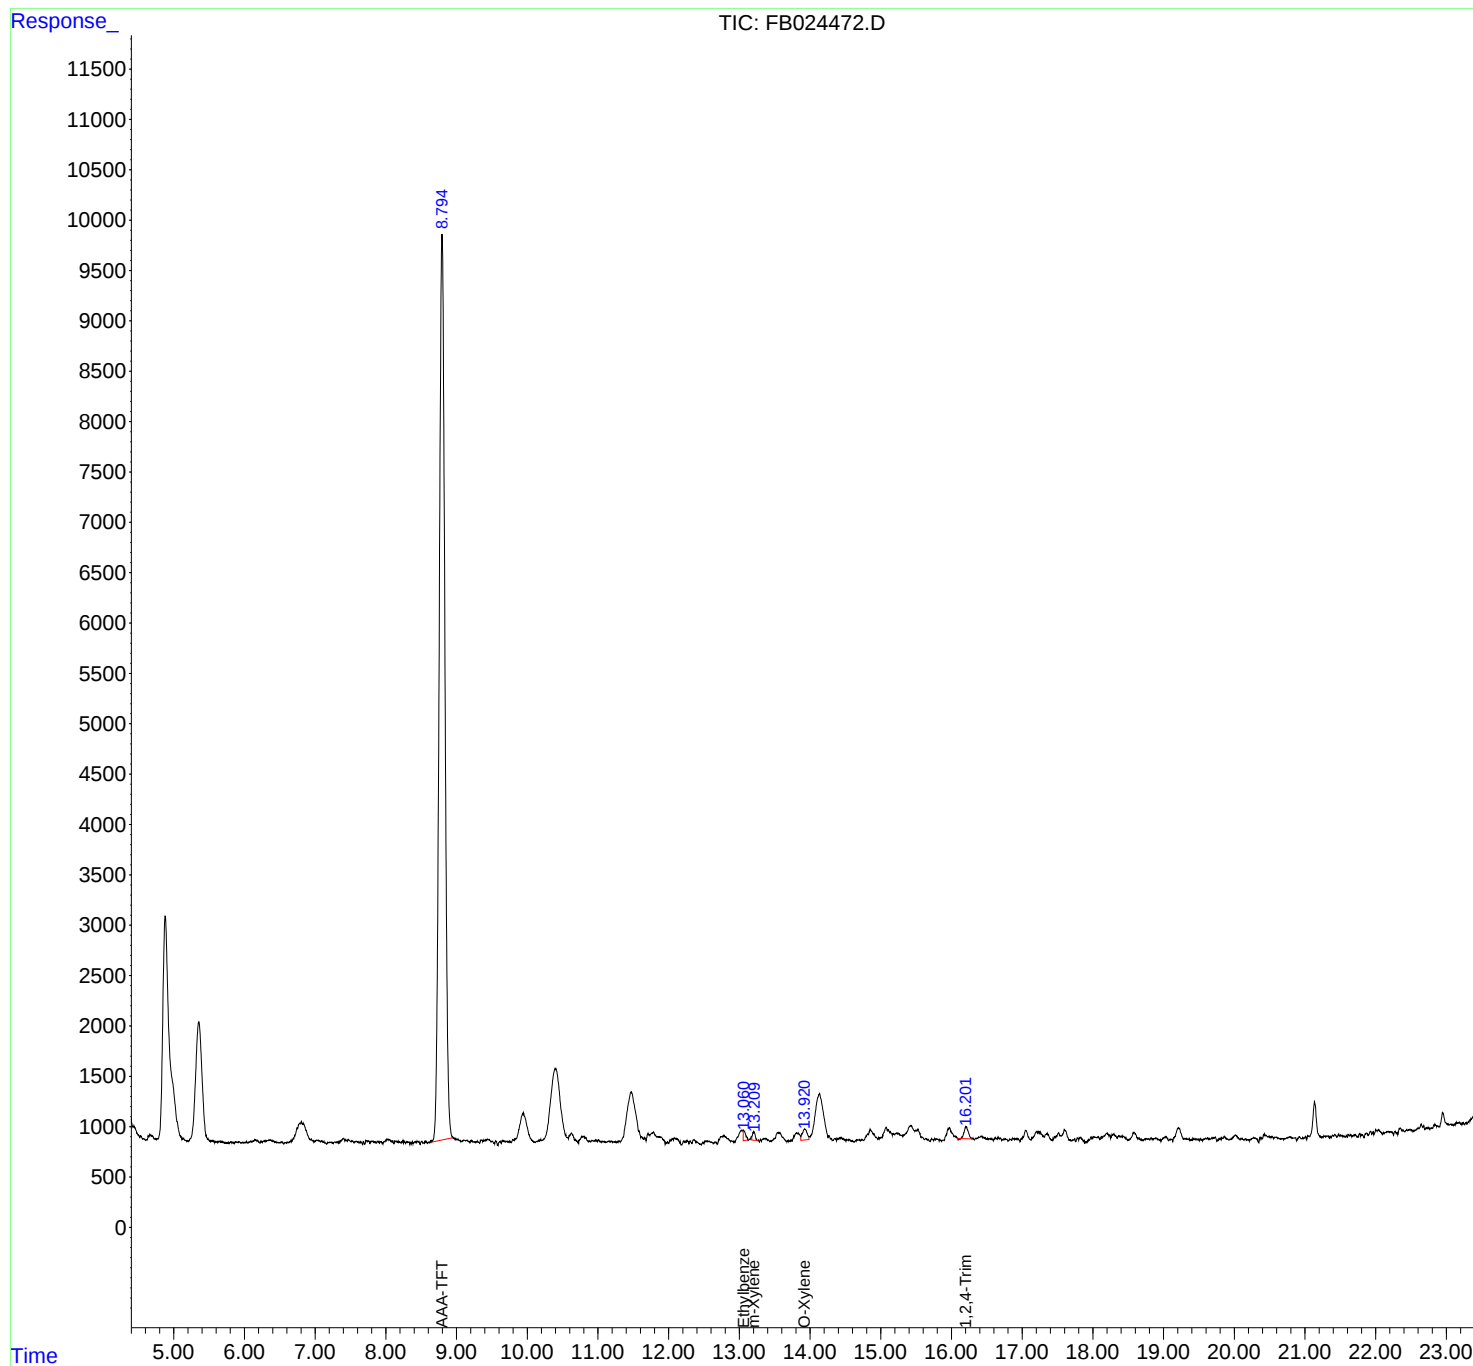

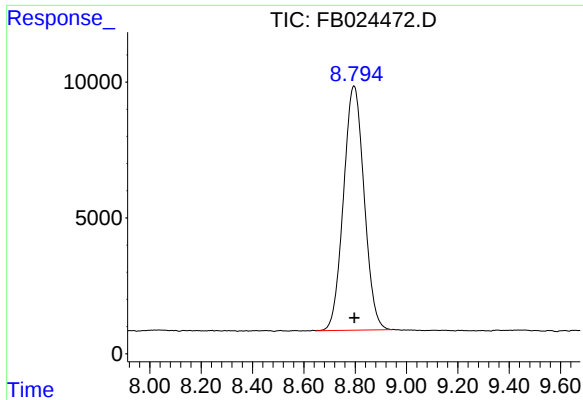


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.001 min
Response: 501443
Conc: 20.73 ng/ml

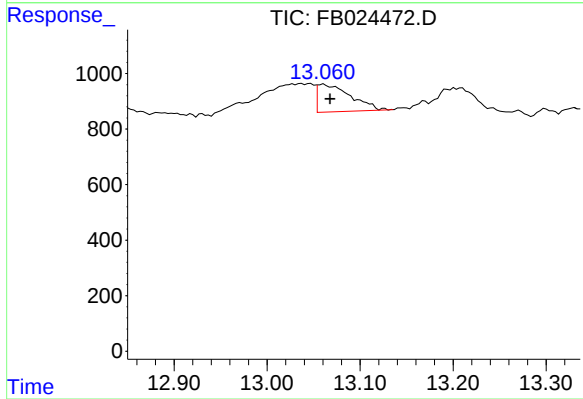


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.007 min
Response: 2435
Conc: 0.07 ng/ml

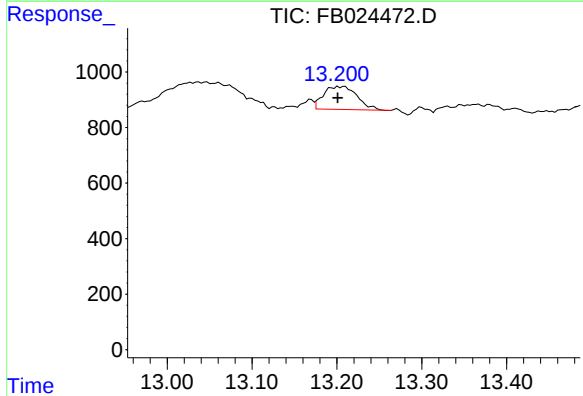


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 2265
Conc: 0.07 ng/ml

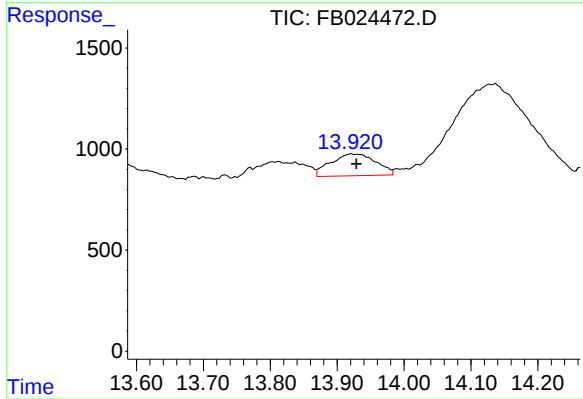

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.007 min
Response: 5027
Conc: 0.15 ng/ml

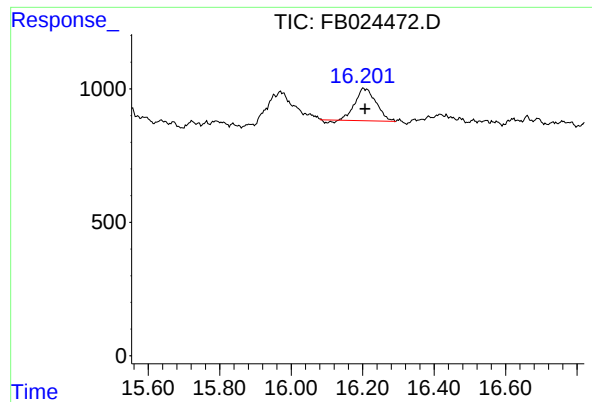

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.004 min
Response: 4885
Conc: 0.18 ng/ml