

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061720\
 Data File : FB024465.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jun 2020 9:48
 Operator : DD/AJ
 Sample : BSF0617S1
 Misc : 5.02gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 18 03:21:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.794	471490	19.488 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.686	901884	28.216 ng/ml
2) t	2,2,4-Trimethylpentane	7.414	971182	28.970 ng/ml
3) t	n-Heptane	7.753	322853	9.547 ng/ml
4) t	Benzene	7.888	381619	9.440 ng/ml
6) t	Toluene	10.626	1074566	27.344 ng/ml
7) t	Ethylbenzene	13.066	334818	9.542 ng/ml
8) t	m-Xylene	13.199	654172	19.102 ng/ml
9) t	O-Xylene	13.926	634054	18.912 ng/ml
10) t	1,2,4-Trimethylbenzene	16.203	529699	19.078 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061720\
Data File : FB024465.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2020 9:48
Operator : DD/AJ
Sample : BSF0617S1
Misc : 5.02gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 18 03:21:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

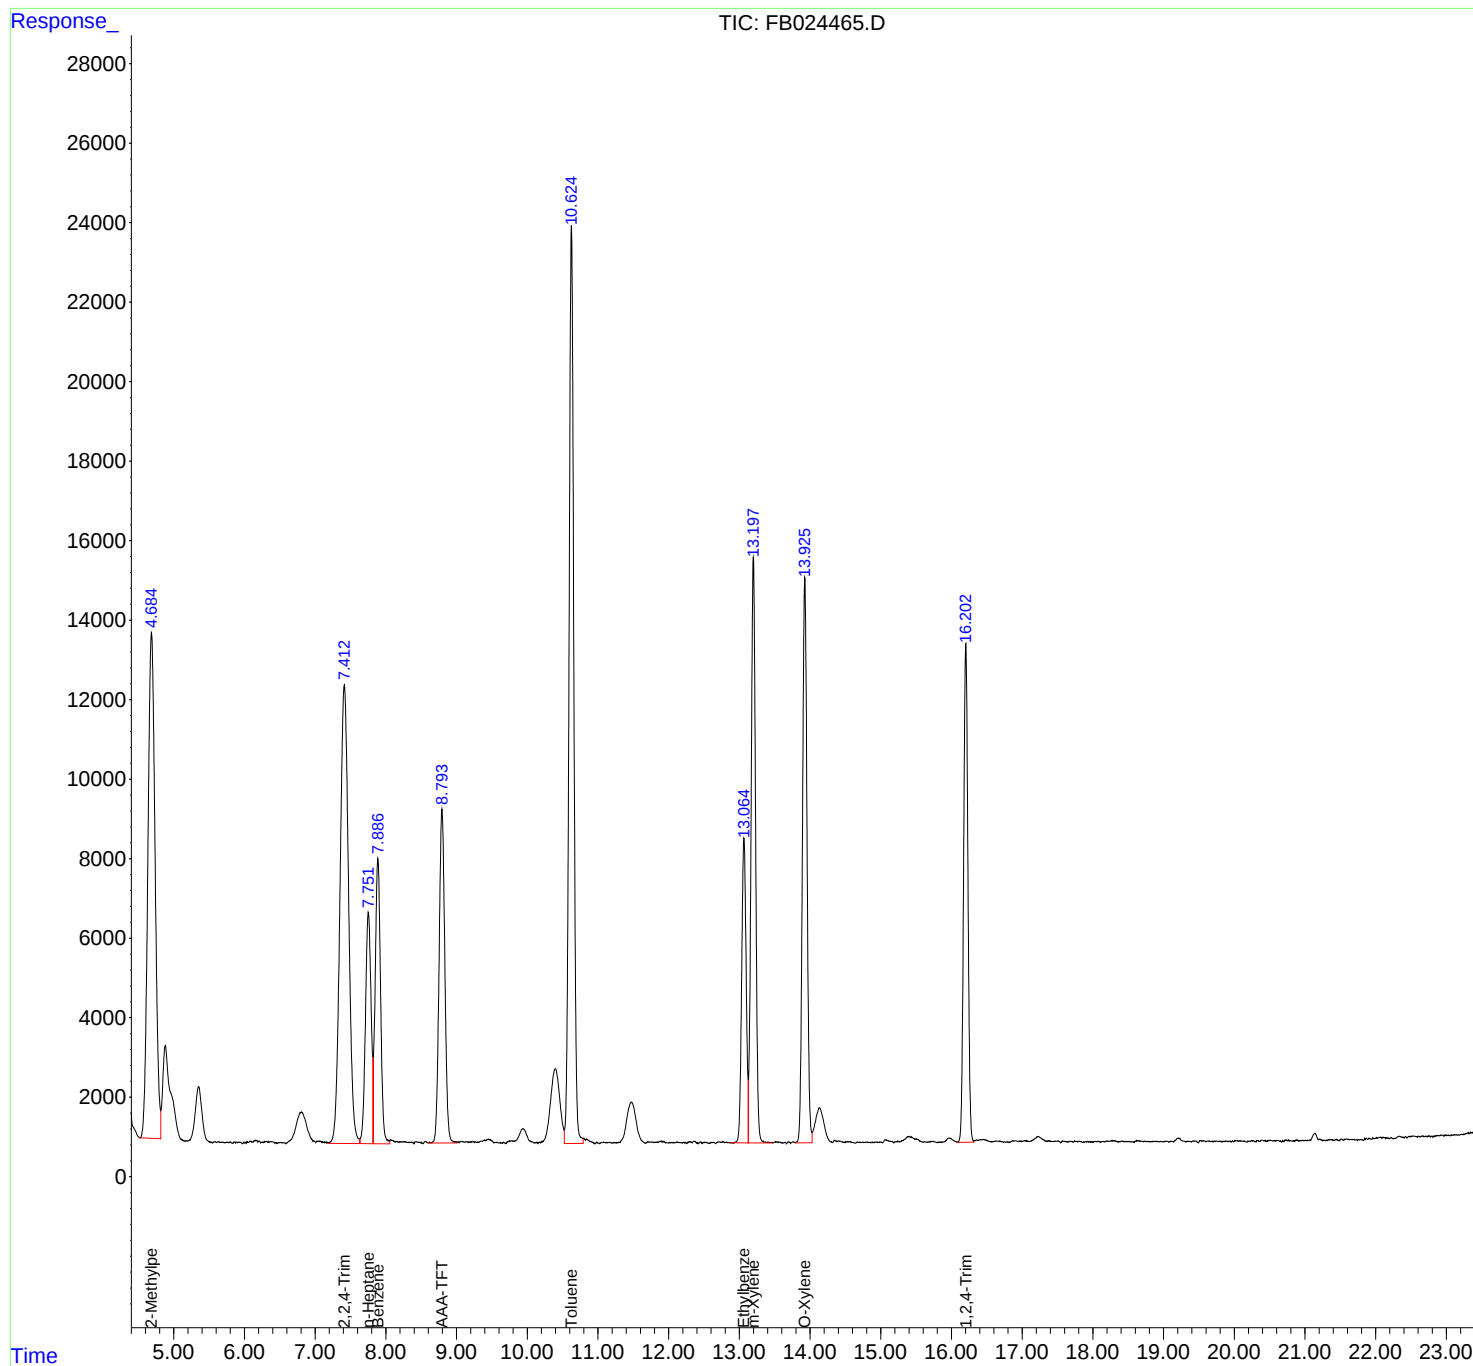

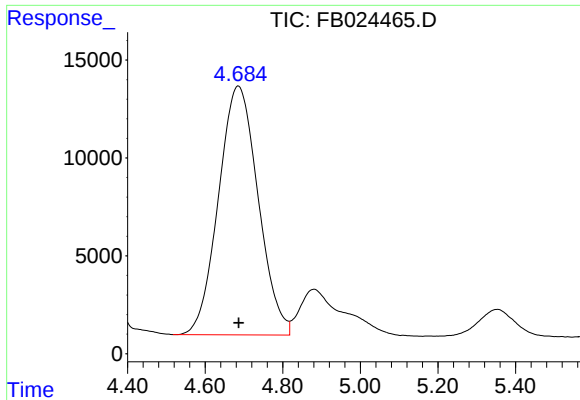


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.001 min
Response: 901884
Conc: 28.22 ng/ml

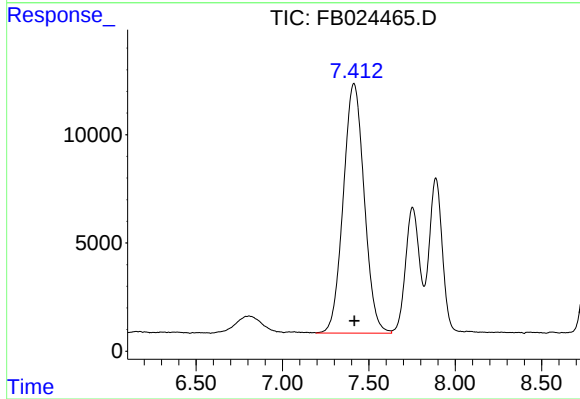


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.002 min
Response: 971182
Conc: 28.97 ng/ml

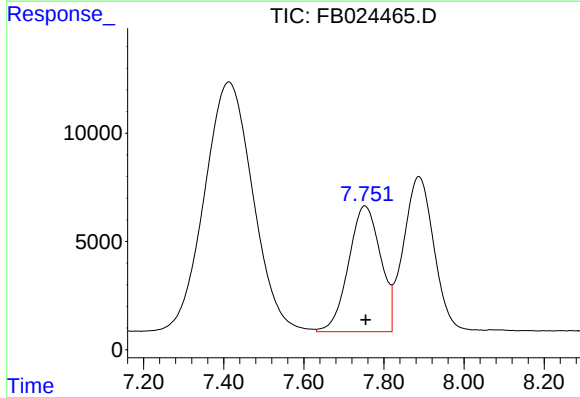


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 322853
Conc: 9.55 ng/ml

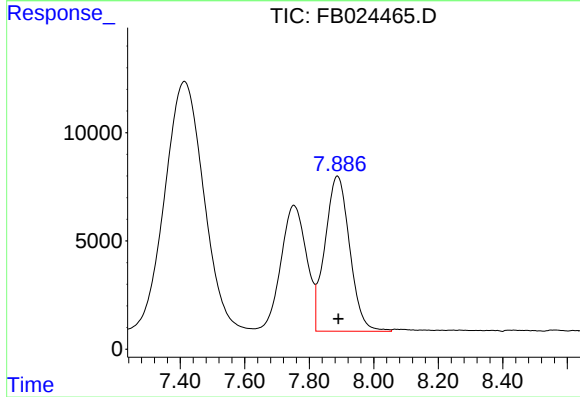


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 381619
Conc: 9.44 ng/ml

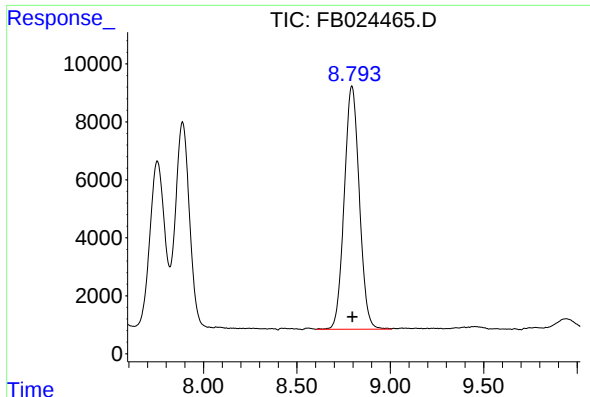


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 471490
Conc: 19.49 ng/ml

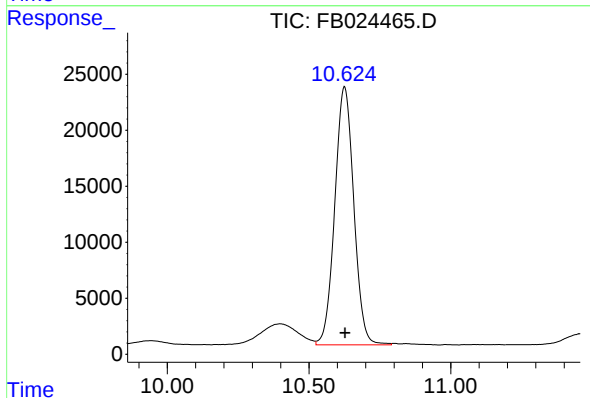


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.003 min
Response: 1074566
Conc: 27.34 ng/ml

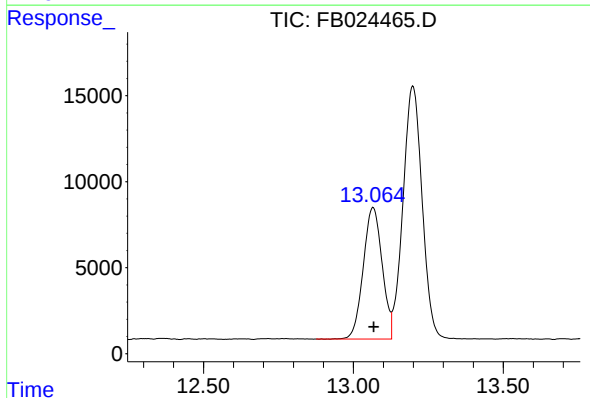


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.002 min
Response: 334818
Conc: 9.54 ng/ml

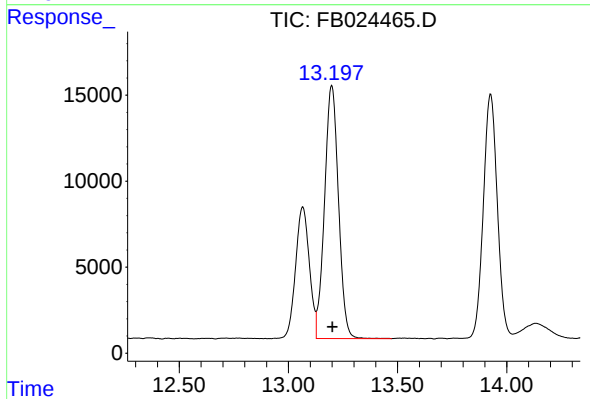

#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.002 min
Response: 654172
Conc: 19.10 ng/ml

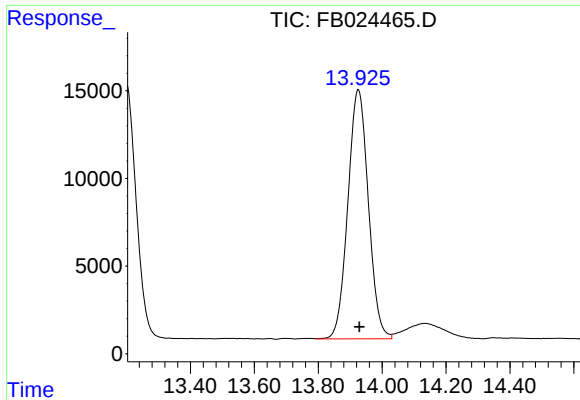


#9 O-Xylene

R.T.: 13.926 min

Delta R.T.: -0.003 min

Response: 634054

Conc: 18.91 ng/ml

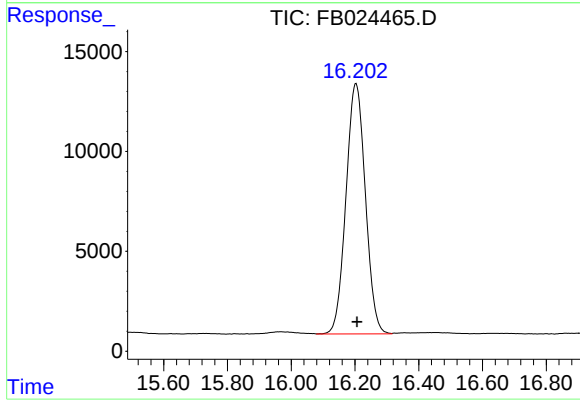

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min

Delta R.T.: -0.003 min

Response: 529699

Conc: 19.08 ng/ml