

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061720\
 Data File : FB024468.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jun 2020 11:47
 Operator : DD/AJ
 Sample : L2811-02MS
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 18 03:21:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	480450	19.858 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	835859	26.150 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	837742	24.989 ng/ml
3) t n-Heptane	7.754	279463	8.264 ng/ml
4) t Benzene	7.888	391171	9.676 ng/ml
6) t Toluene	10.626	1070738	27.246 ng/ml
7) t Ethylbenzene	13.065	324844	9.257 ng/ml
8) t m-Xylene	13.199	628178	18.343 ng/ml
9) t O-Xylene	13.926	617111	18.407 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	491644	17.707 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061720\
Data File : FB024468.D
Signal(s) : FID2B.CH
Acq On : 17 Jun 2020 11:47
Operator : DD/AJ
Sample : L2811-02MS
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 18 03:21:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

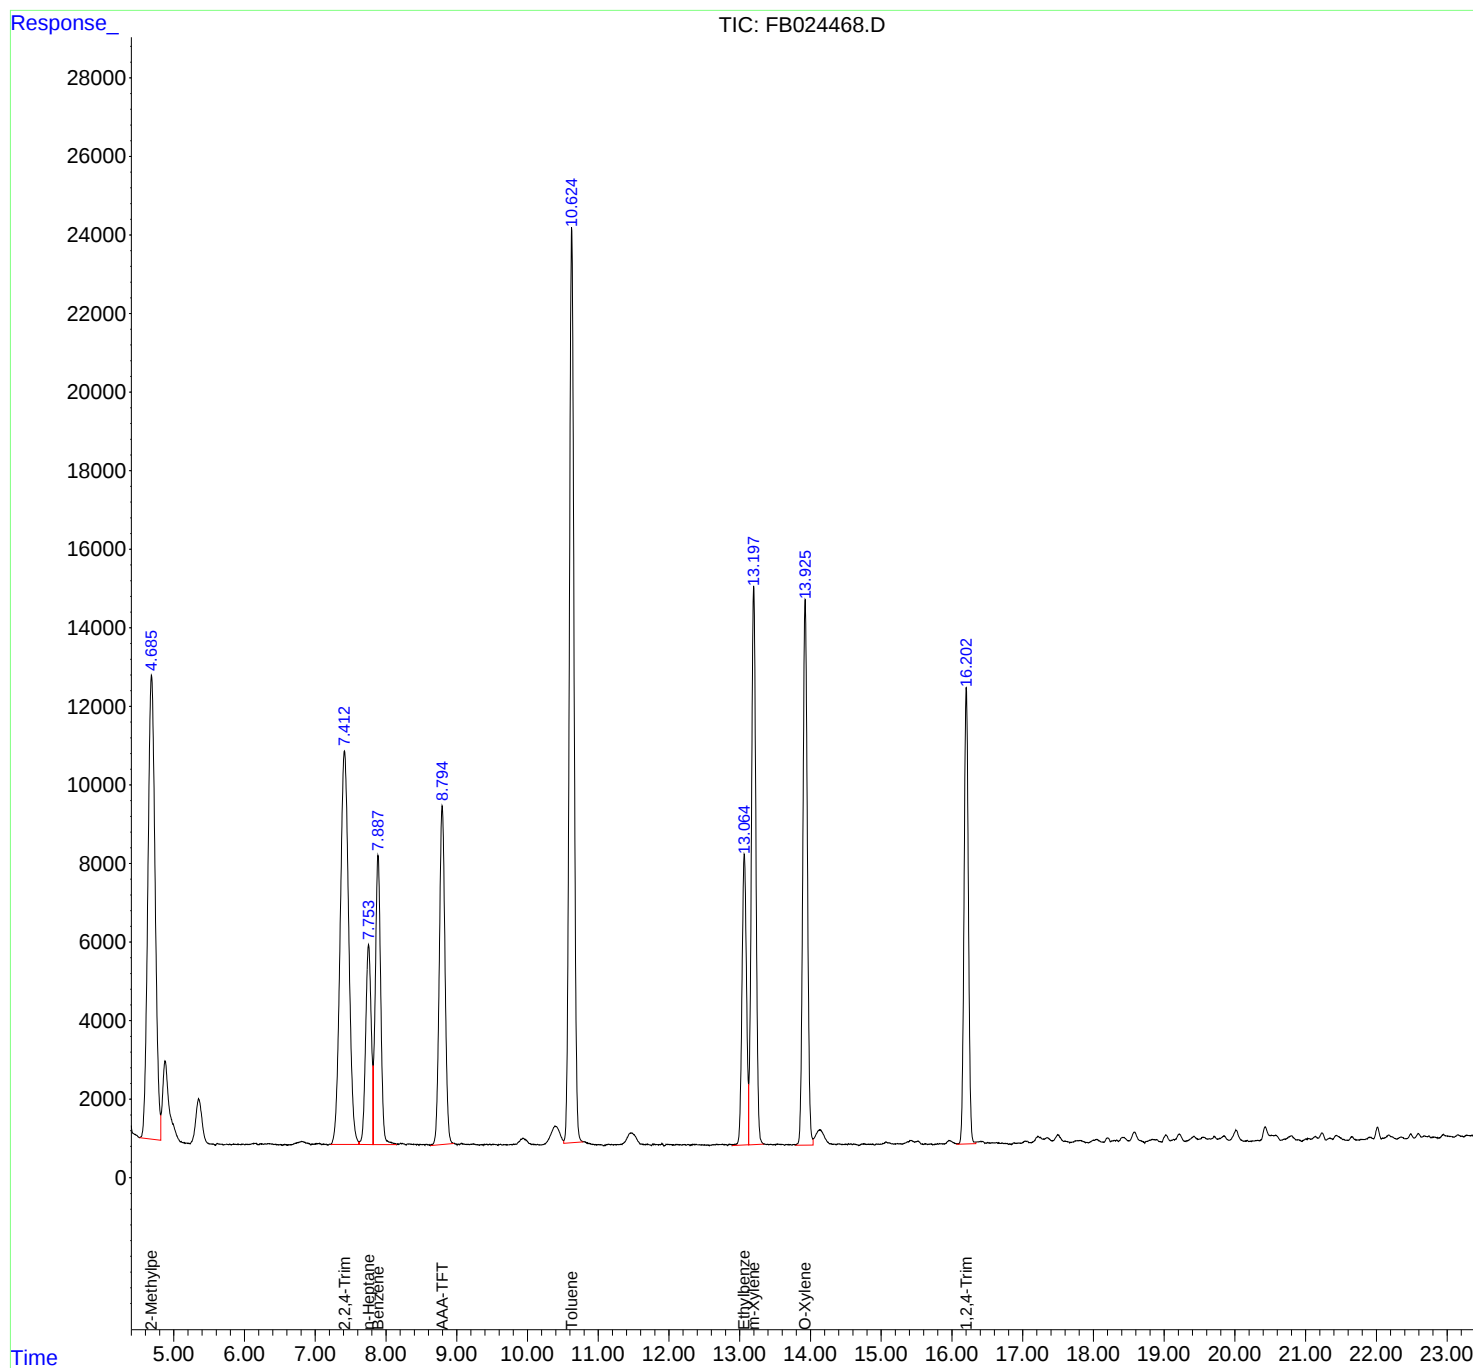

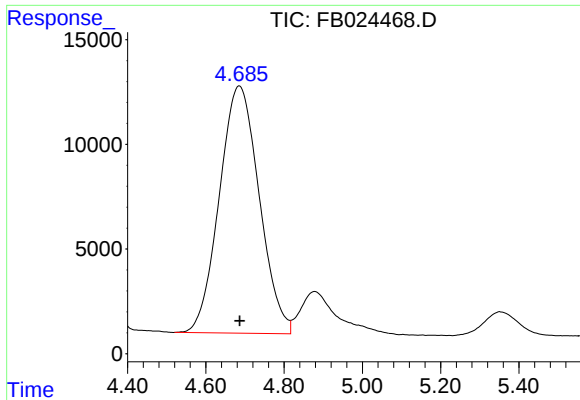


#1 2-Methylpentane

R.T.: 4.686 min
 Delta R.T.: -0.001 min
 Response: 835859
 Conc: 26.15 ng/ml

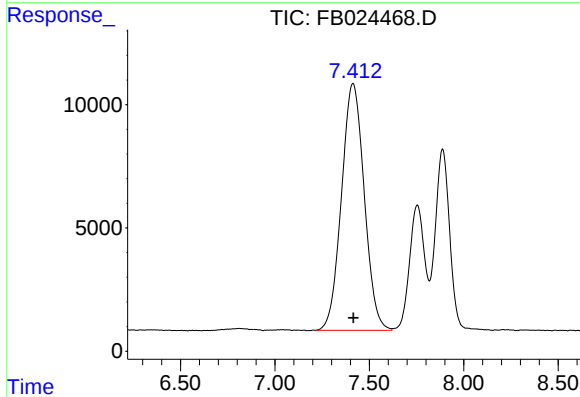


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
 Delta R.T.: -0.002 min
 Response: 837742
 Conc: 24.99 ng/ml

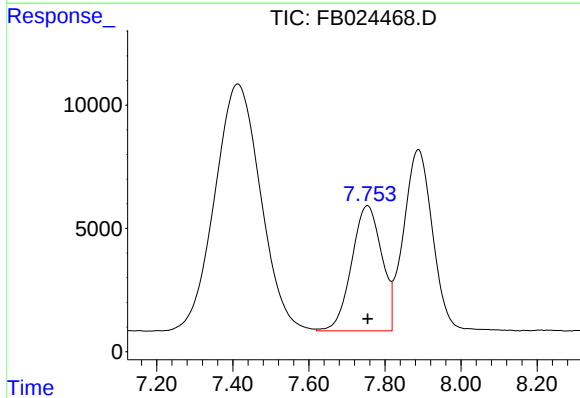


#3 n-Heptane

R.T.: 7.754 min
 Delta R.T.: 0.000 min
 Response: 279463
 Conc: 8.26 ng/ml

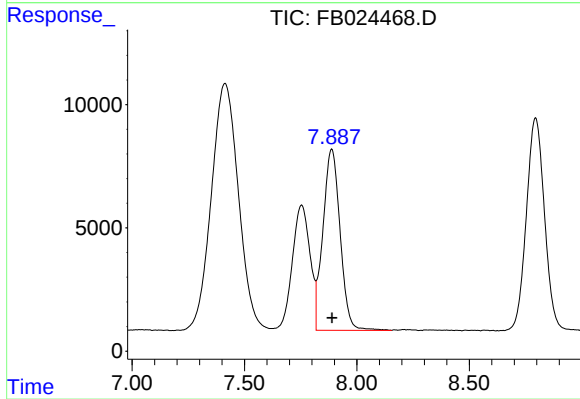


#4 Benzene

R.T.: 7.888 min
 Delta R.T.: -0.002 min
 Response: 391171
 Conc: 9.68 ng/ml

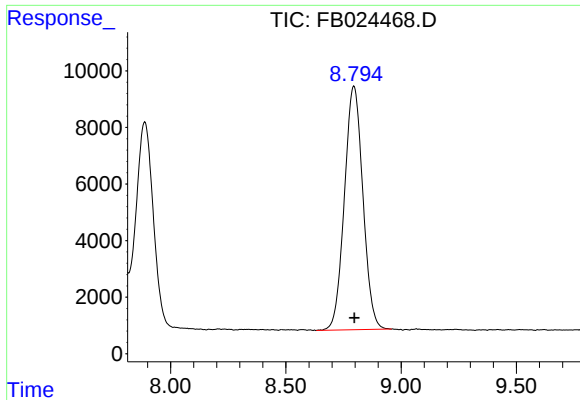


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 480450
Conc: 19.86 ng/ml

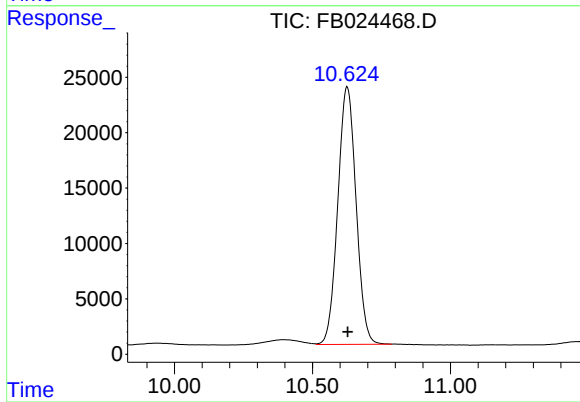


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 1070738
Conc: 27.25 ng/ml

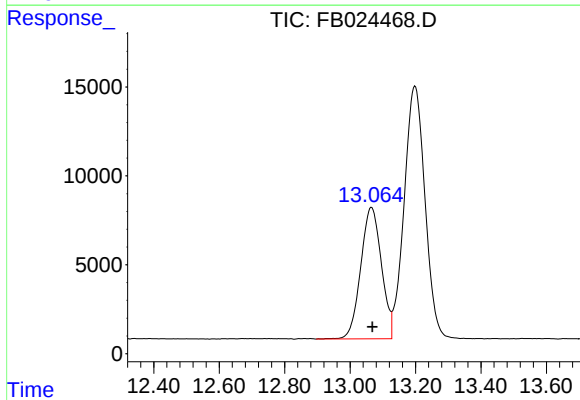


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.002 min
Response: 324844
Conc: 9.26 ng/ml

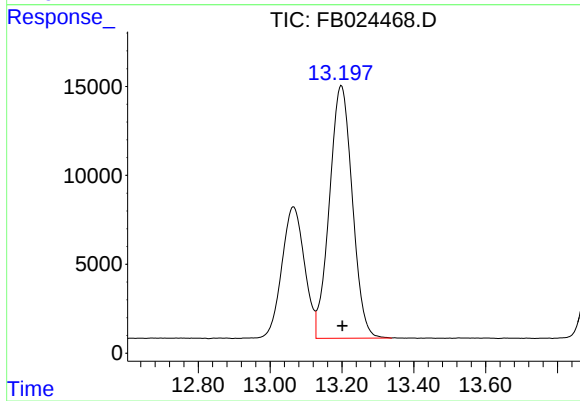

#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.003 min
Response: 628178
Conc: 18.34 ng/ml

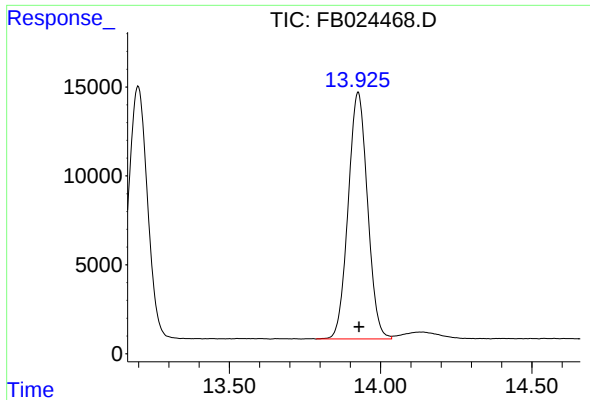


#9 O-Xylene

R.T.: 13.926 min

Delta R.T.: -0.003 min

Response: 617111

Conc: 18.41 ng/ml

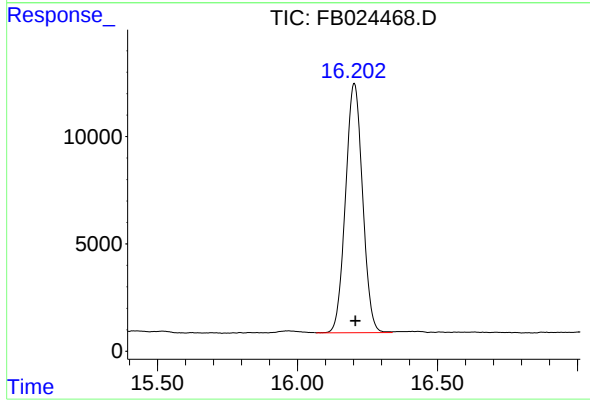

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min

Delta R.T.: -0.003 min

Response: 491644

Conc: 17.71 ng/ml