

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061819\
 Data File : FB021409.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jun 2019 20:27
 Operator : MJ/SJ
 Sample : BSF0618S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 19 03:29:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	310238	21.042 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	877911	23.353 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	1055388	30.904 ng/ml
3) t n-Heptane	7.947	322856	9.903 ng/ml
4) t Benzene	8.089	312228	9.046 ng/ml
6) t Toluene	10.830	753812	31.803 ng/ml
7) t Ethylbenzene	13.274	239096	10.232 ng/ml
8) t m-Xylene	13.407	514558	20.615 ng/ml
9) t O-Xylene	14.136	534401	20.485 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	539172	20.077 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061819\
Data File : FB021409.D
Signal(s) : FID2B.CH
Acq On : 18 Jun 2019 20:27
Operator : MJ/SJ
Sample : BSF0618S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 19 03:29:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

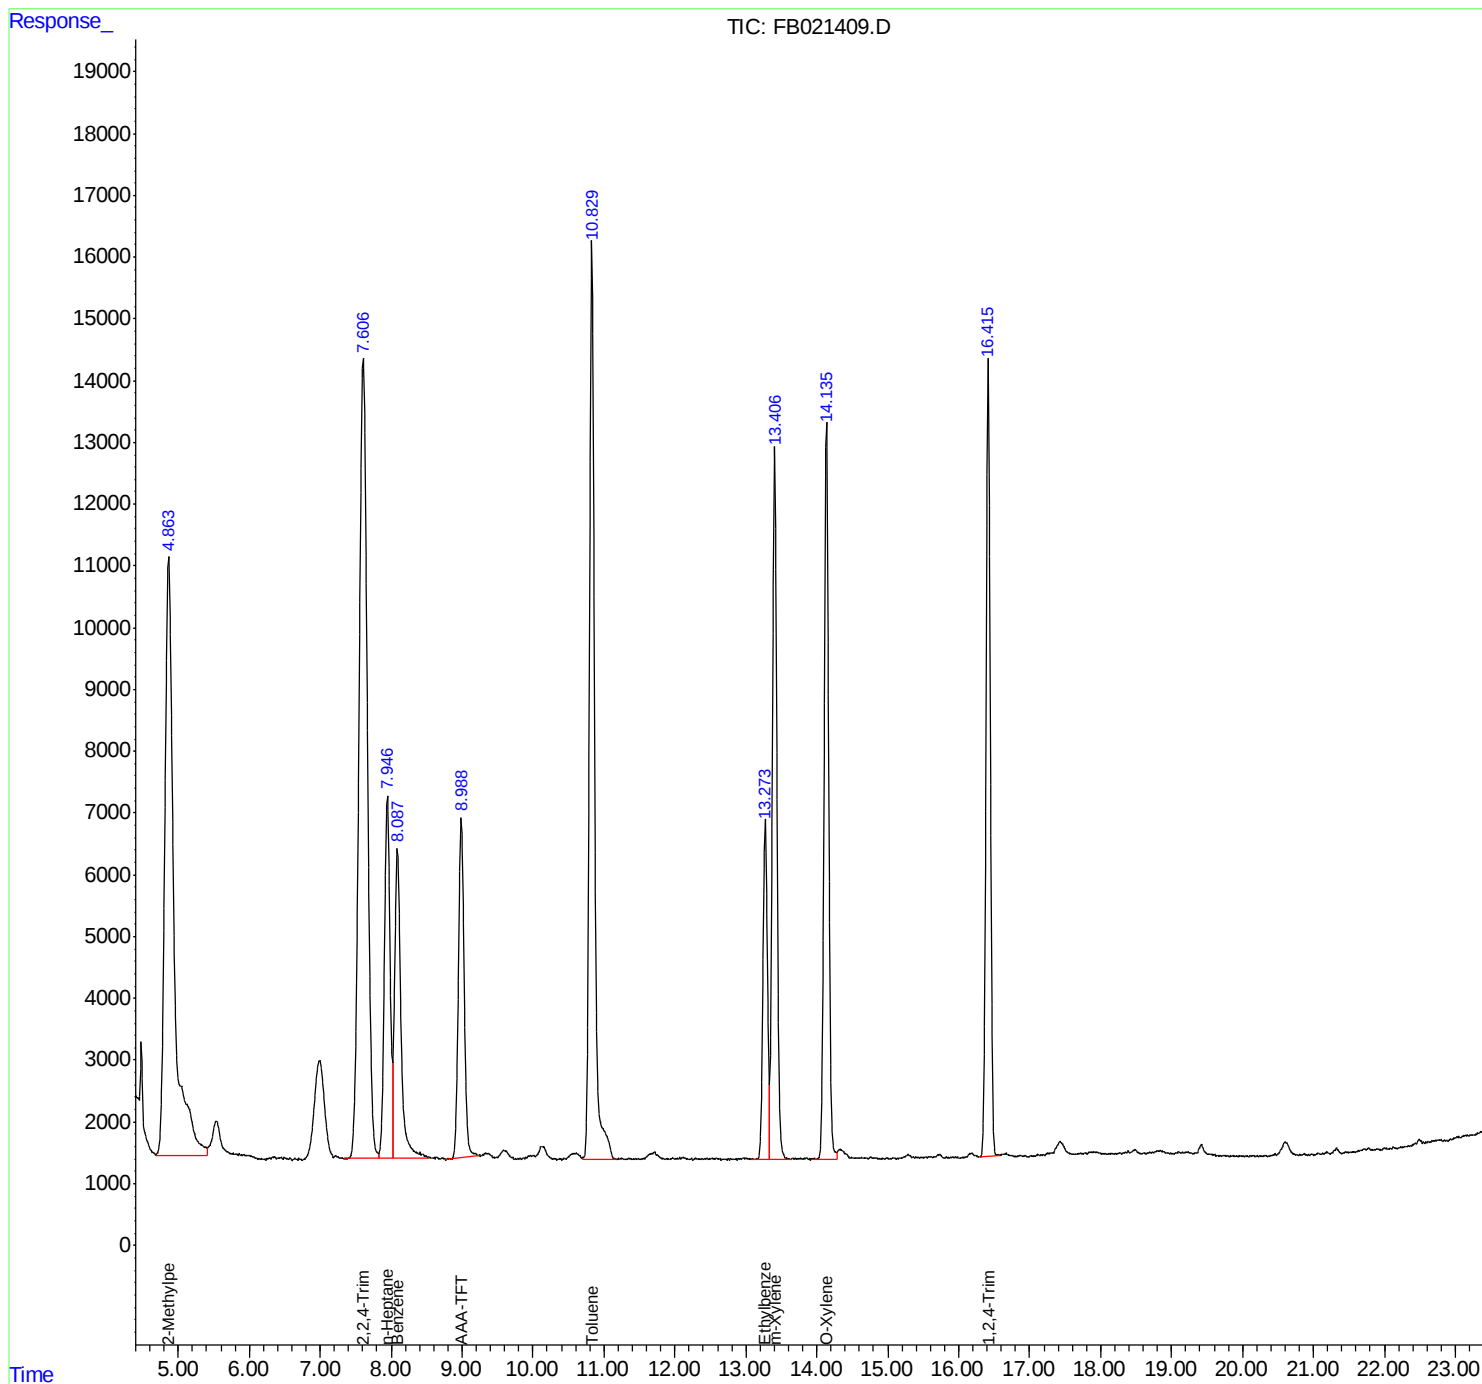

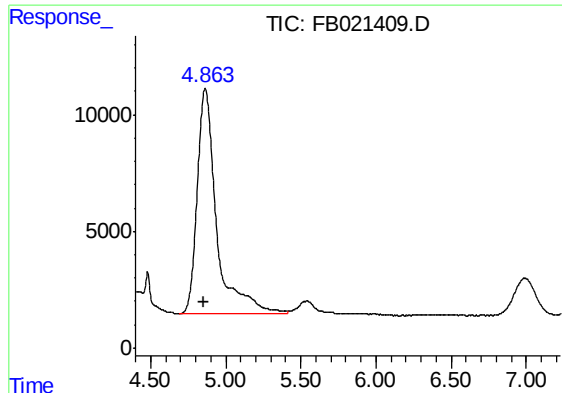


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.007 min
Response: 877911
Conc: 23.35 ng/ml

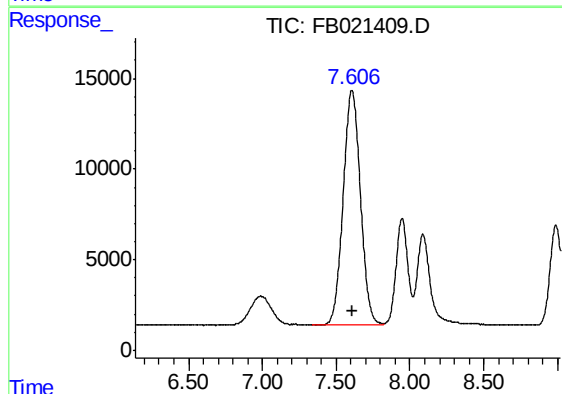


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: -0.007 min
Response: 1055388
Conc: 30.90 ng/ml

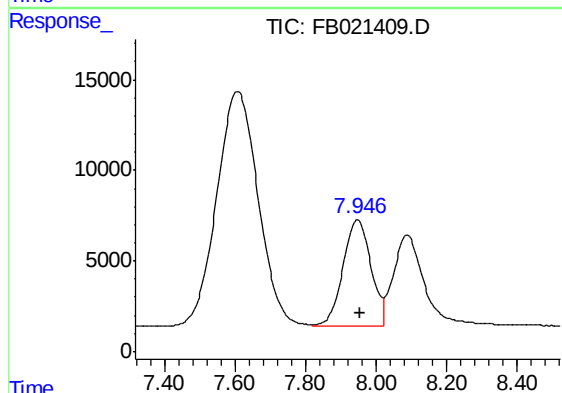


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: -0.007 min
Response: 322856
Conc: 9.90 ng/ml

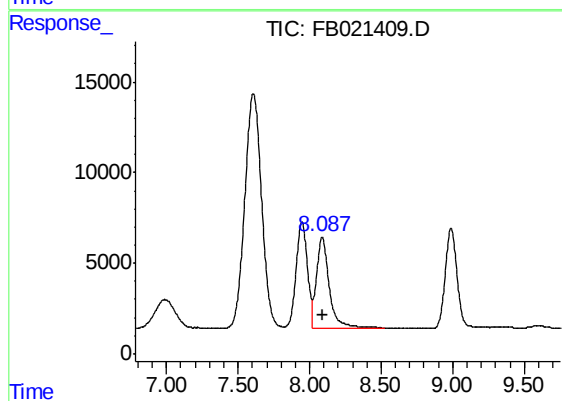


#4 Benzene

R.T.: 8.089 min
Delta R.T.: -0.001 min
Response: 312228
Conc: 9.05 ng/ml

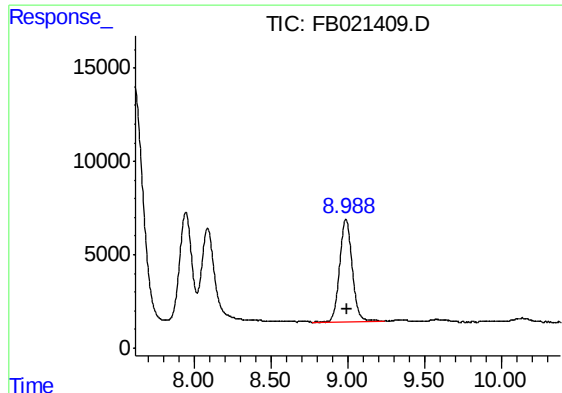


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.009 min
Response: 310238
Conc: 21.04 ng/ml

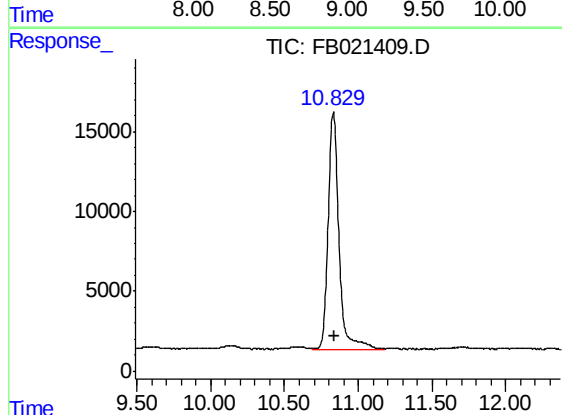


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.012 min
Response: 753812
Conc: 31.80 ng/ml

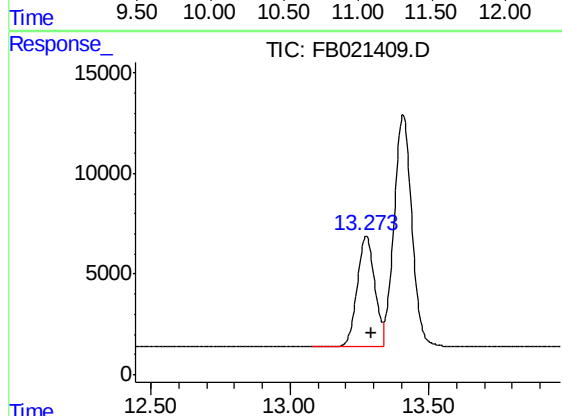


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: -0.019 min
Response: 239096
Conc: 10.23 ng/ml

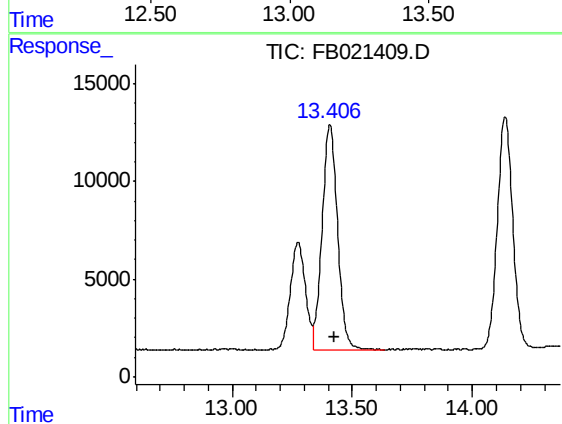


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.019 min
Response: 514558
Conc: 20.62 ng/ml

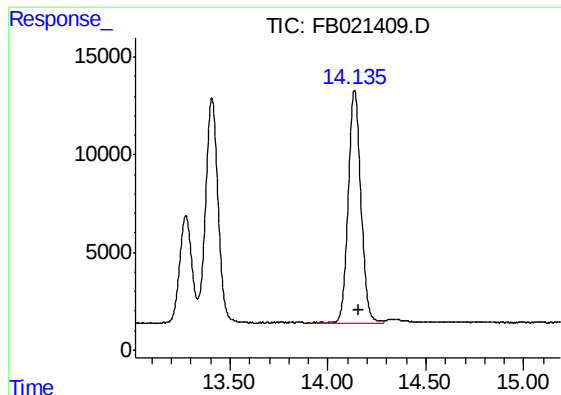

#9 O-Xylene

R.T.: 14.136 min
Delta R.T.: -0.020 min
Response: 534401
Conc: 20.49 ng/ml

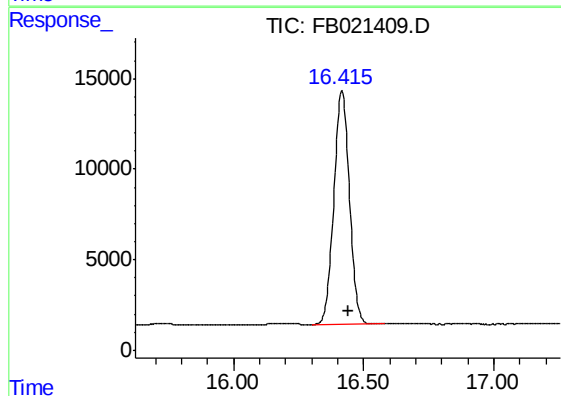

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.024 min
Response: 539172
Conc: 20.08 ng/ml