

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061819\
 Data File : FB021427.D
 Signal(s) : FID2B.CH
 Acq On : 19 Jun 2019 5:30
 Operator : MJ/SJ
 Sample : K3157-01MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 19 06:43:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	306796	20.808 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	712507	18.953 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	968589	28.362 ng/ml
3) t n-Heptane	7.948	290233	8.903 ng/ml
4) t Benzene	8.090	315777	9.149 ng/ml
6) t Toluene	10.832	718996	30.335 ng/ml
7) t Ethylbenzene	13.275	215847	9.237 ng/ml
8) t m-Xylene	13.407	460640	18.455 ng/ml
9) t O-Xylene	14.137	475383	18.223 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	474158	17.656 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061819\
Data File : FB021427.D
Signal(s) : FID2B.CH
Acq On : 19 Jun 2019 5:30
Operator : MJ/SJ
Sample : K3157-01MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 19 06:43:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

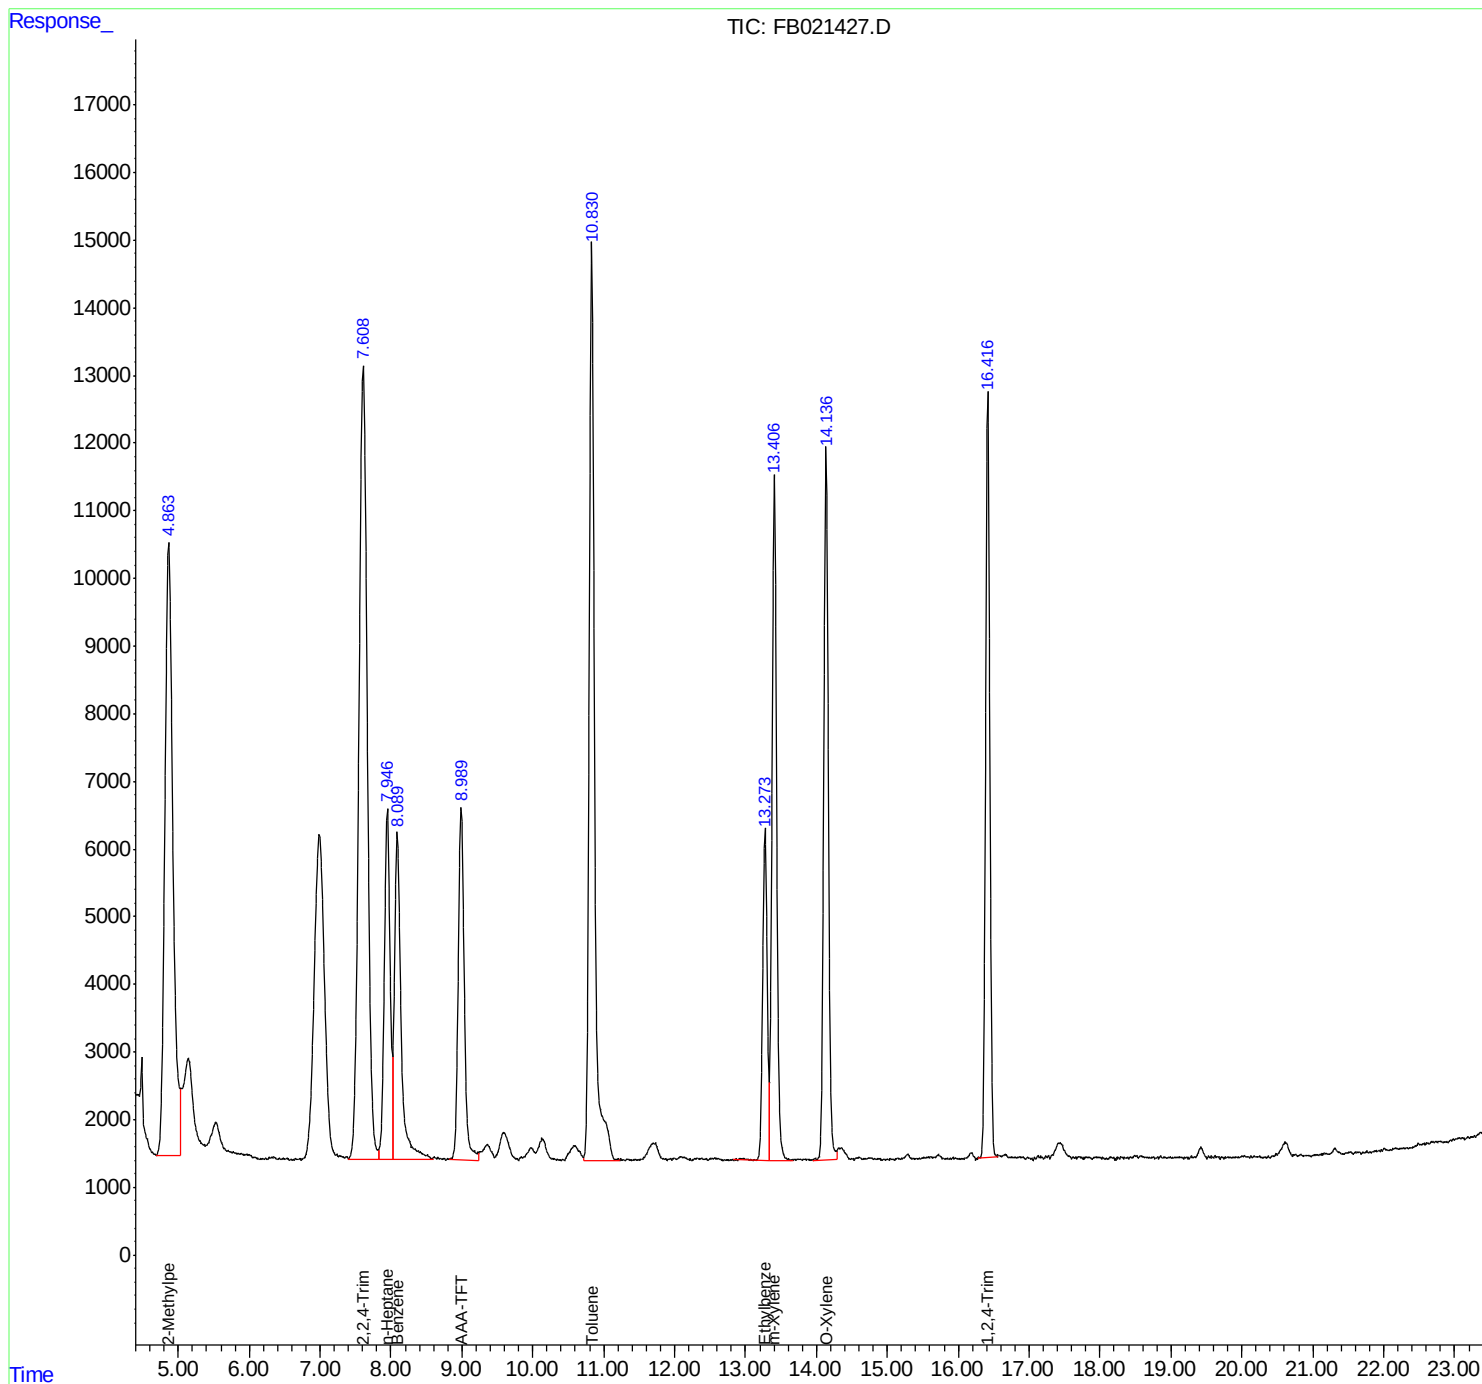

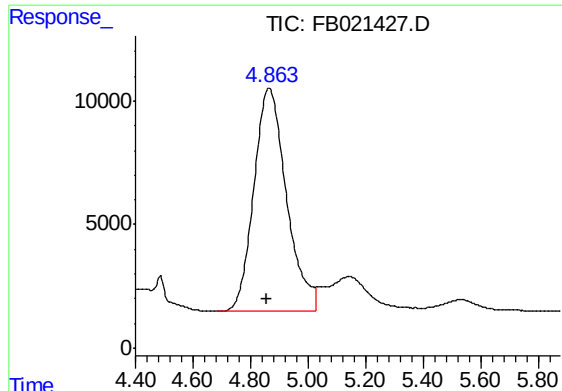


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.007 min
Response: 712507
Conc: 18.95 ng/ml

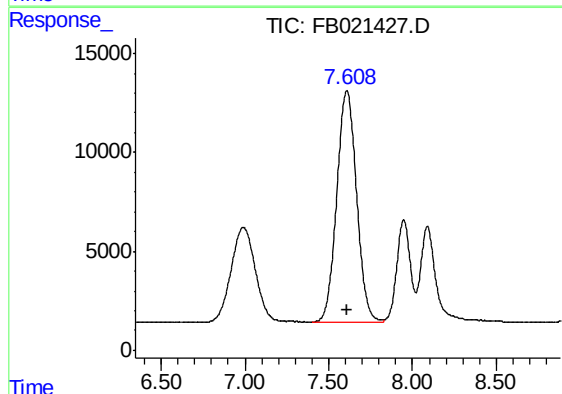


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.005 min
Response: 968589
Conc: 28.36 ng/ml

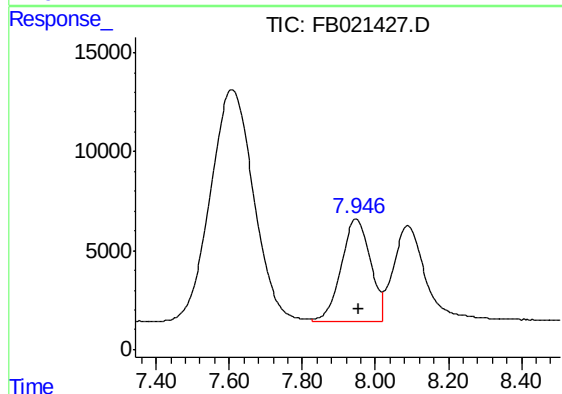


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.006 min
Response: 290233
Conc: 8.90 ng/ml

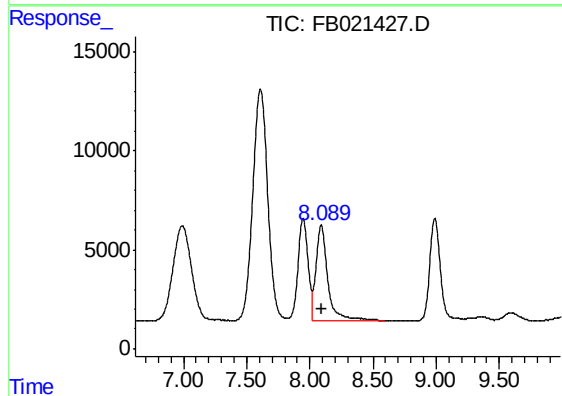


#4 Benzene

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 315777
Conc: 9.15 ng/ml

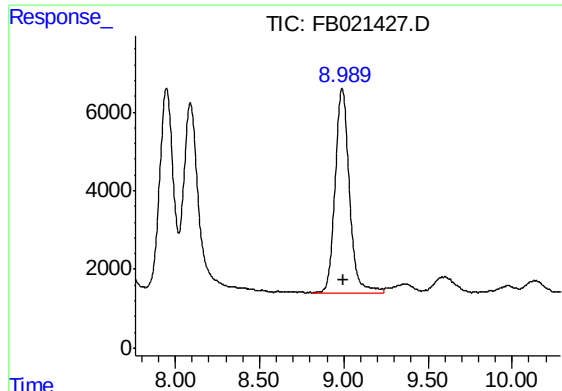


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.008 min
Response: 306796
Conc: 20.81 ng/ml

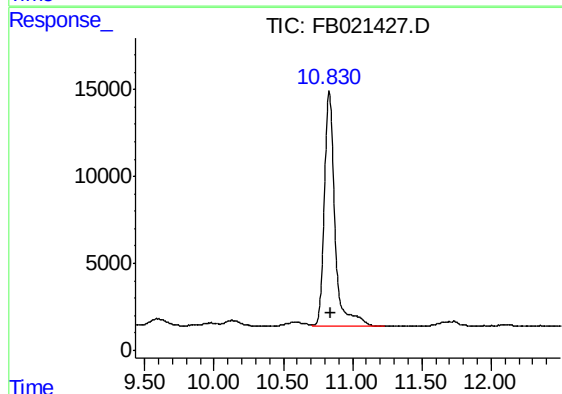


#6 Toluene

R.T.: 10.832 min
Delta R.T.: -0.011 min
Response: 718996
Conc: 30.33 ng/ml

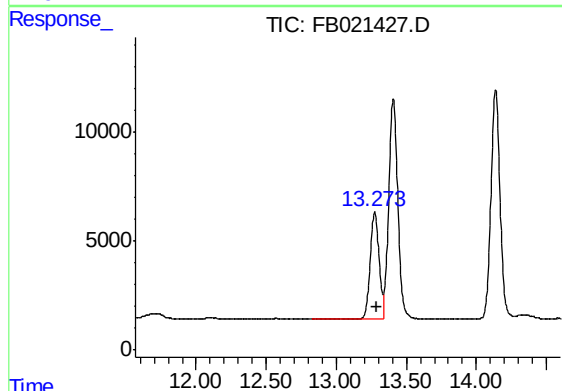


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.018 min
Response: 215847
Conc: 9.24 ng/ml

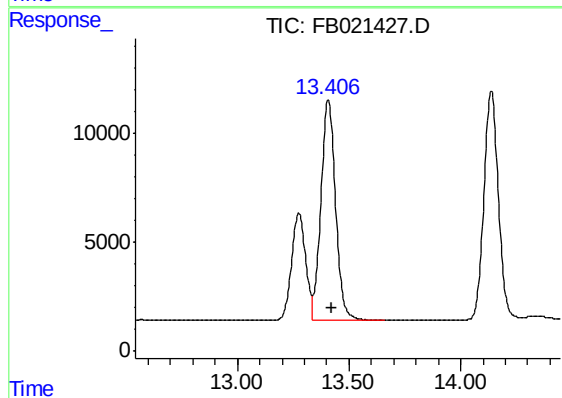


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.018 min
Response: 460640
Conc: 18.46 ng/ml

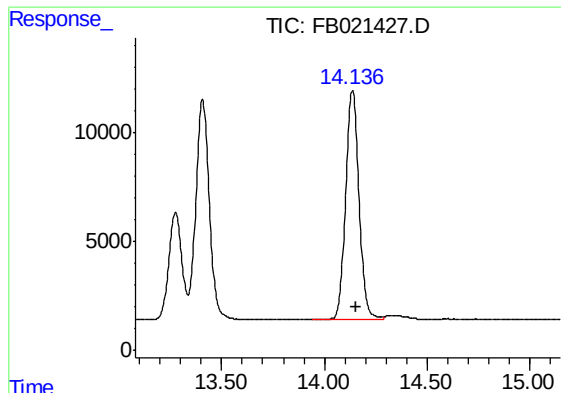

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.020 min
Response: 475383
Conc: 18.22 ng/ml

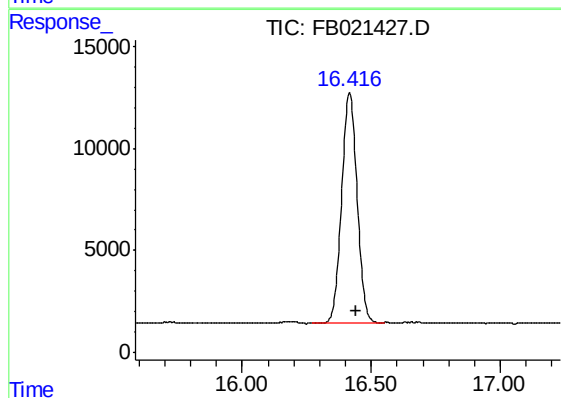

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.024 min
Response: 474158
Conc: 17.66 ng/ml