

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061820\
 Data File : FB024485.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jun 2020 13:44
 Operator : DD/AJ
 Sample : L3035-16MSD
 Misc : 5.05gm/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 19 01:03:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	530946	21.945 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	871997	27.281 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	878504	26.205 ng/ml
3) t n-Heptane	7.755	287300	8.496 ng/ml
4) t Benzene	7.890	392652	9.713 ng/ml
6) t Toluene	10.628	1106641	28.160 ng/ml
7) t Ethylbenzene	13.067	331562	9.449 ng/ml
8) t m-Xylene	13.200	652020	19.039 ng/ml
9) t O-Xylene	13.928	641437	19.132 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	519955	18.727 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061820\
Data File : FB024485.D
Signal(s) : FID2B.CH
Acq On : 18 Jun 2020 13:44
Operator : DD/AJ
Sample : L3035-16MSD
Misc : 5.05gm/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 19 01:03:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

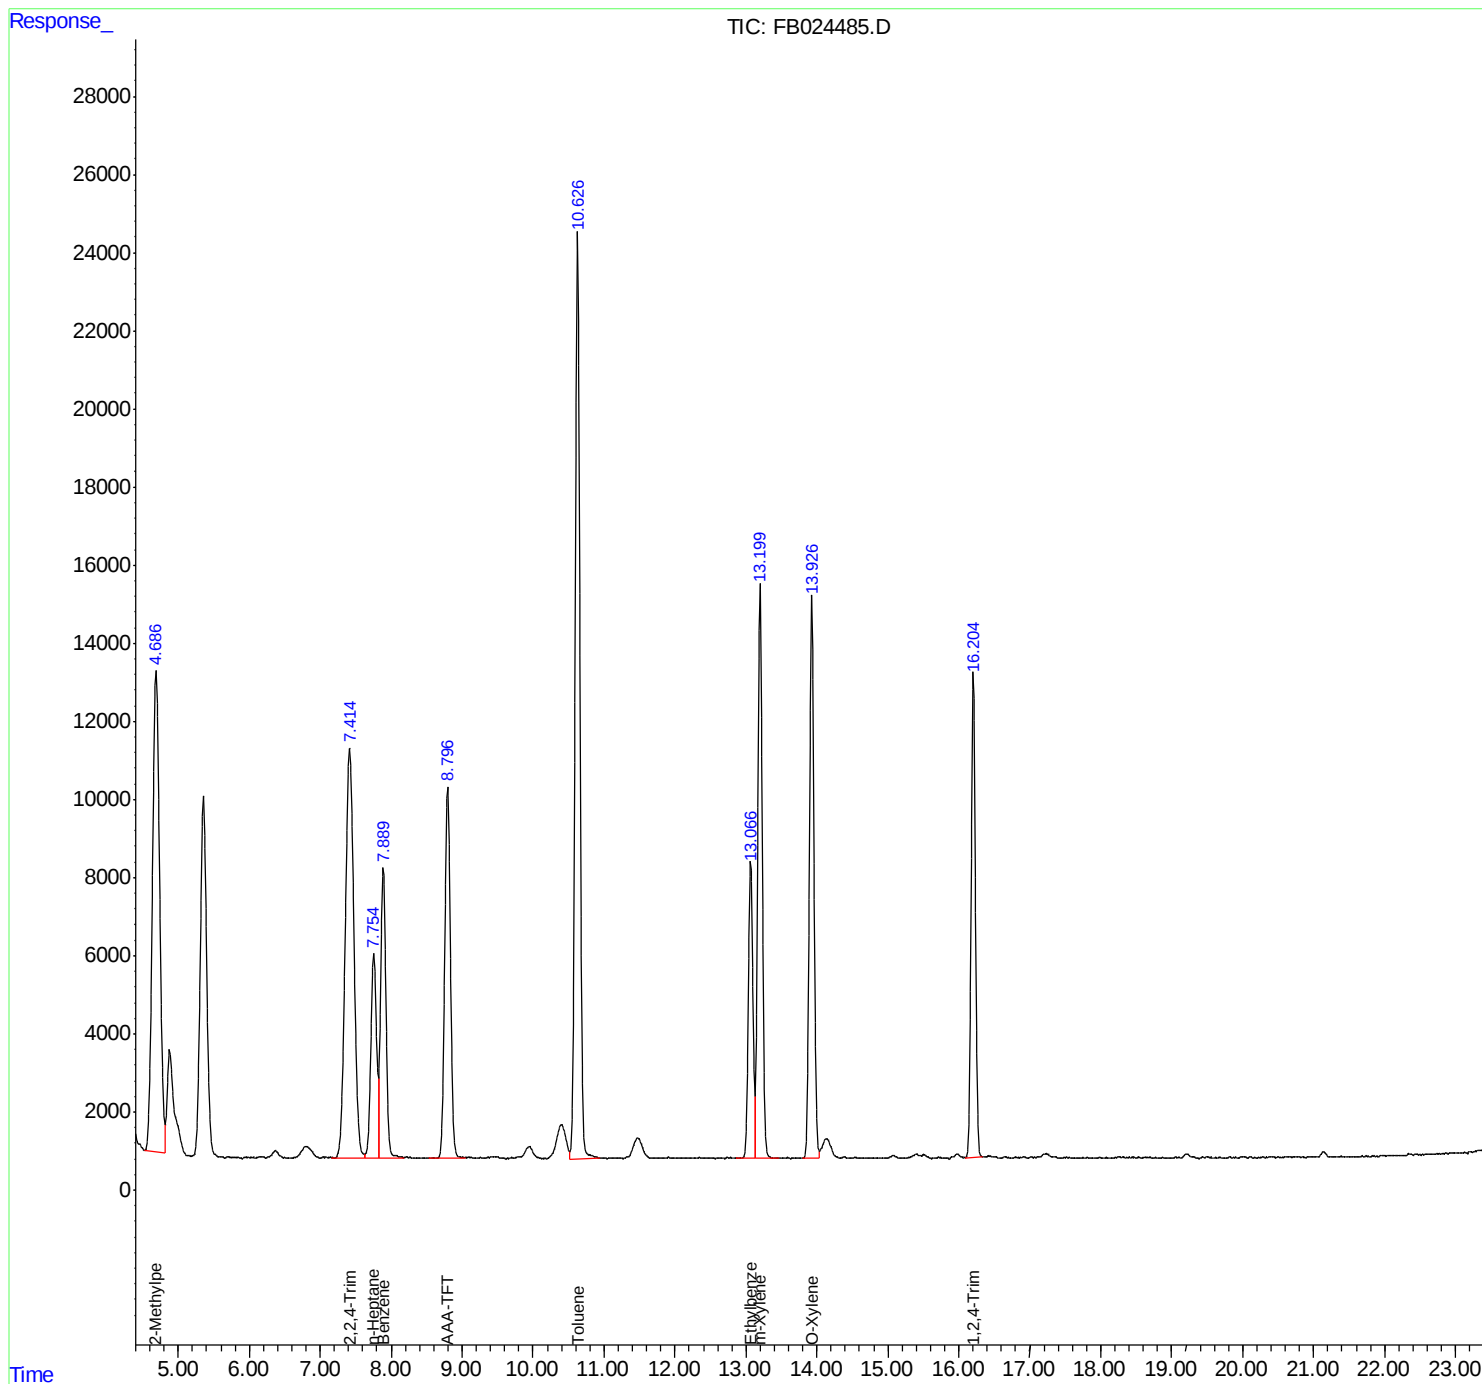

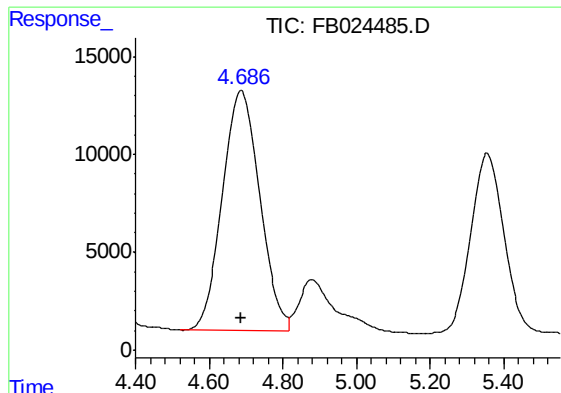


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 871997
Conc: 27.28 ng/ml

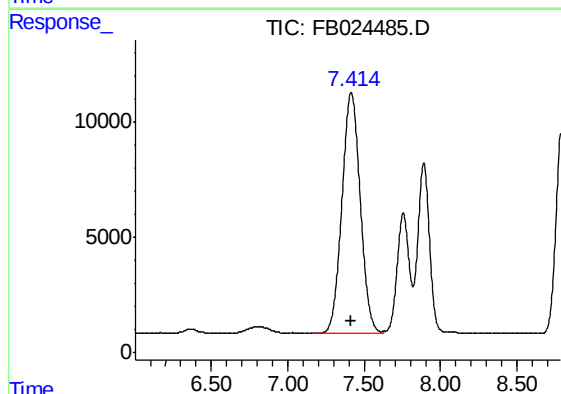


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 878504
Conc: 26.21 ng/ml

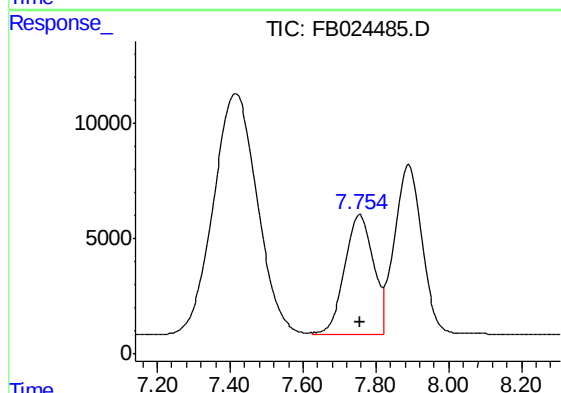


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 287300
Conc: 8.50 ng/ml

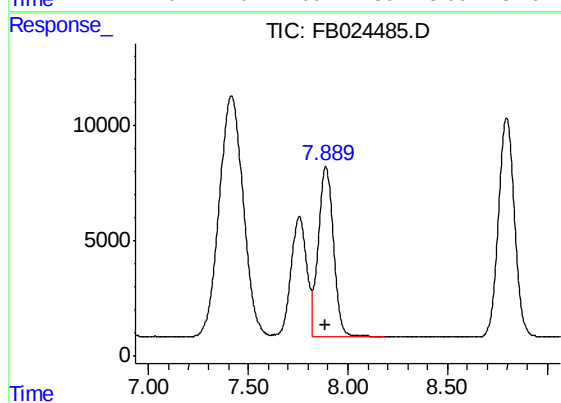


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 392652
Conc: 9.71 ng/ml

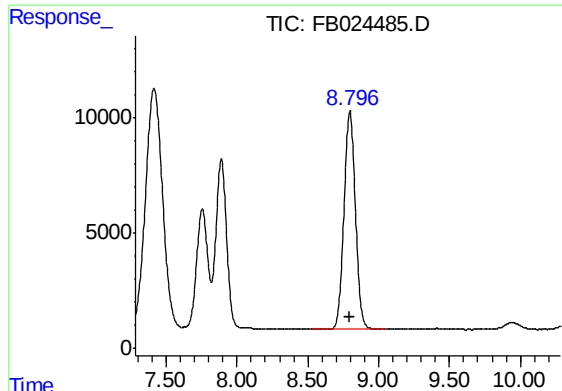


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 530946
Conc: 21.95 ng/ml

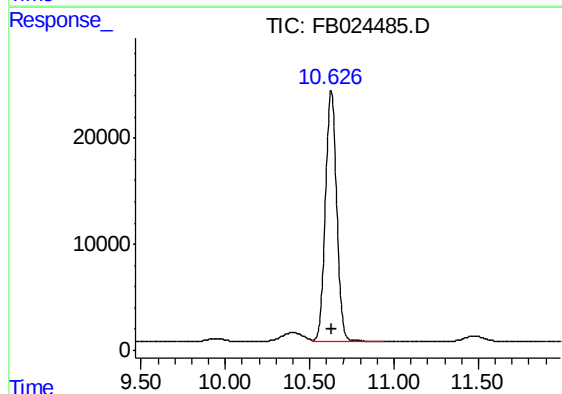


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 1106641
Conc: 28.16 ng/ml

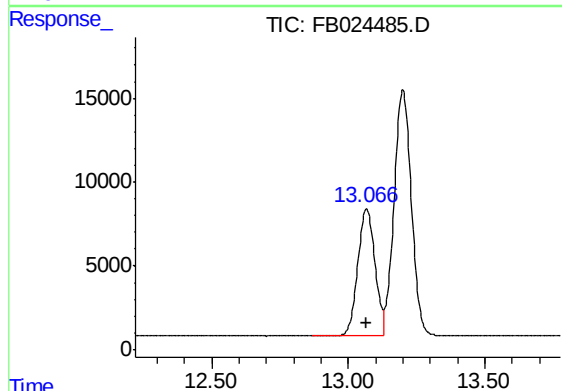


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.000 min
Response: 331562
Conc: 9.45 ng/ml

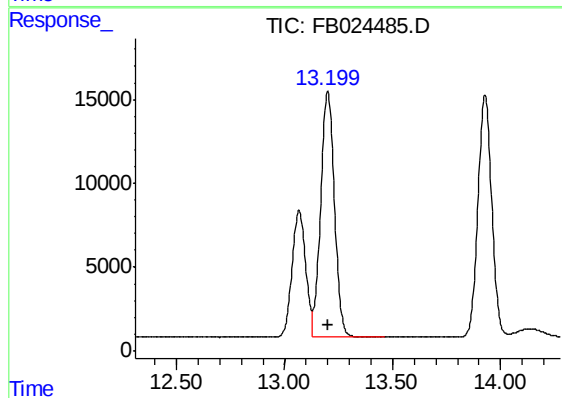


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: 0.000 min
Response: 652020
Conc: 19.04 ng/ml

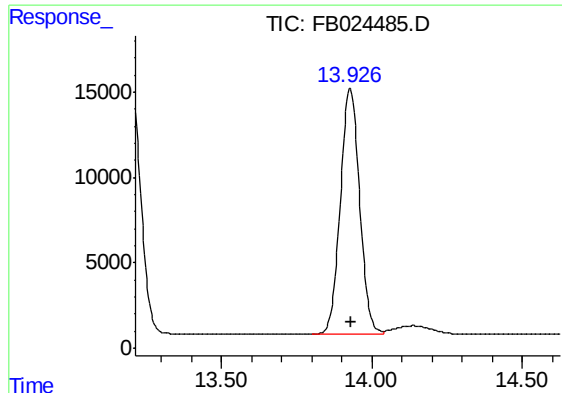

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.001 min
Response: 641437
Conc: 19.13 ng/ml

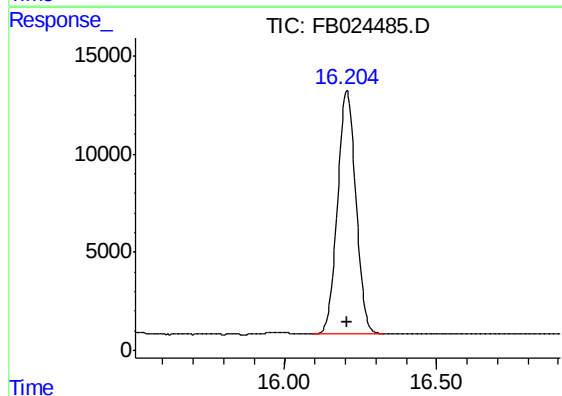

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.001 min
Response: 519955
Conc: 18.73 ng/ml