

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061820\
 Data File : FB024478.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jun 2020 10:11
 Operator : DD/AJ
 Sample : BSF0618S1
 Misc : 5.00gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 19 01:02:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	516927	21.366 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	900554	28.174 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	967826	28.870 ng/ml
3) t n-Heptane	7.755	320535	9.479 ng/ml
4) t Benzene	7.889	381242	9.431 ng/ml
6) t Toluene	10.627	1081296	27.515 ng/ml
7) t Ethylbenzene	13.066	332982	9.489 ng/ml
8) t m-Xylene	13.199	651039	19.011 ng/ml
9) t O-Xylene	13.927	633336	18.891 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	530438	19.104 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061820\
Data File : FB024478.D
Signal(s) : FID2B.CH
Acq On : 18 Jun 2020 10:11
Operator : DD/AJ
Sample : BSF0618S1
Misc : 5.00gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 19 01:02:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

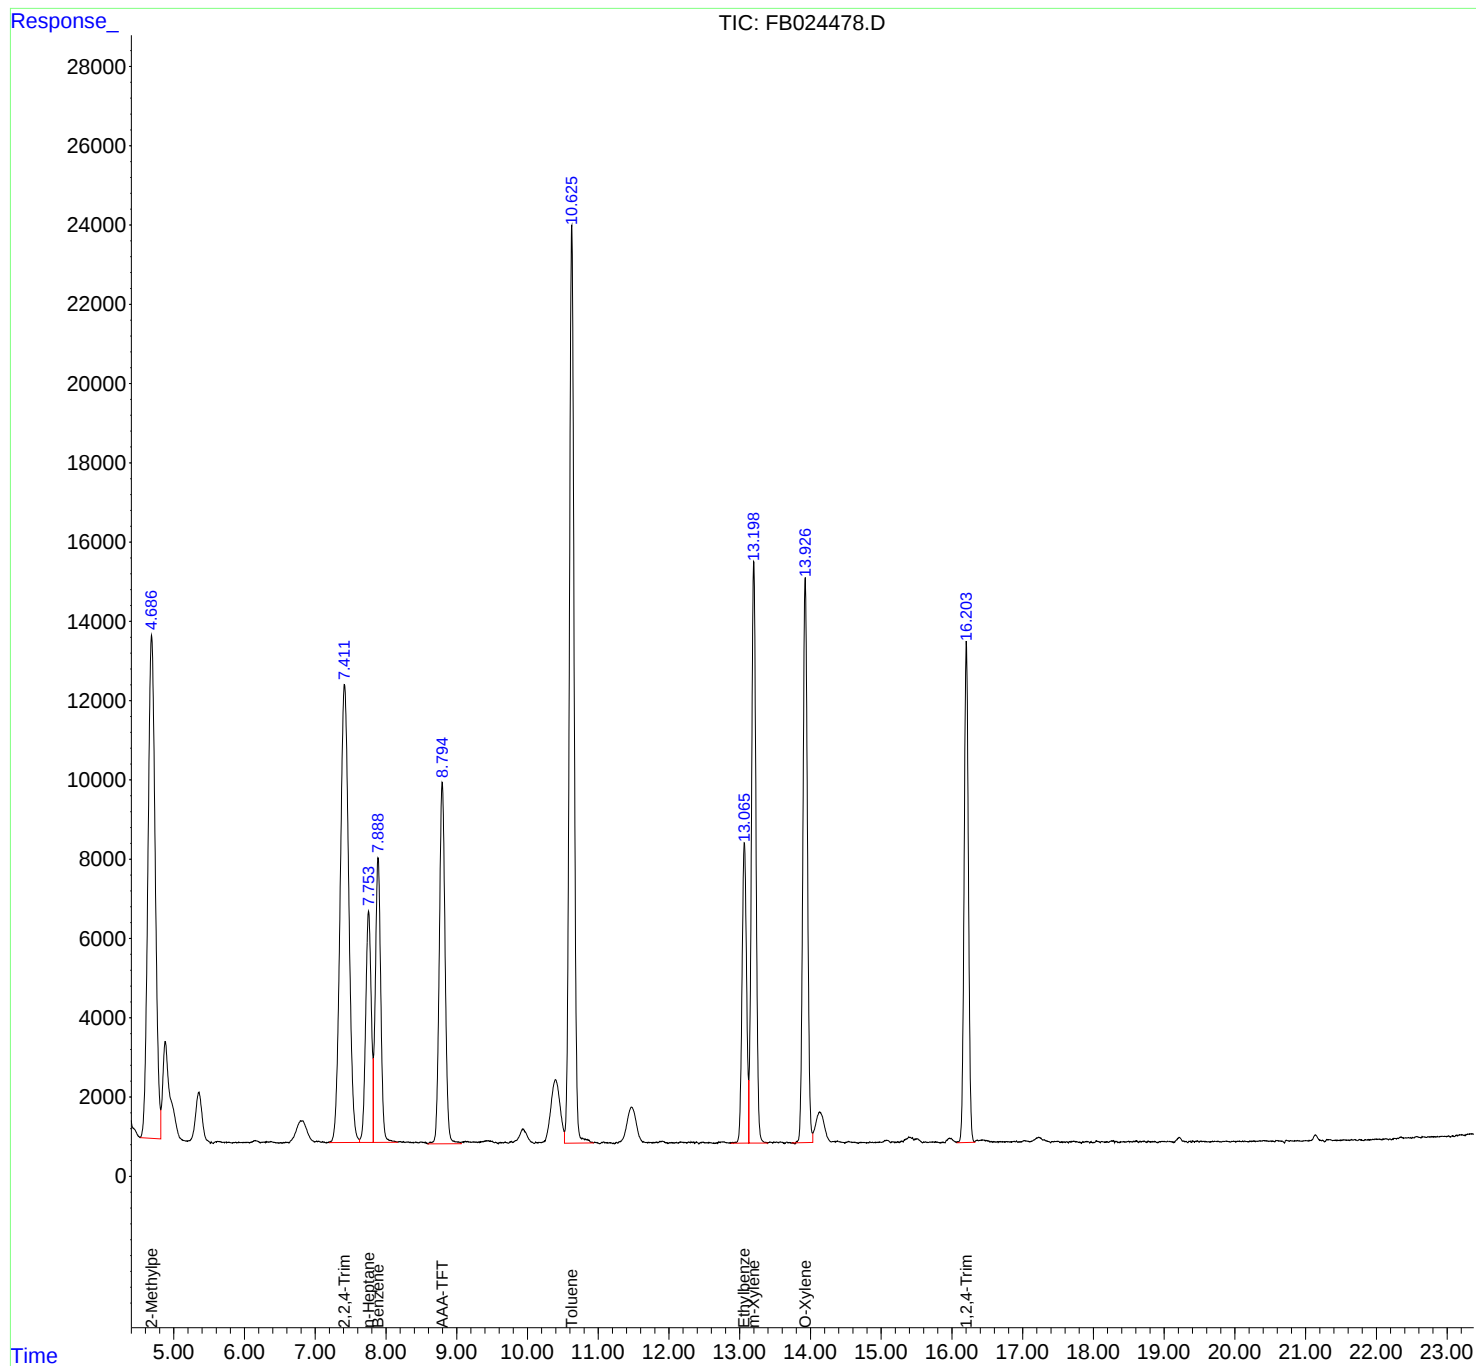

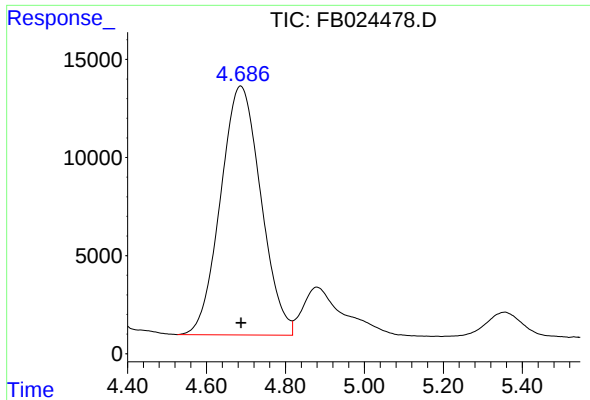


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 900554
Conc: 28.17 ng/ml

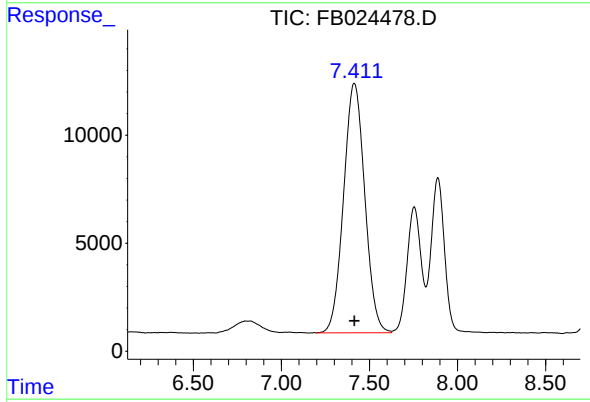


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.003 min
Response: 967826
Conc: 28.87 ng/ml

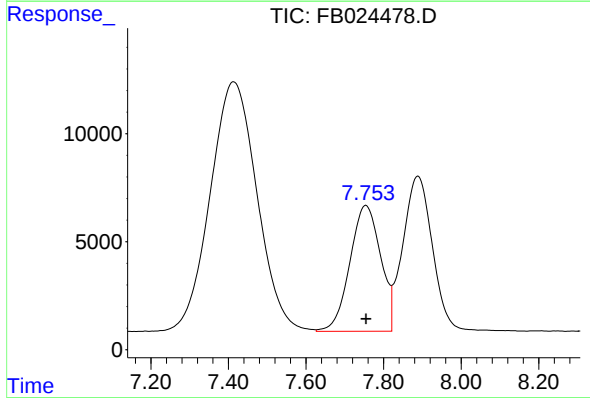


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 320535
Conc: 9.48 ng/ml

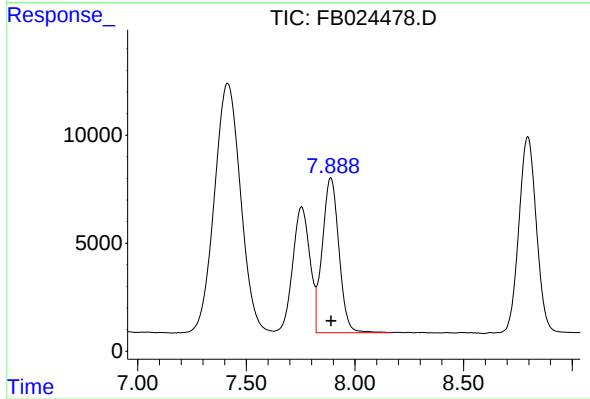


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 381242
Conc: 9.43 ng/ml

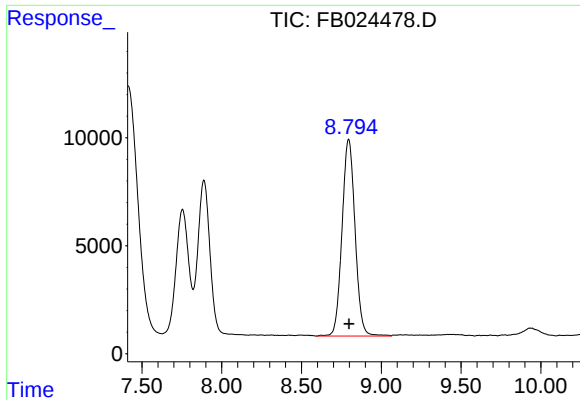


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.001 min
Response: 516927
Conc: 21.37 ng/ml

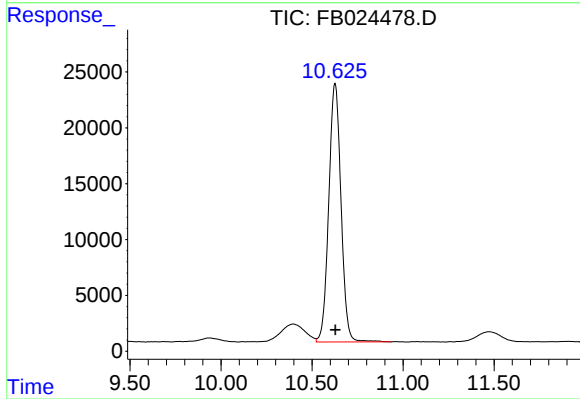


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.002 min
Response: 1081296
Conc: 27.52 ng/ml

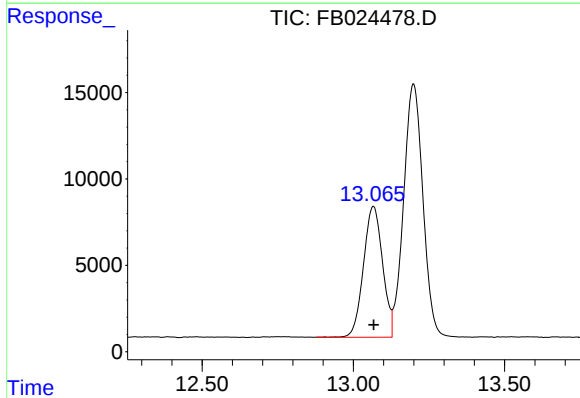


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.001 min
Response: 332982
Conc: 9.49 ng/ml

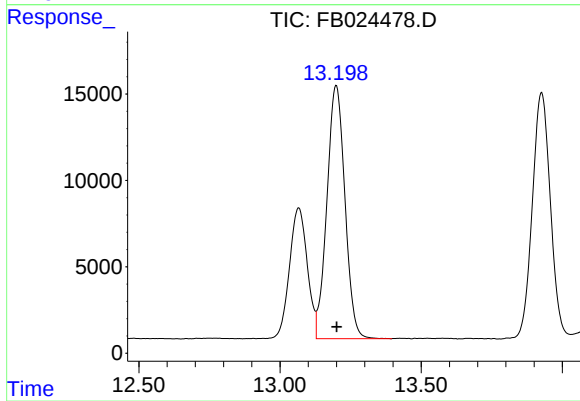


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.002 min
Response: 651039
Conc: 19.01 ng/ml

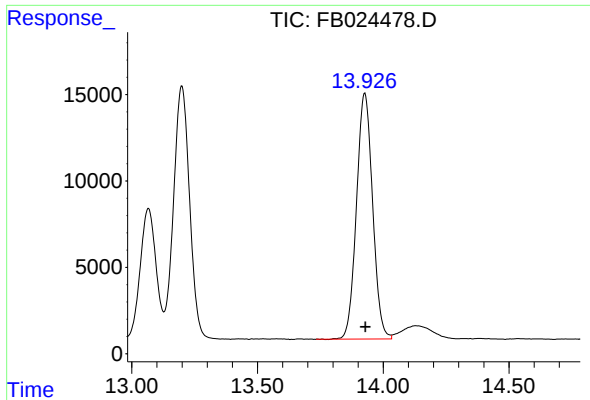

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.002 min
Response: 633336
Conc: 18.89 ng/ml

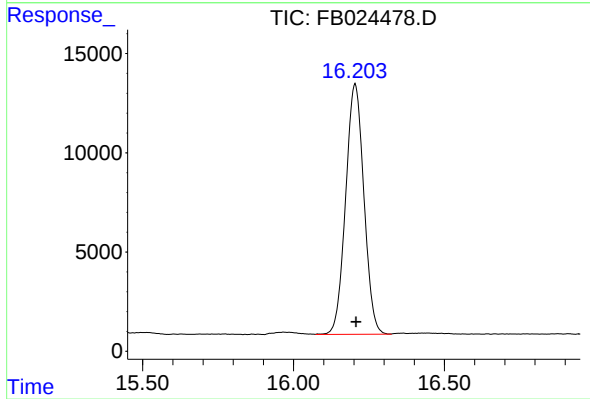

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.003 min
Response: 530438
Conc: 19.10 ng/ml