

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061821\
 Data File : FB025886.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jun 2021 12:56
 Operator : DD/AJ
 Sample : M2746-02MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 18 23:31:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.219	467193	19.332 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.182	708661	26.928 ng/ml
2) t 2,2,4-Trimethylpentane	7.876	562933	27.944 ng/ml
3) t n-Heptane	8.196	295225	8.213 ng/ml
4) t Benzene	8.347	384603	9.213 ng/ml
6) t Toluene	11.038	1050714	25.533 ng/ml
7) t Ethylbenzene	13.445	318528	8.358 ng/ml
8) t m-Xylene	13.575	619832	15.767 ng/ml
9) t O-Xylene	14.298	561747	17.618 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	331228	16.828 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061821\
Data File : FB025886.D
Signal(s) : FID2B.CH
Acq On : 18 Jun 2021 12:56
Operator : DD/AJ
Sample : M2746-02MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 18 23:31:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

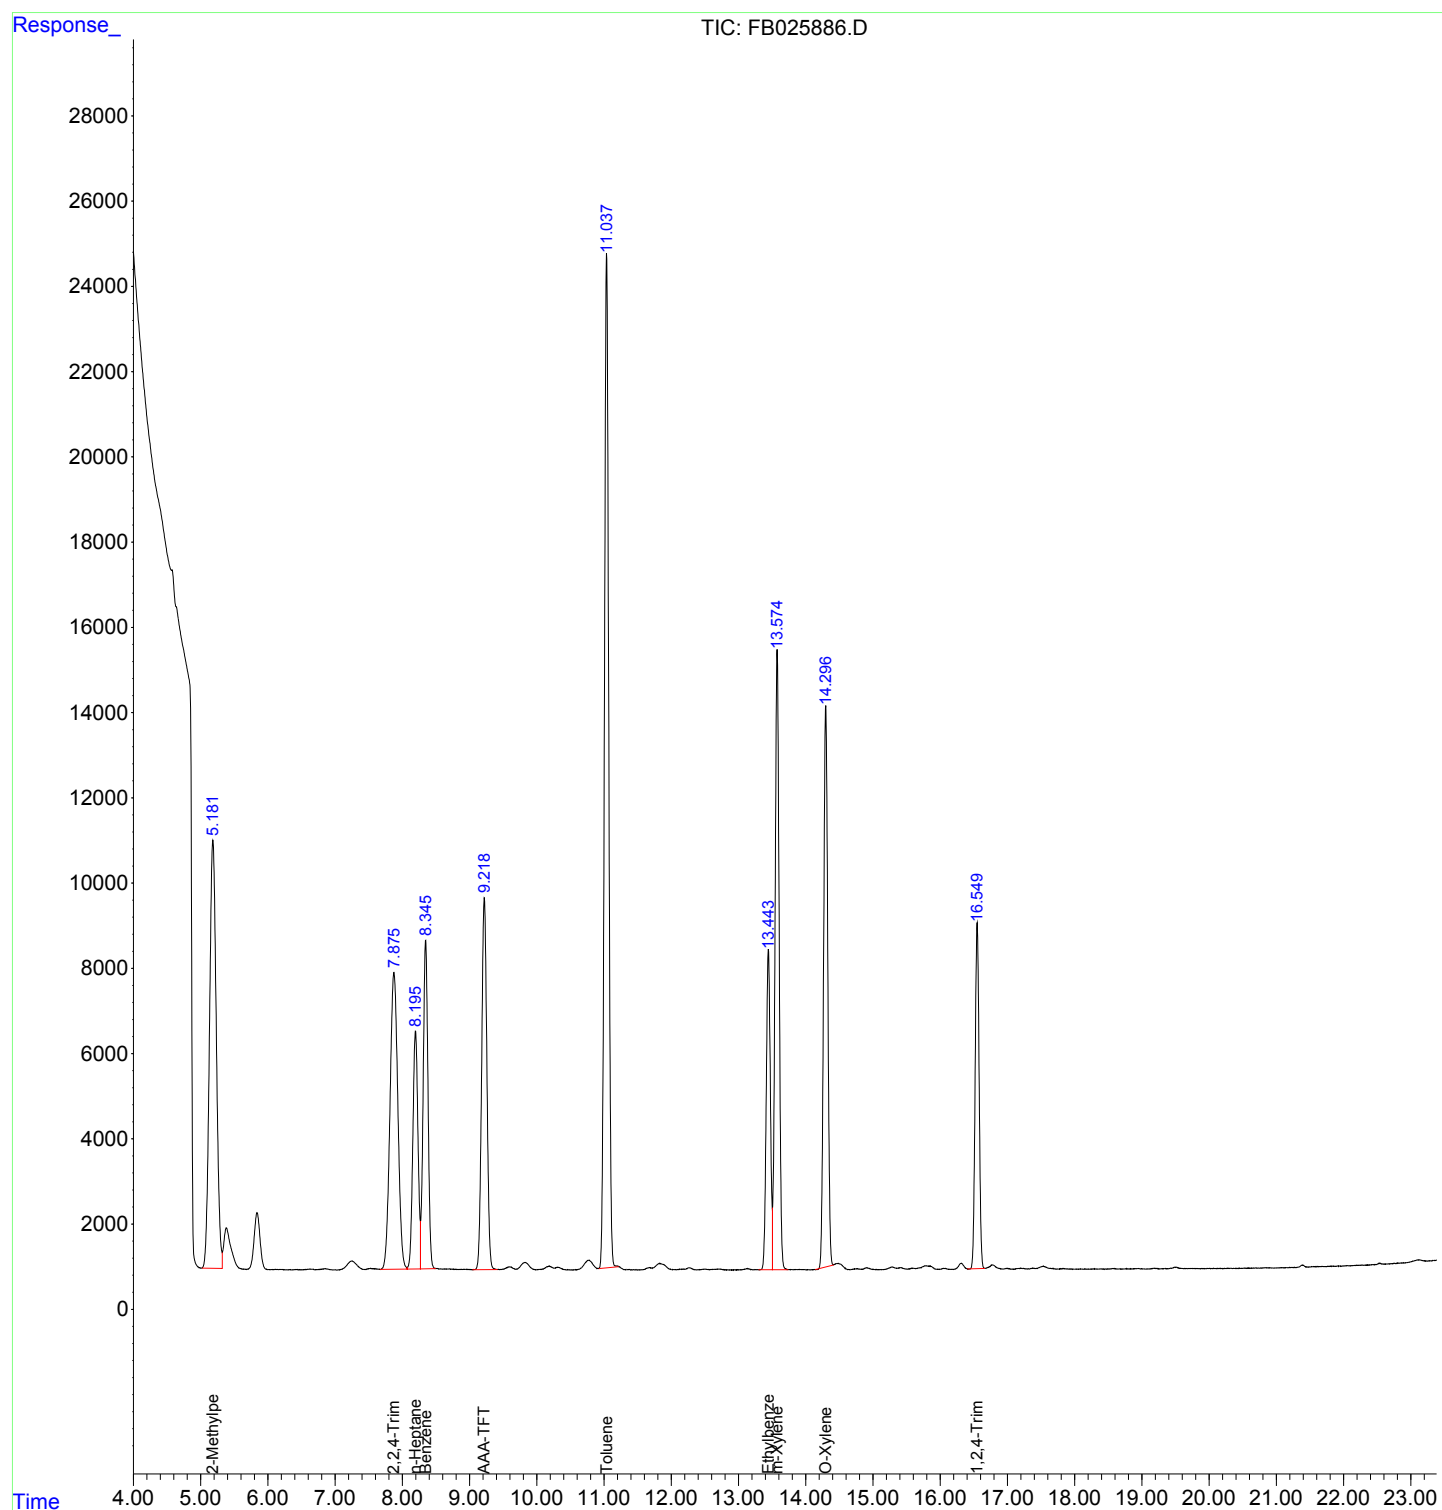

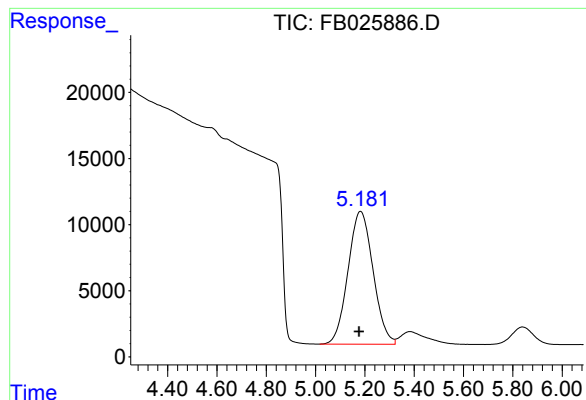


#1 2-Methylpentane

R.T.: 5.182 min
Delta R.T.: 0.005 min
Response: 708661
Conc: 26.93 ng/ml

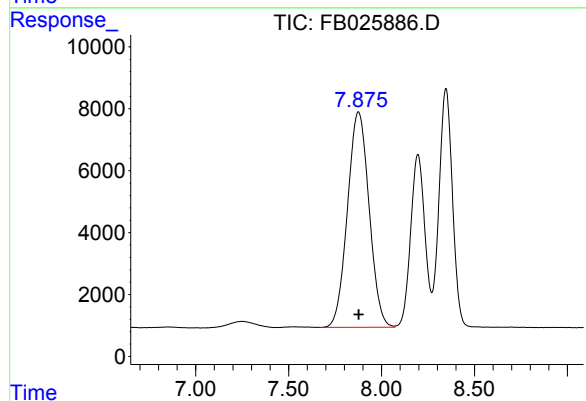


#2 2,2,4-Trimethylpentane

R.T.: 7.876 min
Delta R.T.: -0.002 min
Response: 562933
Conc: 27.94 ng/ml

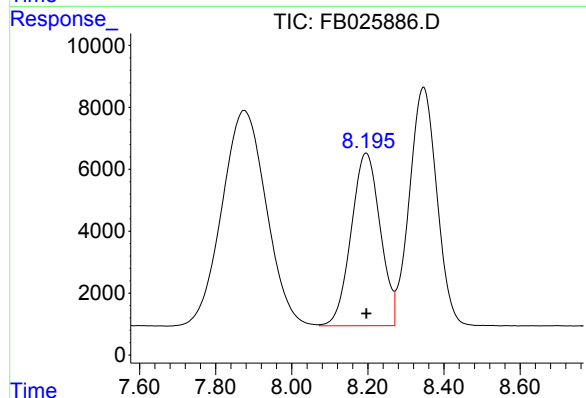


#3 n-Heptane

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 295225
Conc: 8.21 ng/ml

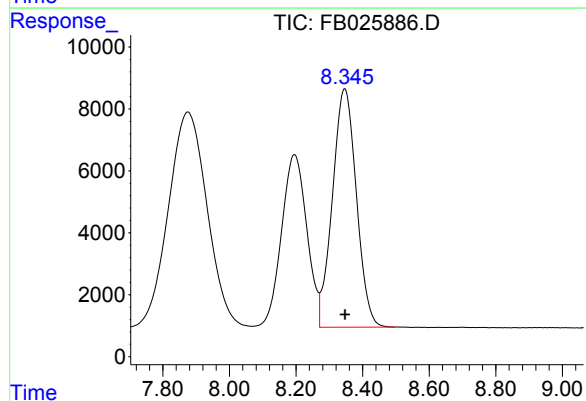


#4 Benzene

R.T.: 8.347 min
Delta R.T.: 0.000 min
Response: 384603
Conc: 9.21 ng/ml

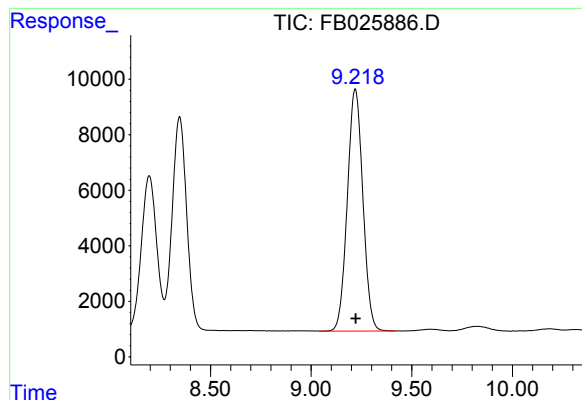


#5 AAA-TFT

R.T.: 9.219 min
Delta R.T.: -0.002 min
Response: 467193
Conc: 19.33 ng/ml

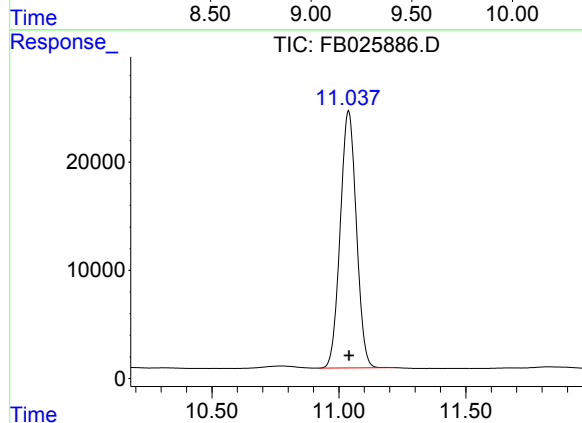


#6 Toluene

R.T.: 11.038 min
Delta R.T.: -0.003 min
Response: 1050714
Conc: 25.53 ng/ml

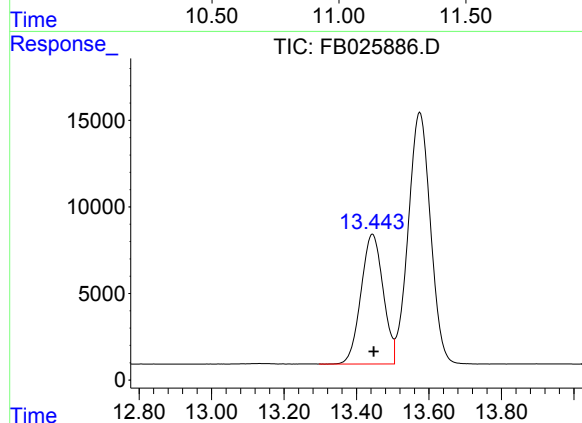


#7 Ethylbenzene

R.T.: 13.445 min
Delta R.T.: -0.004 min
Response: 318528
Conc: 8.36 ng/ml

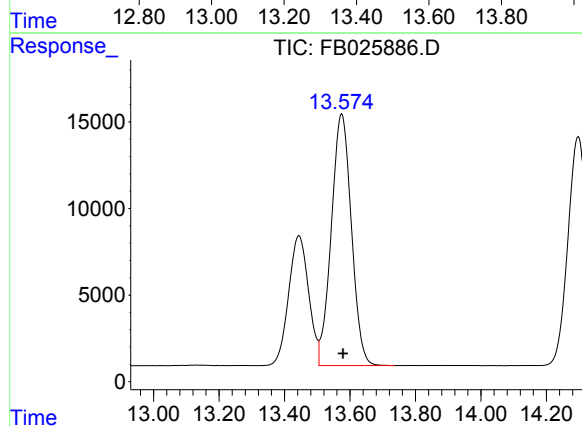


#8 m-Xylene

R.T.: 13.575 min
Delta R.T.: -0.004 min
Response: 619832
Conc: 15.77 ng/ml

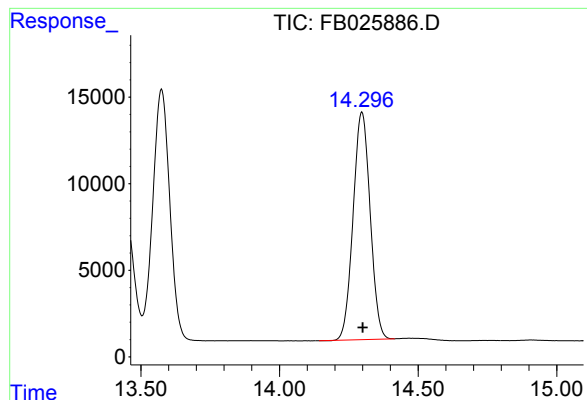

#9 O-Xylene

R.T.: 14.298 min
Delta R.T.: -0.003 min
Response: 561747
Conc: 17.62 ng/ml

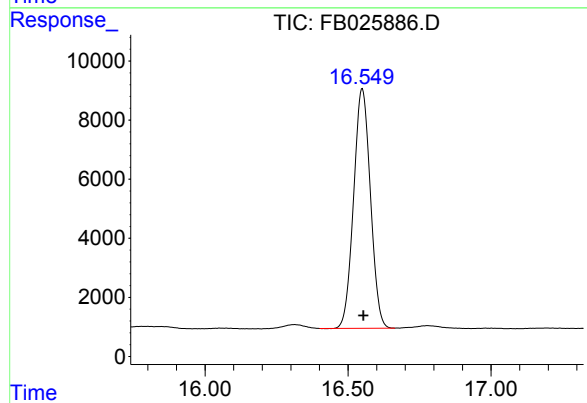

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: -0.004 min
Response: 331228
Conc: 16.83 ng/ml