

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061919\
 Data File : FB021432.D
 Signal(s) : FID2B.CH
 Acq On : 19 Jun 2019 10:32
 Operator : MJ/SJ
 Sample : BSF0619S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 19 14:56:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	267325	18.131 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	742080	19.740 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	903734	26.463 ng/ml
3) t n-Heptane	7.948	257813	7.908 ng/ml
4) t Benzene	8.089	358328	10.381 ng/ml
6) t Toluene	10.833	737653	31.122 ng/ml
7) t Ethylbenzene	13.276	212298	9.085 ng/ml
8) t m-Xylene	13.408	464411	18.606 ng/ml
9) t O-Xylene	14.138	468589	17.963 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	468467	17.444 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061919\
Data File : FB021432.D
Signal(s) : FID2B.CH
Acq On : 19 Jun 2019 10:32
Operator : MJ/SJ
Sample : BSF0619S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 19 14:56:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

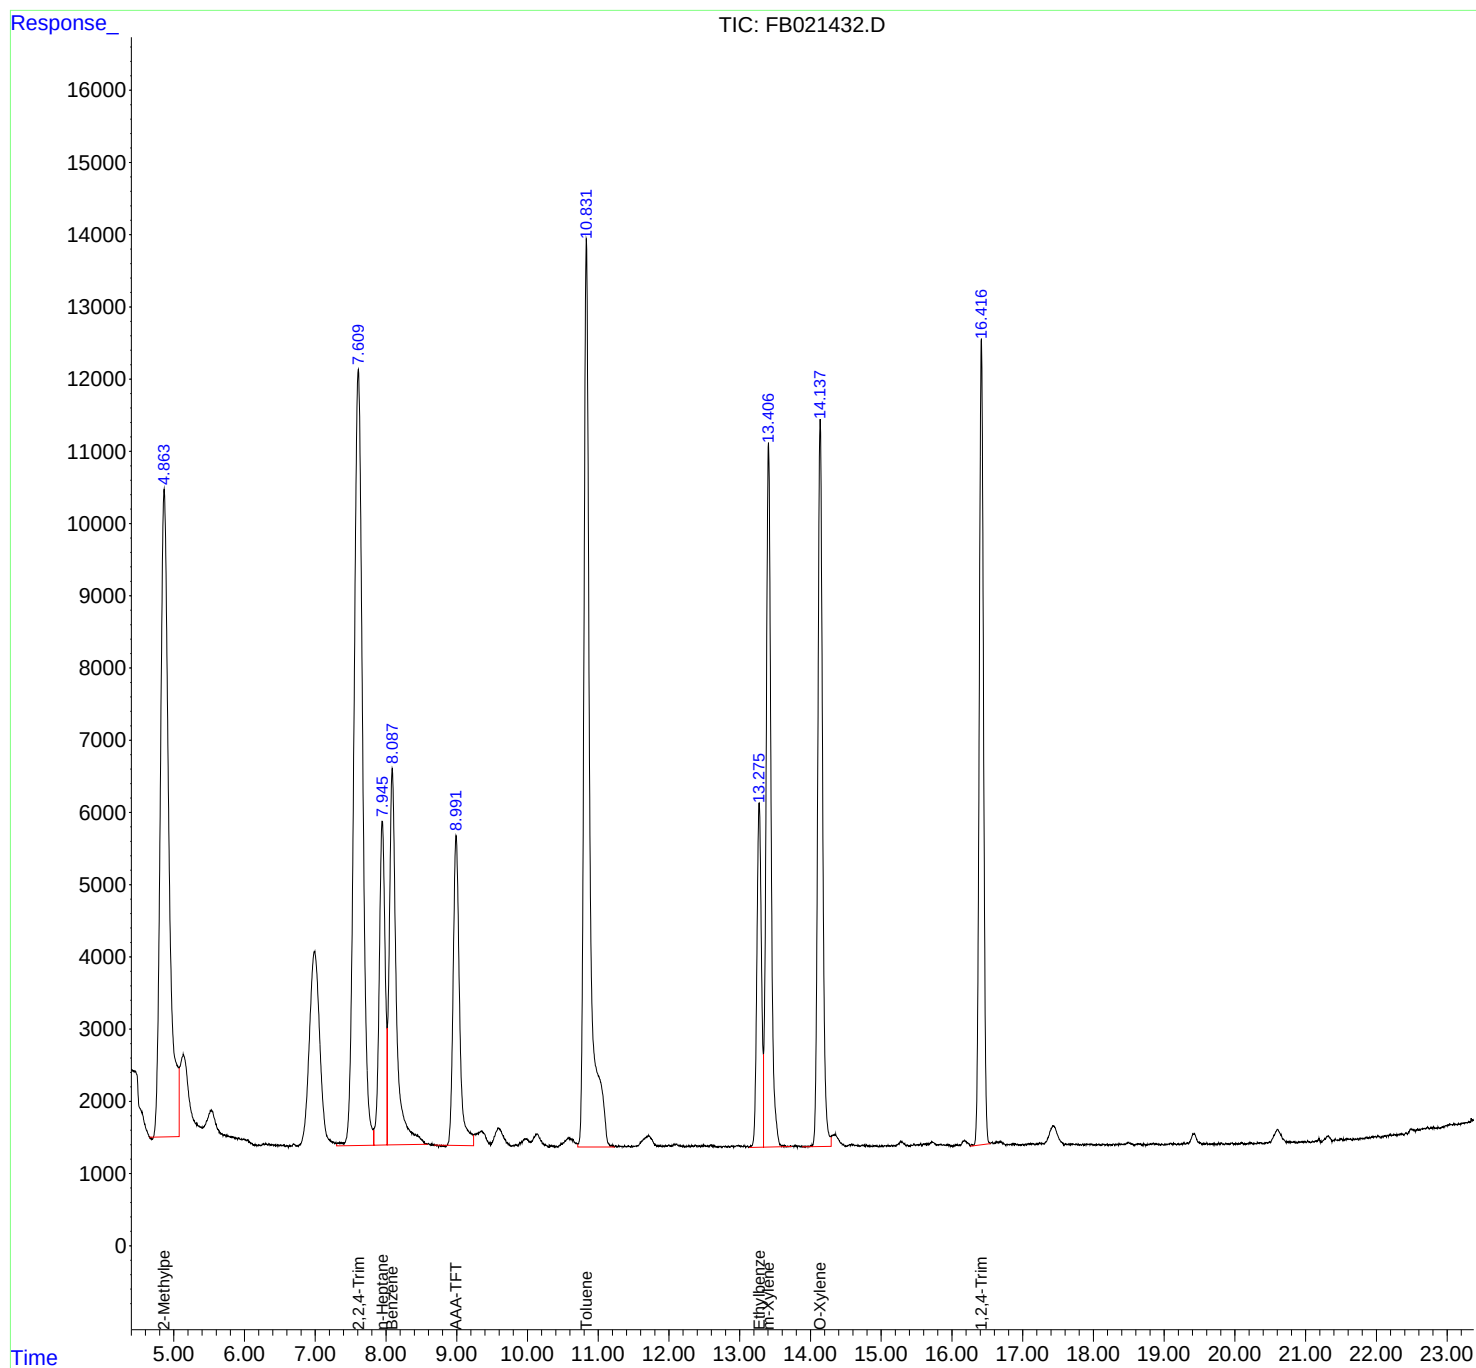

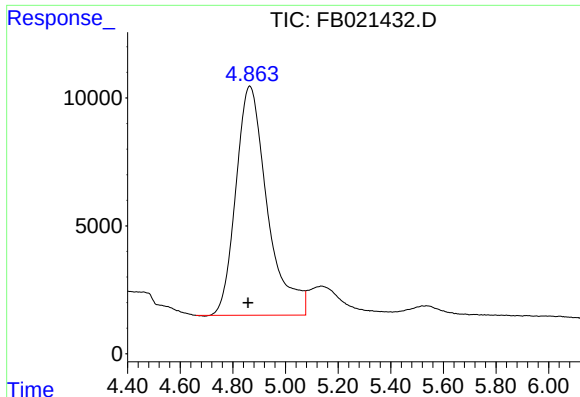


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.007 min
Response: 742080
Conc: 19.74 ng/ml

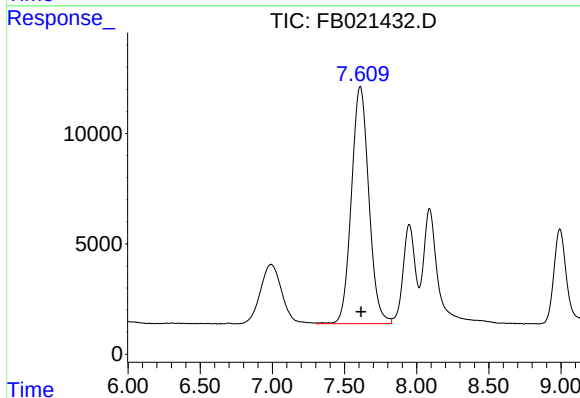


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.005 min
Response: 903734
Conc: 26.46 ng/ml

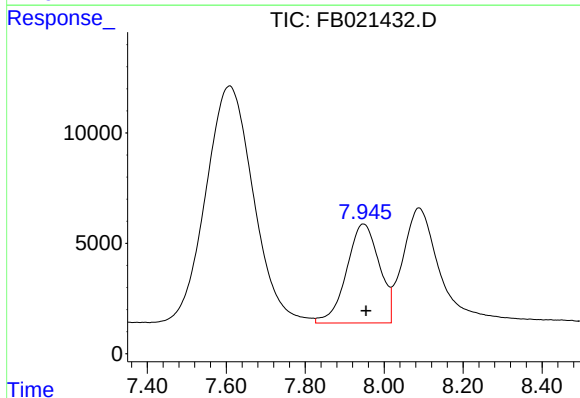


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.006 min
Response: 257813
Conc: 7.91 ng/ml

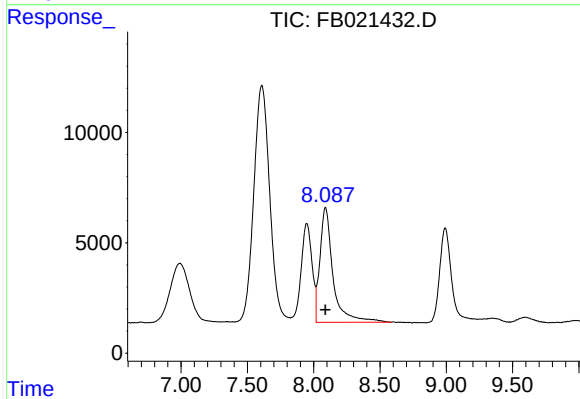


#4 Benzene

R.T.: 8.089 min
Delta R.T.: -0.001 min
Response: 358328
Conc: 10.38 ng/ml

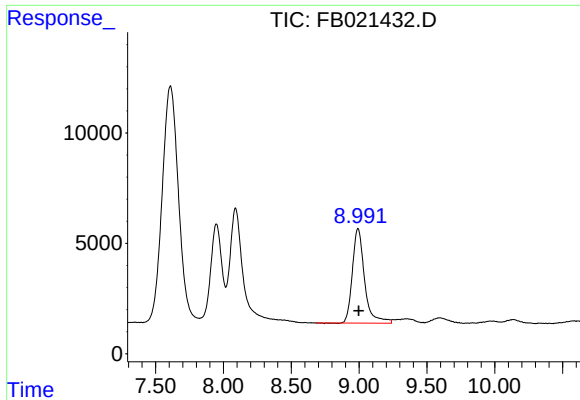


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: -0.006 min
Response: 267325
Conc: 18.13 ng/ml

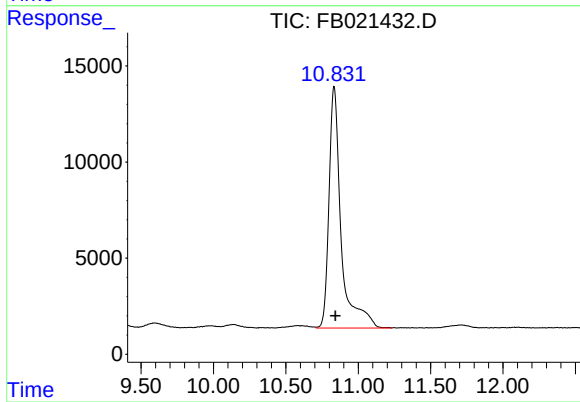


#6 Toluene

R.T.: 10.833 min
Delta R.T.: -0.010 min
Response: 737653
Conc: 31.12 ng/ml

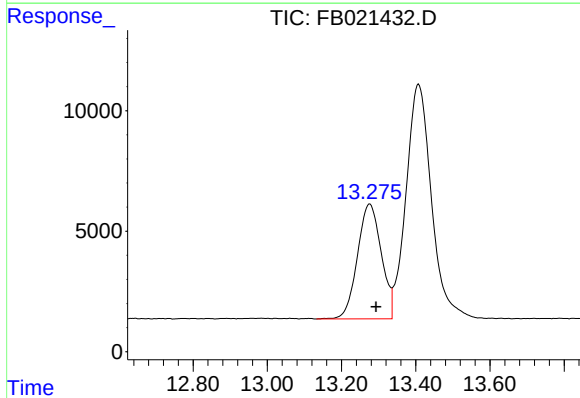


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.017 min
Response: 212298
Conc: 9.09 ng/ml

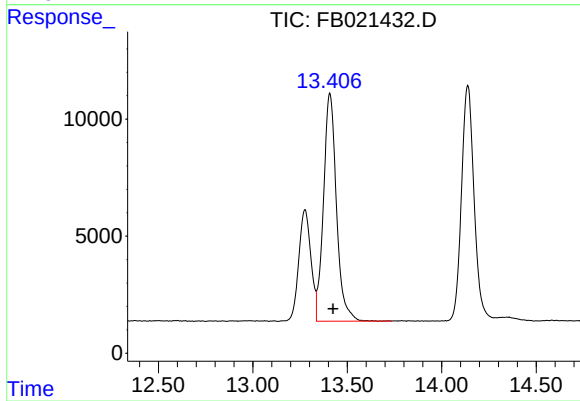

#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.018 min
Response: 464411
Conc: 18.61 ng/ml

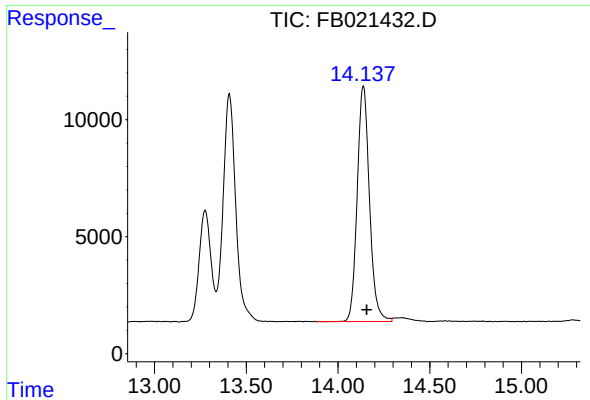


#9 O-Xylene

R.T.: 14.138 min

Delta R.T.: -0.019 min

Response: 468589

Conc: 17.96 ng/ml

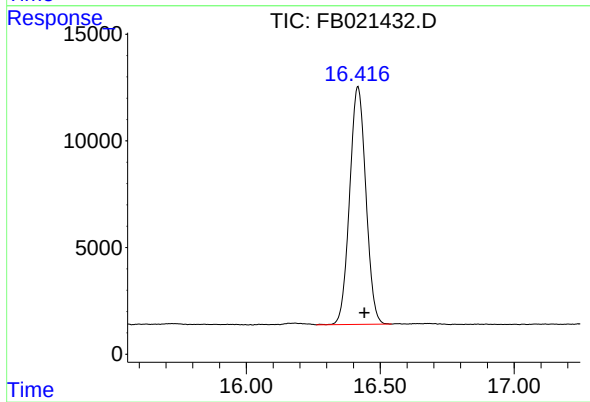

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min

Delta R.T.: -0.024 min

Response: 468467

Conc: 17.44 ng/ml