

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061919\
 Data File : FB021437.D
 Signal(s) : FID2B.CH
 Acq On : 19 Jun 2019 13:19
 Operator : MJ/SJ
 Sample : K3369-06MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 19 14:56:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	255058	17.299 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.866	624907	16.623 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	756194	22.143 ng/ml
3) t	n-Heptane	7.949	219299	6.727 ng/ml
4) t	Benzene	8.090	293321	8.498 ng/ml
6) t	Toluene	10.833	667139	28.147 ng/ml
7) t	Ethylbenzene	13.276	195092	8.349 ng/ml
8) t	m-Xylene	13.408	426689	17.095 ng/ml
9) t	O-Xylene	14.138	438143	16.796 ng/ml
10) t	1,2,4-Trimethylbenzene	16.417	429639	15.998 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061919\
Data File : FB021437.D
Signal(s) : FID2B.CH
Acq On : 19 Jun 2019 13:19
Operator : MJ/SJ
Sample : K3369-06MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1


Integration File: Calibration.e
Quant Time: Jun 19 14:56:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

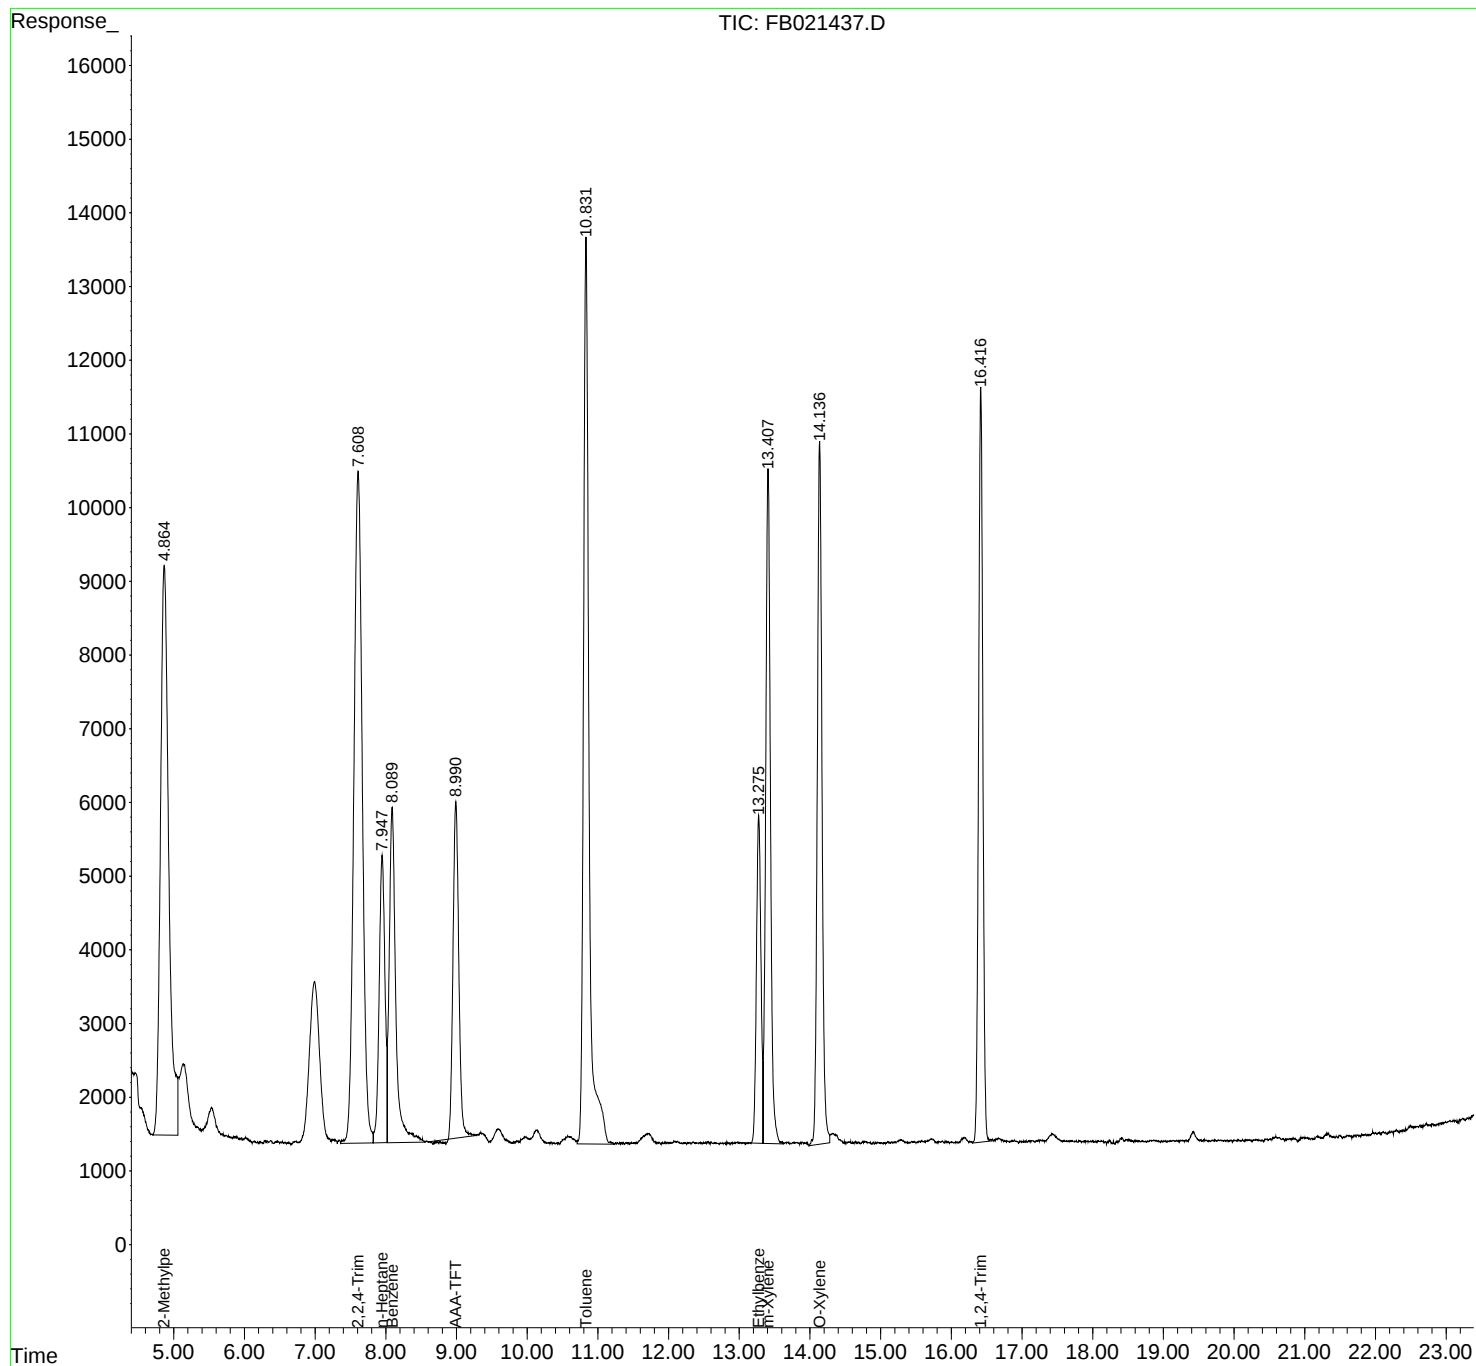


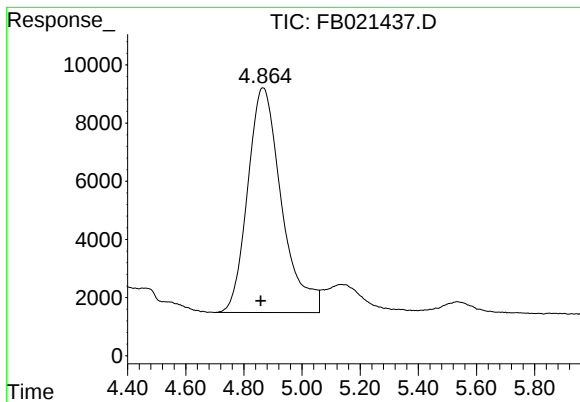


#1 2-Methylpentane
 R.T.: 4.866 min
 Delta R.T.: 0.008 min
 Response: 624907
 Conc: 16.62 ng/ml

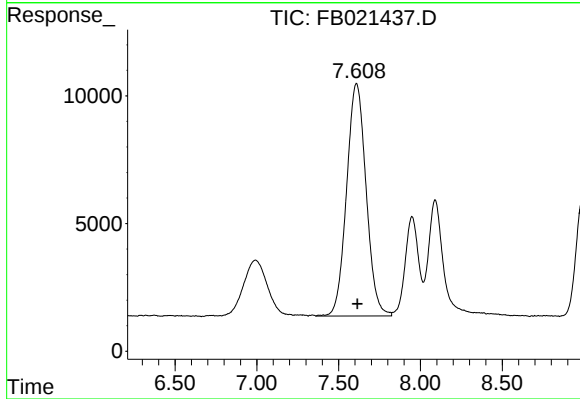


#2 2,2,4-Trimethylpentane
 R.T.: 7.609 min
 Delta R.T.: -0.005 min
 Response: 756194
 Conc: 22.14 ng/ml

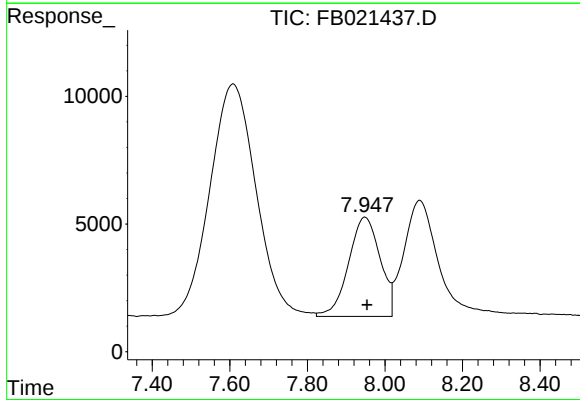

#3 n-Heptane
 R.T.: 7.949 min
 Delta R.T.: -0.005 min
 Response: 219299
 Conc: 6.73 ng/ml

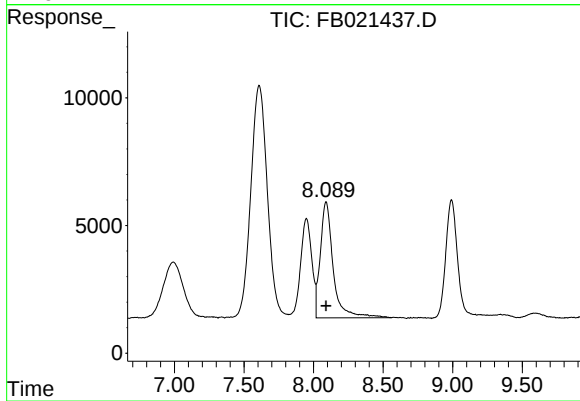


#4 Benzene
 R.T.: 8.090 min
 Delta R.T.: 0.000 min
 Response: 293321
 Conc: 8.50 ng/ml

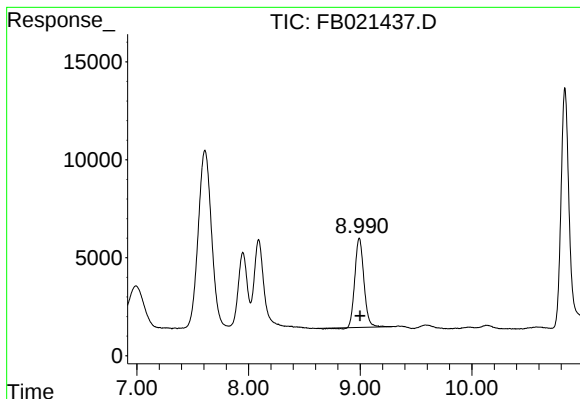


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: -0.007 min
Response: 255058
Conc: 17.30 ng/ml

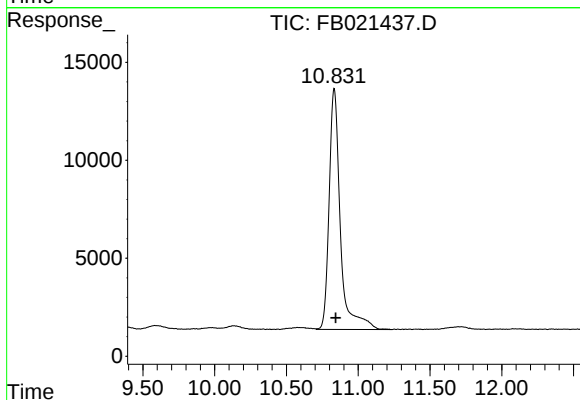


#6 Toluene

R.T.: 10.833 min
Delta R.T.: -0.010 min
Response: 667139
Conc: 28.15 ng/ml

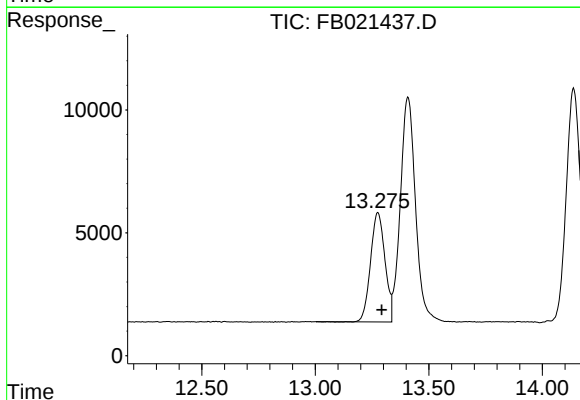


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.017 min
Response: 195092
Conc: 8.35 ng/ml

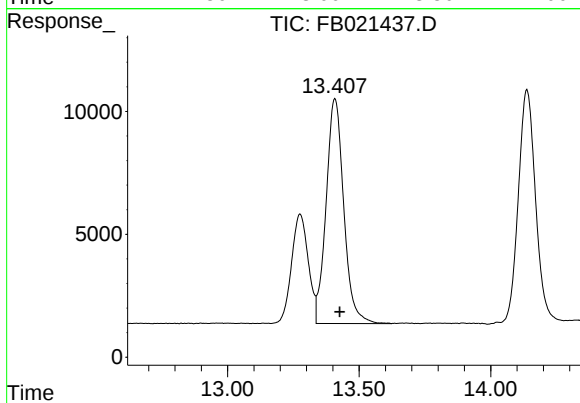


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.018 min
Response: 426689
Conc: 17.09 ng/ml

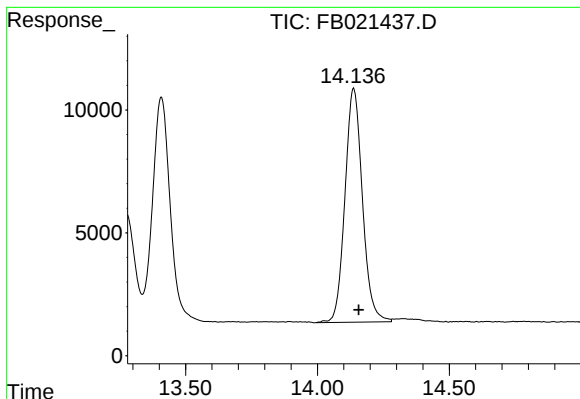

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.019 min
Response: 438143
Conc: 16.80 ng/ml

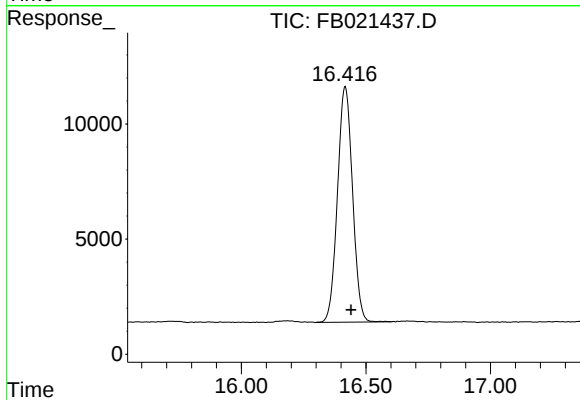

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.024 min
Response: 429639
Conc: 16.00 ng/ml