

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062019\
 Data File : FB021442.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jun 2019 9:26
 Operator : MJ/SJ
 Sample : BSF0620S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 21 00:38:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	307954	20.887 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.867	776809	20.663 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	977255	28.616 ng/ml
3) t n-Heptane	7.949	282977	8.680 ng/ml
4) t Benzene	8.091	383422	11.108 ng/ml
6) t Toluene	10.834	754229	31.821 ng/ml
7) t Ethylbenzene	13.277	217929	9.326 ng/ml
8) t m-Xylene	13.409	472508	18.931 ng/ml
9) t O-Xylene	14.139	491420	18.838 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	498698	18.570 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062019\
Data File : FB021442.D
Signal(s) : FID2B.CH
Acq On : 20 Jun 2019 9:26
Operator : MJ/SJ
Sample : BSF0620S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 21 00:38:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

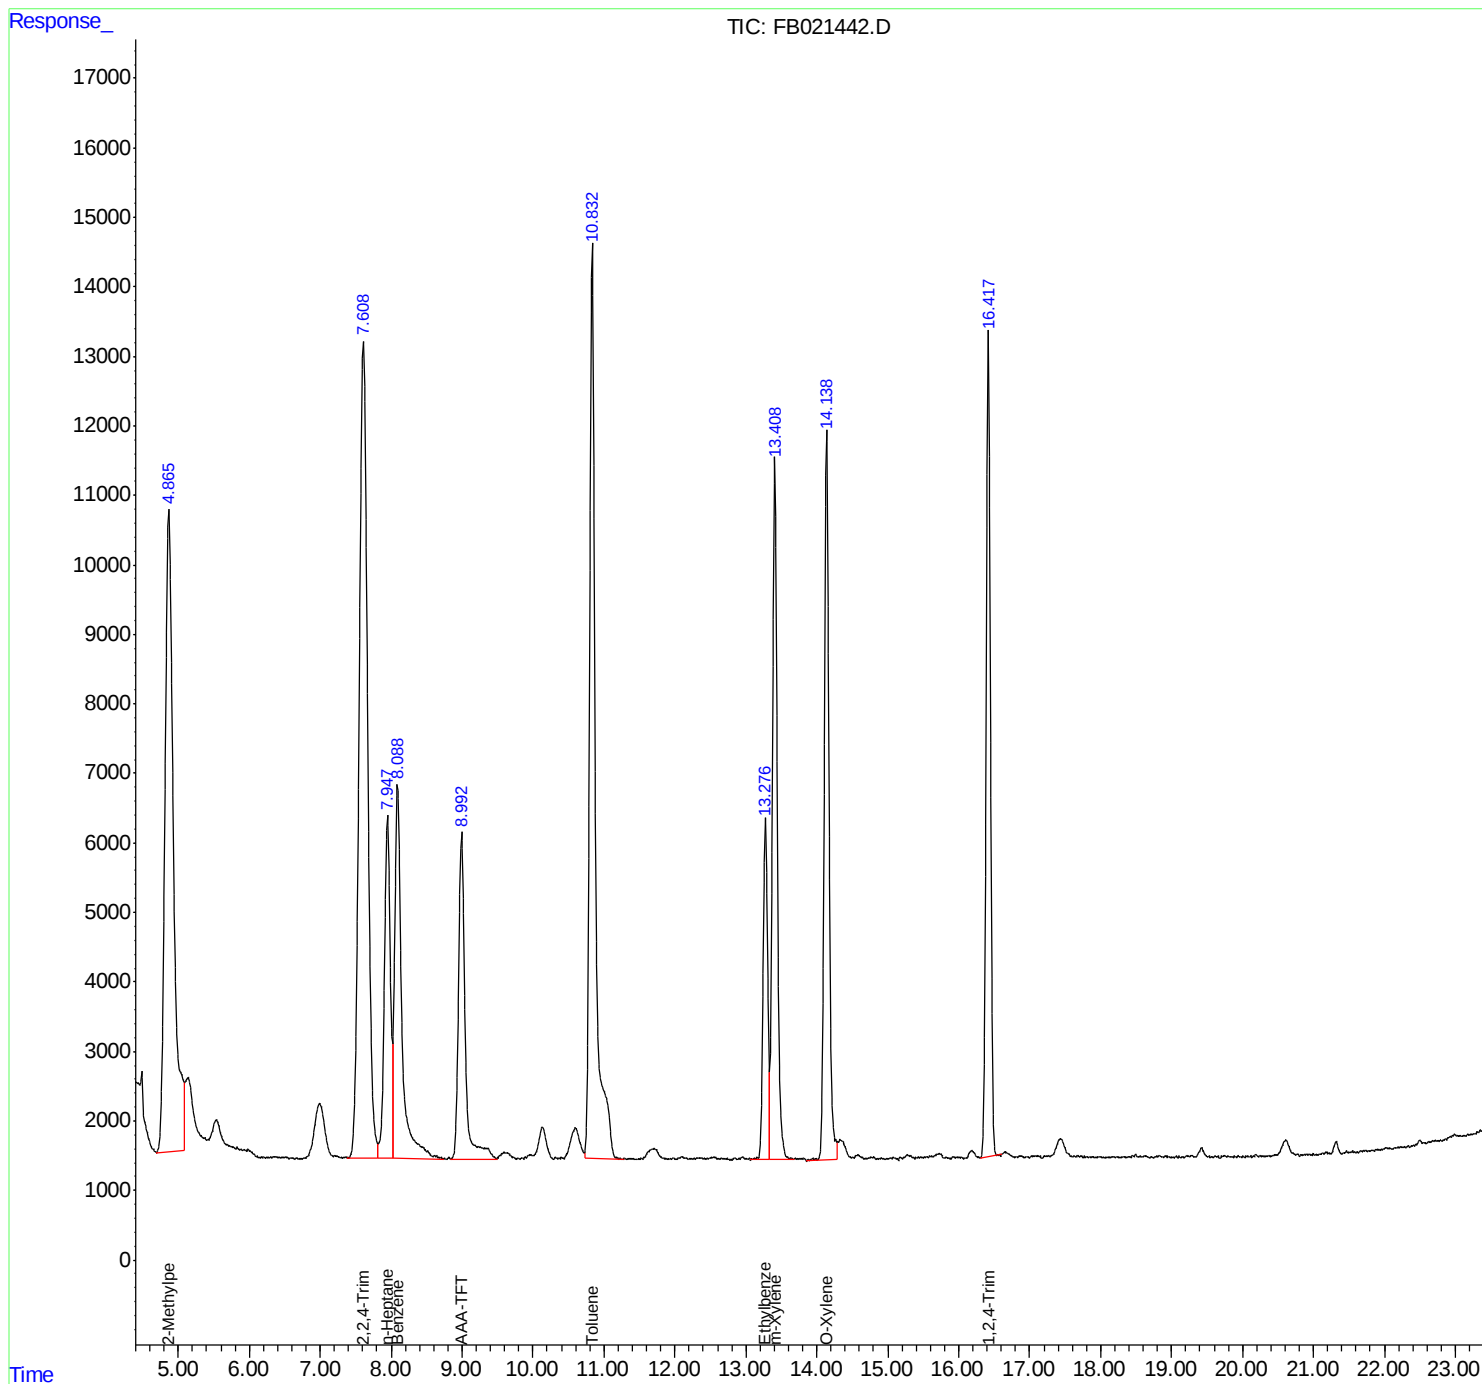

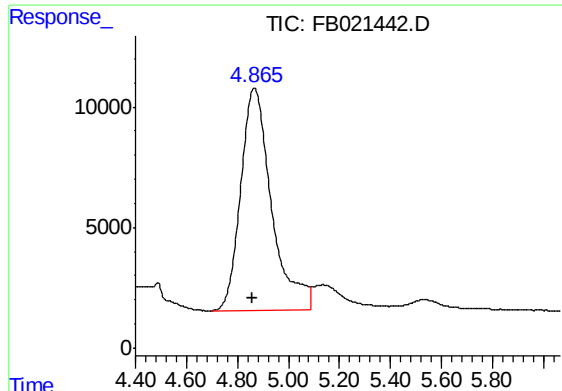


#1 2-Methylpentane

R.T.: 4.867 min
Delta R.T.: 0.009 min
Response: 776809
Conc: 20.66 ng/ml

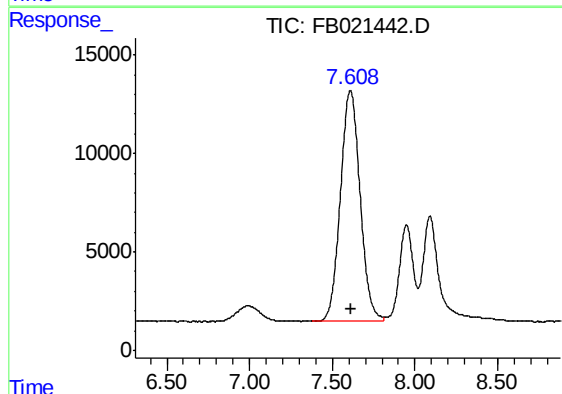


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.004 min
Response: 977255
Conc: 28.62 ng/ml

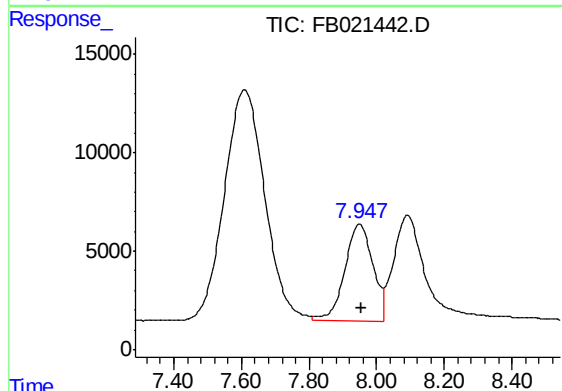


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.005 min
Response: 282977
Conc: 8.68 ng/ml

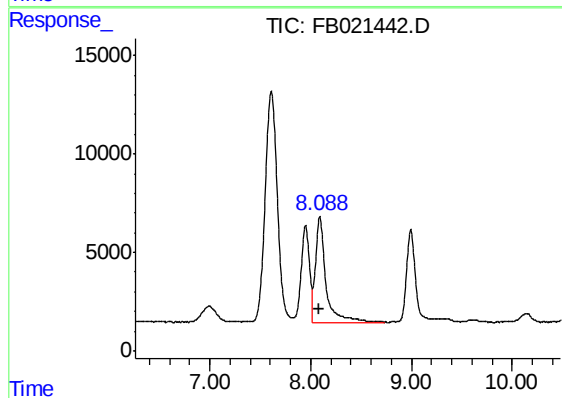


#4 Benzene

R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 383422
Conc: 11.11 ng/ml

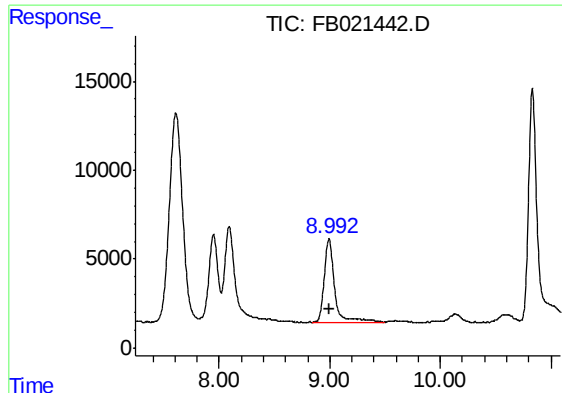


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: -0.005 min
Response: 307954
Conc: 20.89 ng/ml

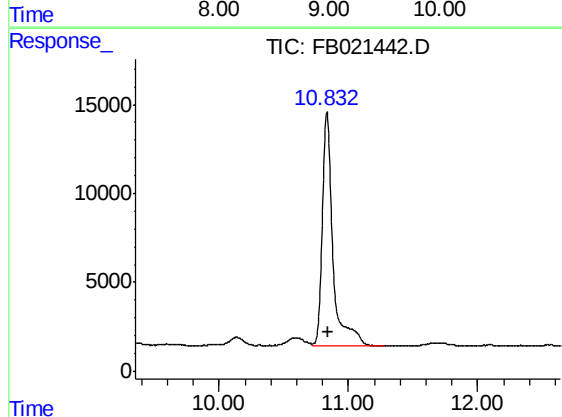


#6 Toluene

R.T.: 10.834 min
Delta R.T.: -0.009 min
Response: 754229
Conc: 31.82 ng/ml

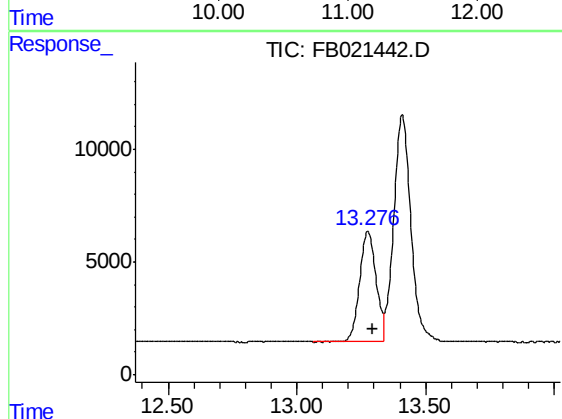


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: -0.016 min
Response: 217929
Conc: 9.33 ng/ml

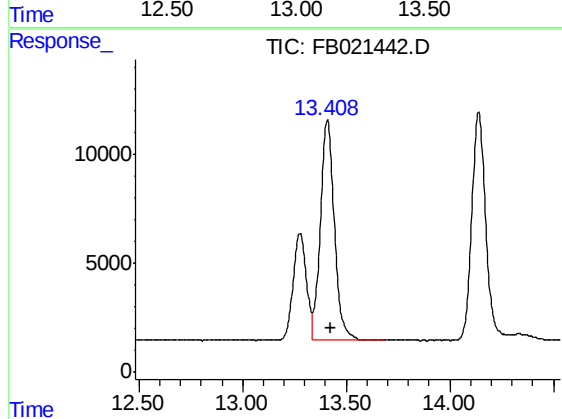


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.016 min
Response: 472508
Conc: 18.93 ng/ml

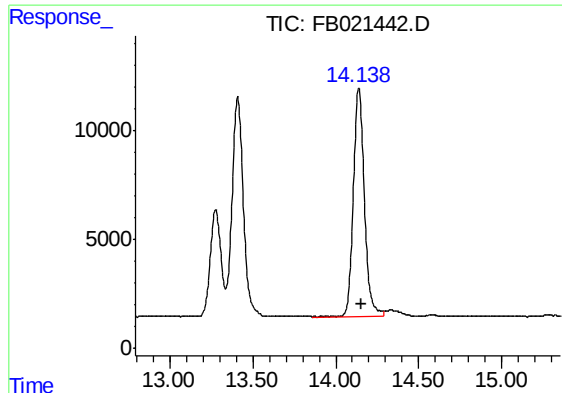

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.018 min
Response: 491420
Conc: 18.84 ng/ml

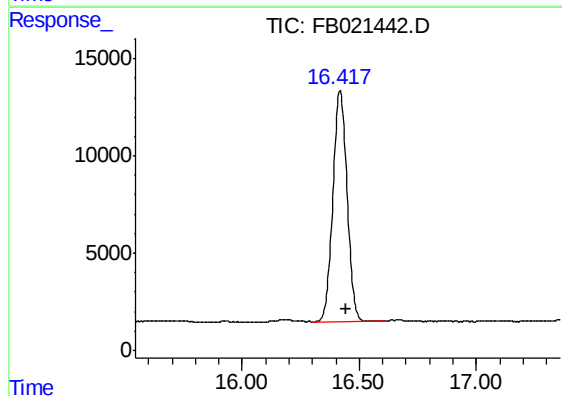

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.023 min
Response: 498698
Conc: 18.57 ng/ml