

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062019\
 Data File : FB021450.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jun 2019 13:28
 Operator : MJ/SJ
 Sample : K3455-05MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 21 00:39:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	280736	19.041 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.871	616240	16.392 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	727699	21.309 ng/ml
3) t n-Heptane	7.951	197917	6.071 ng/ml
4) t Benzene	8.094	297314	8.614 ng/ml
6) t Toluene	10.837	662598	27.955 ng/ml
7) t Ethylbenzene	13.279	187445	8.022 ng/ml
8) t m-Xylene	13.411	415337	16.640 ng/ml
9) t O-Xylene	14.140	436902	16.748 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	450328	16.768 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062019\
Data File : FB021450.D
Signal(s) : FID2B.CH
Acq On : 20 Jun 2019 13:28
Operator : MJ/SJ
Sample : K3455-05MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 21 00:39:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

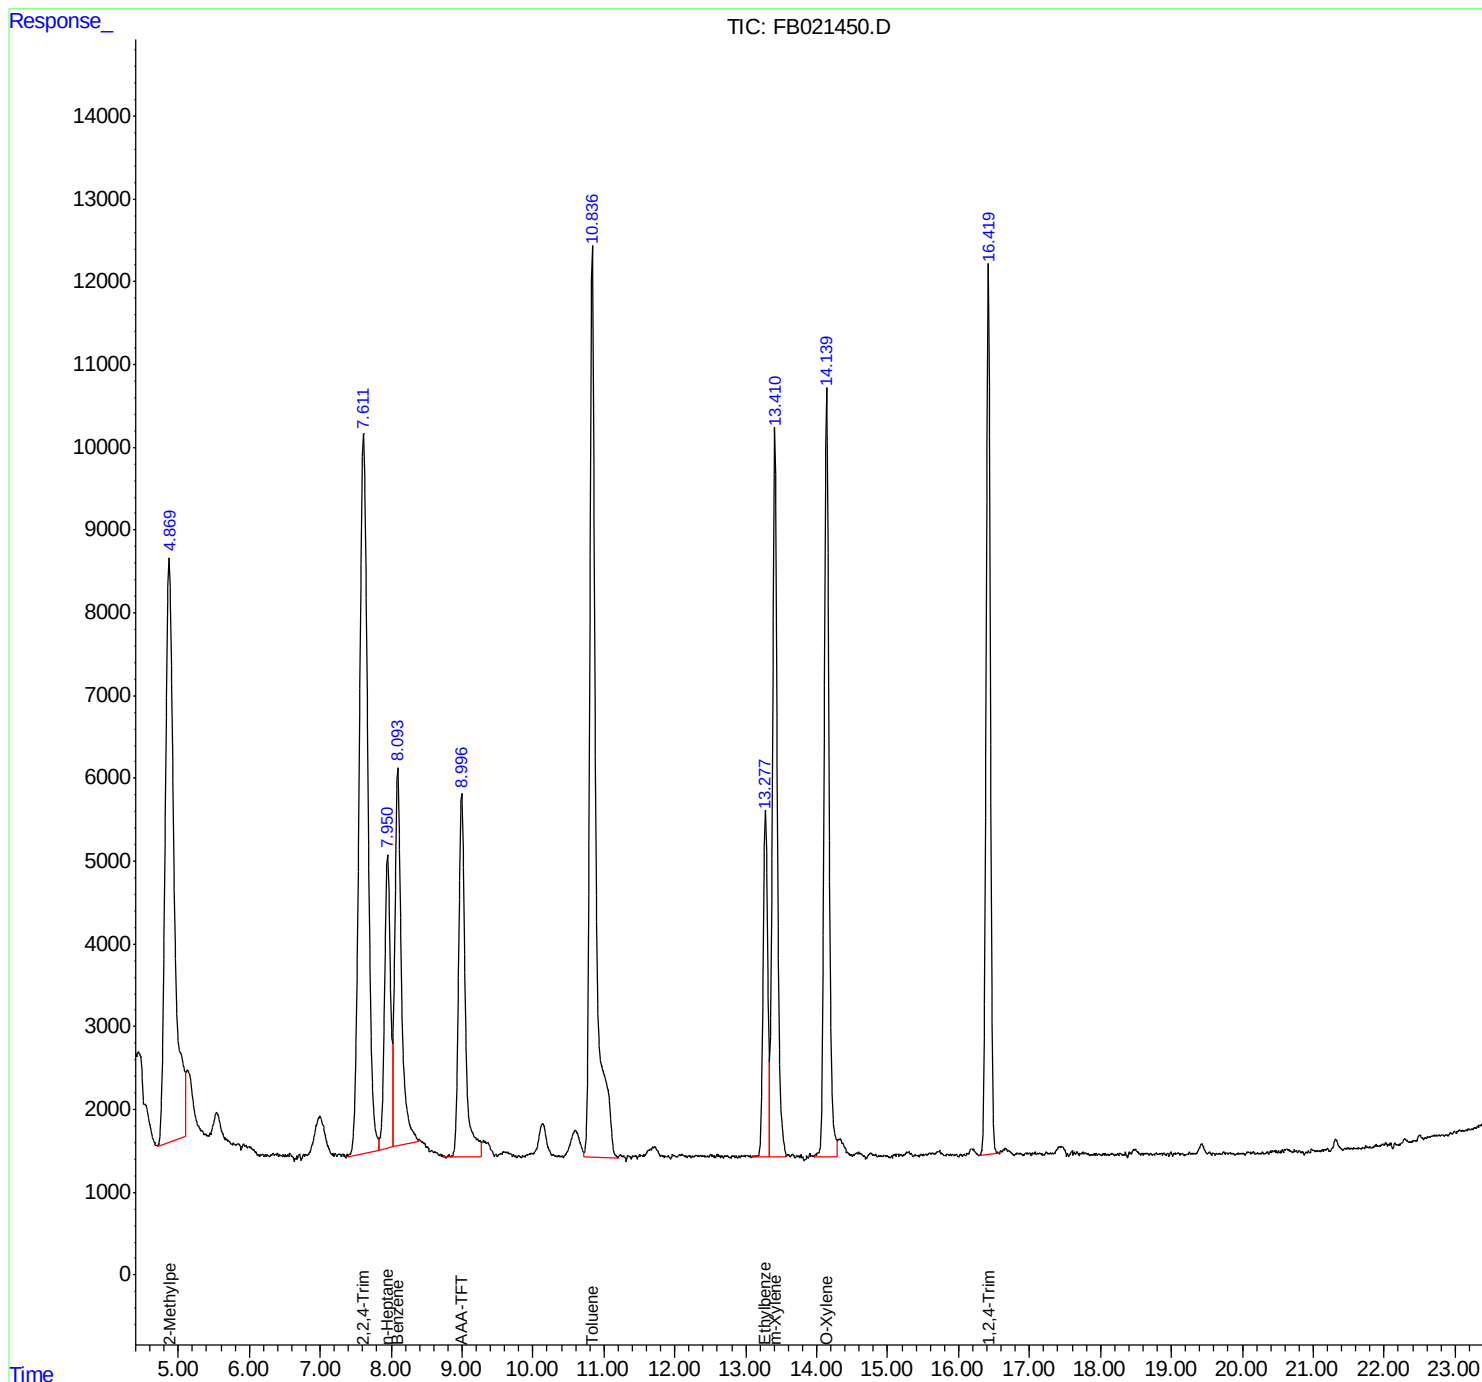

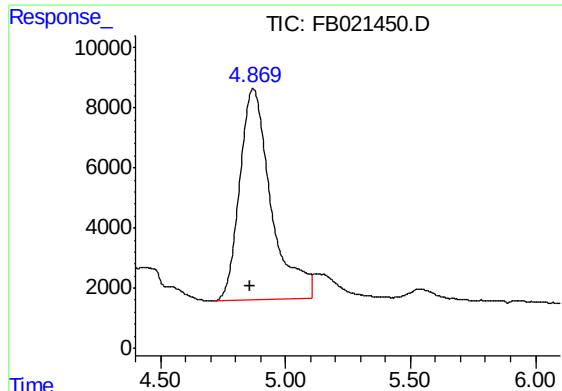


#1 2-Methylpentane

R.T.: 4.871 min
Delta R.T.: 0.013 min
Response: 616240
Conc: 16.39 ng/ml

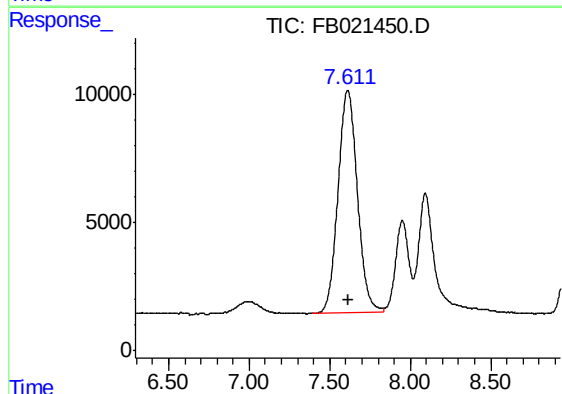


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 727699
Conc: 21.31 ng/ml

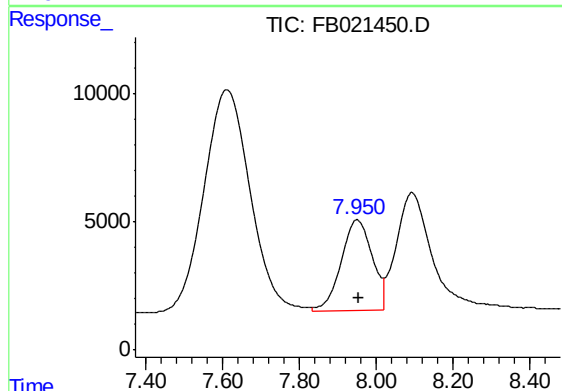


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.003 min
Response: 197917
Conc: 6.07 ng/ml

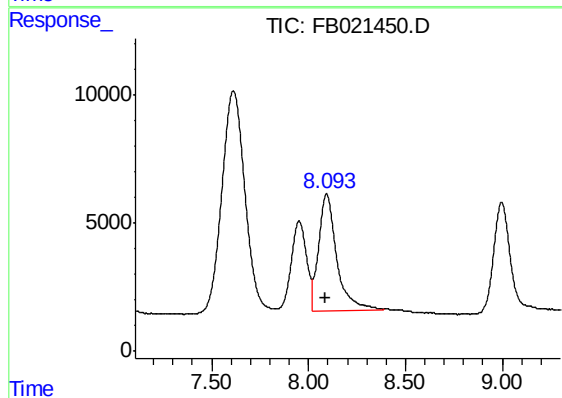


#4 Benzene

R.T.: 8.094 min
Delta R.T.: 0.004 min
Response: 297314
Conc: 8.61 ng/ml

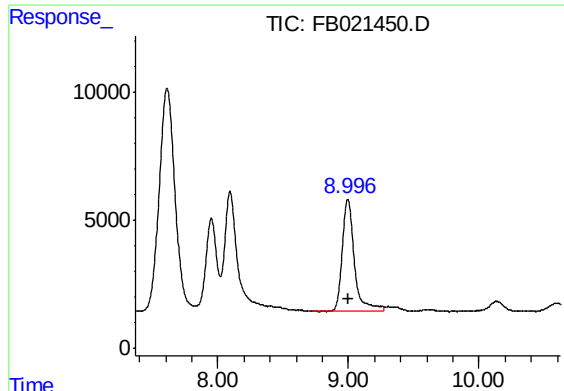


#5 AAA-TFT

R.T.: 8.996 min
Delta R.T.: -0.002 min
Response: 280736
Conc: 19.04 ng/ml

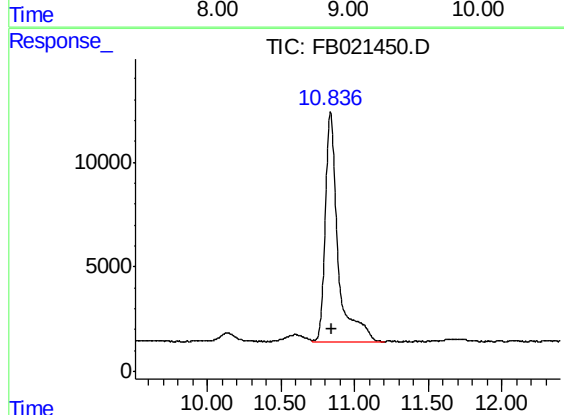


#6 Toluene

R.T.: 10.837 min
Delta R.T.: -0.006 min
Response: 662598
Conc: 27.96 ng/ml

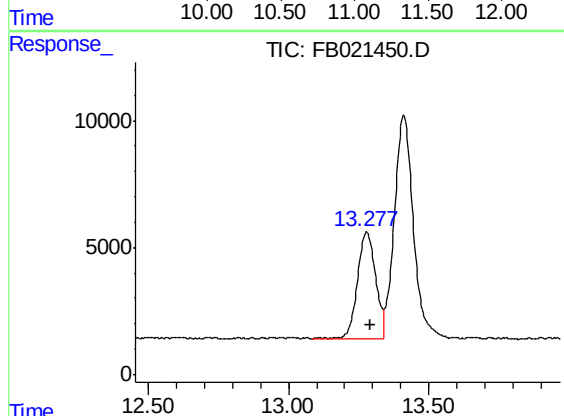


#7 Ethylbenzene

R.T.: 13.279 min
Delta R.T.: -0.014 min
Response: 187445
Conc: 8.02 ng/ml

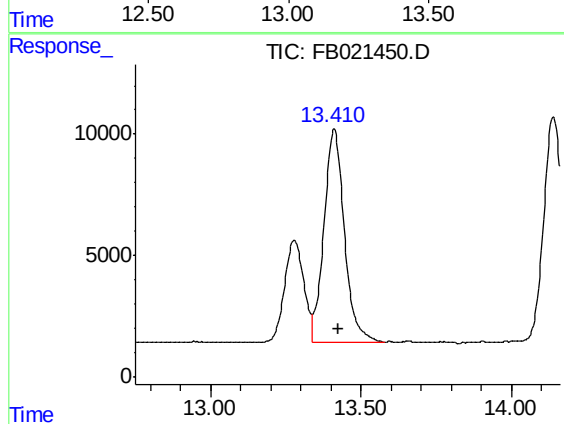


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: -0.015 min
Response: 415337
Conc: 16.64 ng/ml

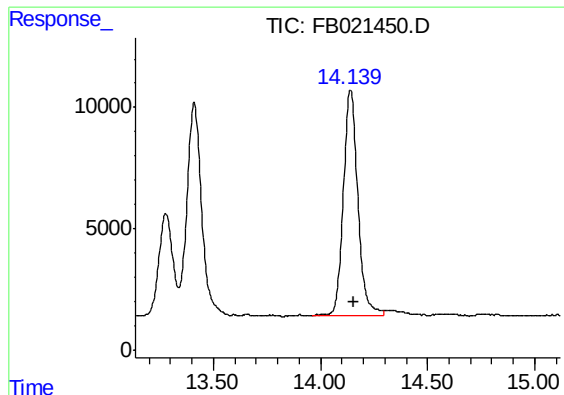

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: -0.017 min
Response: 436902
Conc: 16.75 ng/ml

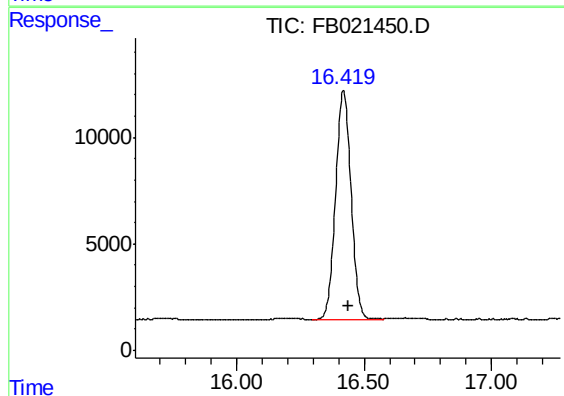

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: -0.021 min
Response: 450328
Conc: 16.77 ng/ml