

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
 Data File : FB027465.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jun 2022 15:57
 Operator : AJ/MA
 Sample : N3373-13
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 21 01:11:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	167040	14.892 ng/ml
Target Compounds			
9) t O-Xylene	13.872	5087	0.293 ng/ml
10) t 1,2,4-Trimethylbenzene	16.143	9556	0.556 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
Data File : FB027465.D
Signal(s) : FID2B.CH
Acq On : 20 Jun 2022 15:57
Operator : AJ/MA
Sample : N3373-13
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 21 01:11:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

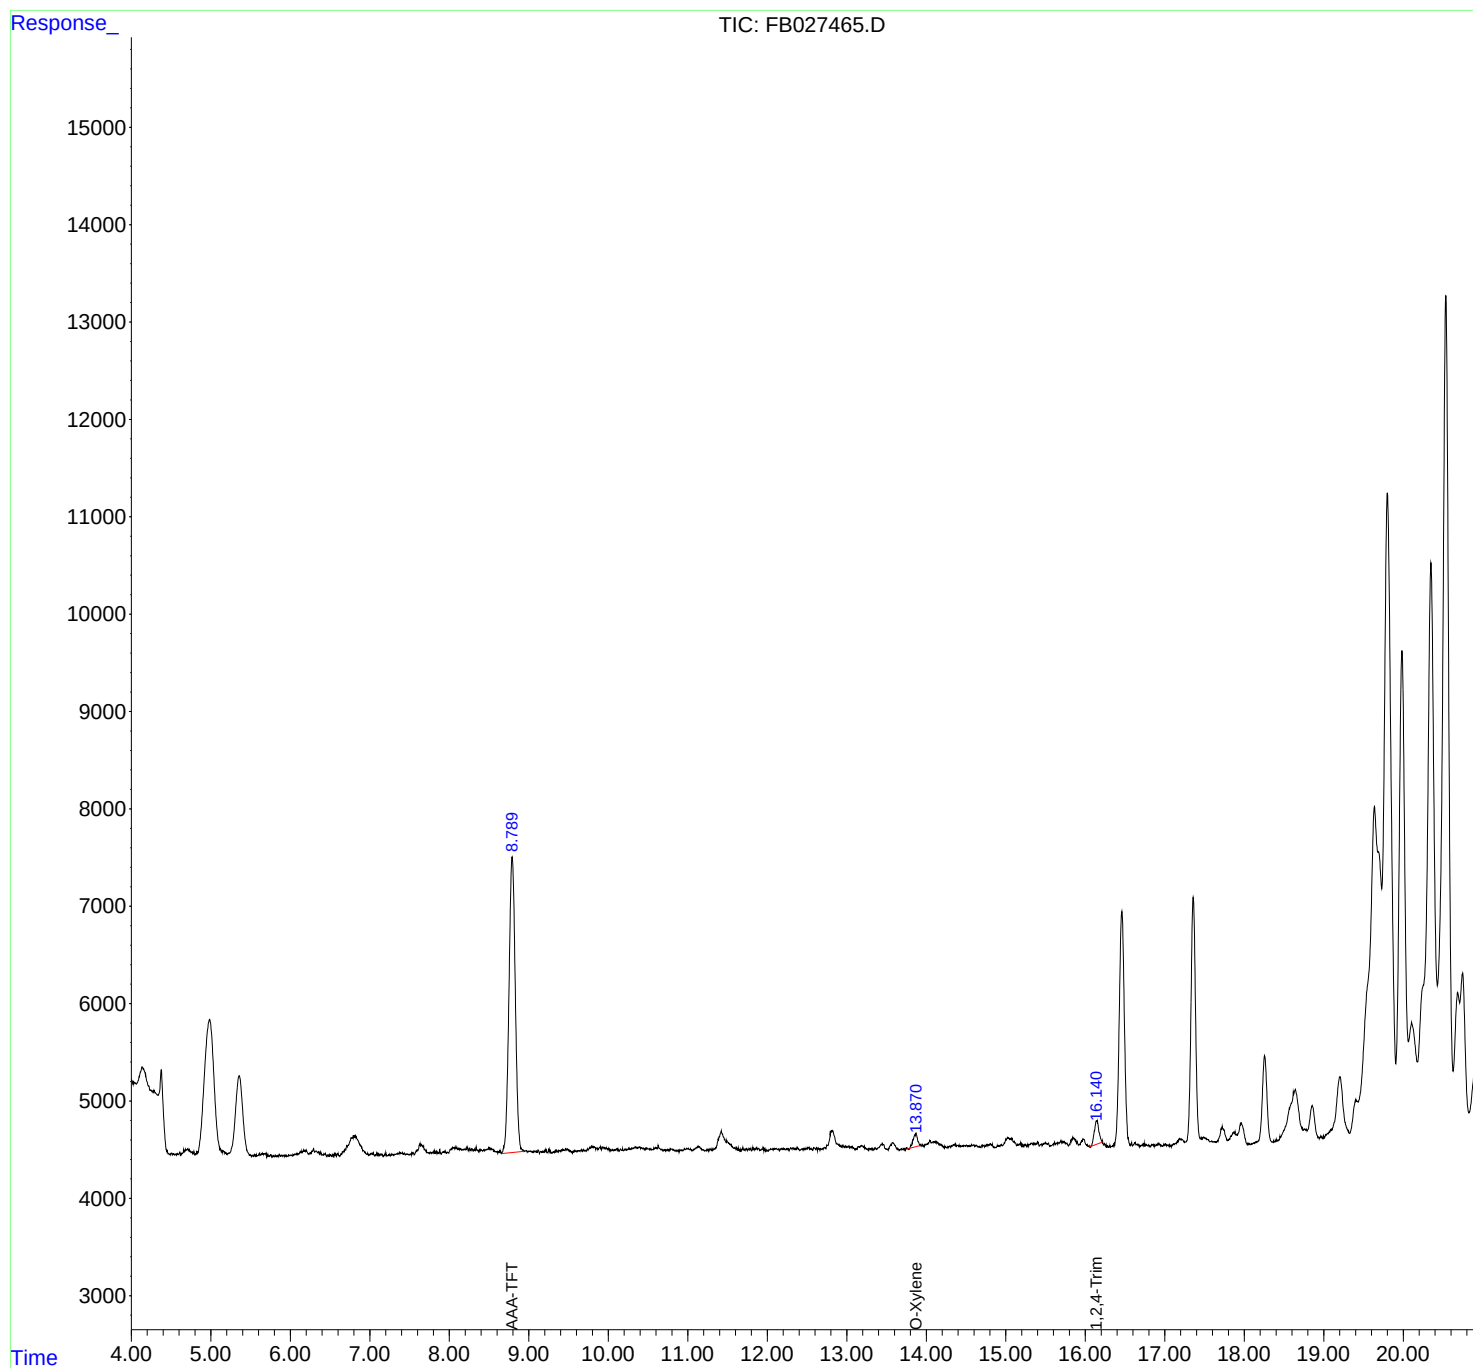


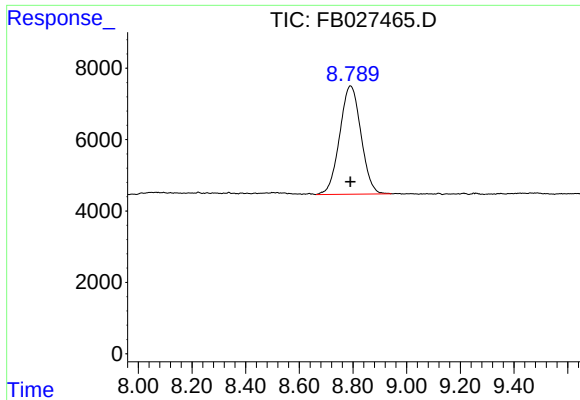

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 167040
Conc: 14.89 ng/ml

Instrument :
FID_B
ClientSampleId :

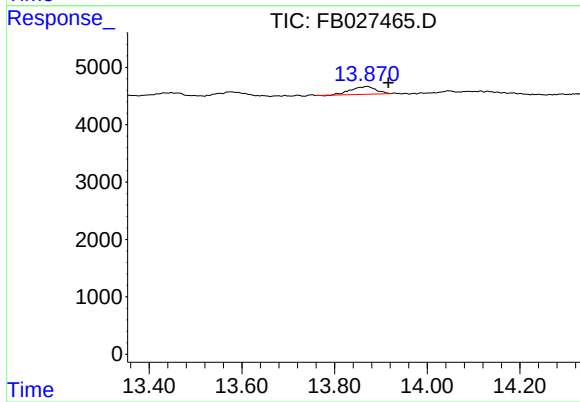

#9 O-Xylene

R.T.: 13.872 min
Delta R.T.: -0.044 min
Response: 5087
Conc: 0.29 ng/ml

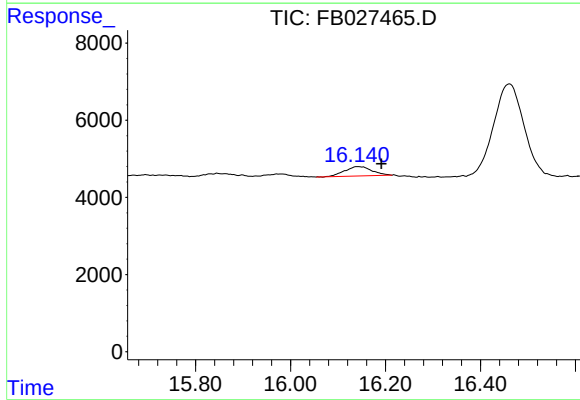

#10 1,2,4-Trimethylbenzene

R.T.: 16.143 min
Delta R.T.: -0.048 min
Response: 9556
Conc: 0.56 ng/ml