

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
 Data File : FB027460.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jun 2022 12:28
 Operator : AJ/MA
 Sample : BSF0620S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0620S1

Integration File: Calibration.e
 Quant Time: Jun 21 01:09:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	231284	20.620 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	481963	28.608 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	508075	28.936 ng/ml
3) t n-Heptane	7.748	164035	9.363 ng/ml
4) t Benzene	7.885	193624	9.495 ng/ml
6) t Toluene	10.617	551573	28.487 ng/ml
7) t Ethylbenzene	13.054	175016	9.664 ng/ml
8) t m-Xylene	13.186	344307	19.315 ng/ml
9) t O-Xylene	13.913	335243	19.293 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	341378	19.873 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
Data File : FB027460.D
Signal(s) : FID2B.CH
Acq On : 20 Jun 2022 12:28
Operator : AJ/MA
Sample : BSF0620S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0620S1

Integration File: Calibration.e
Quant Time: Jun 21 01:09:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

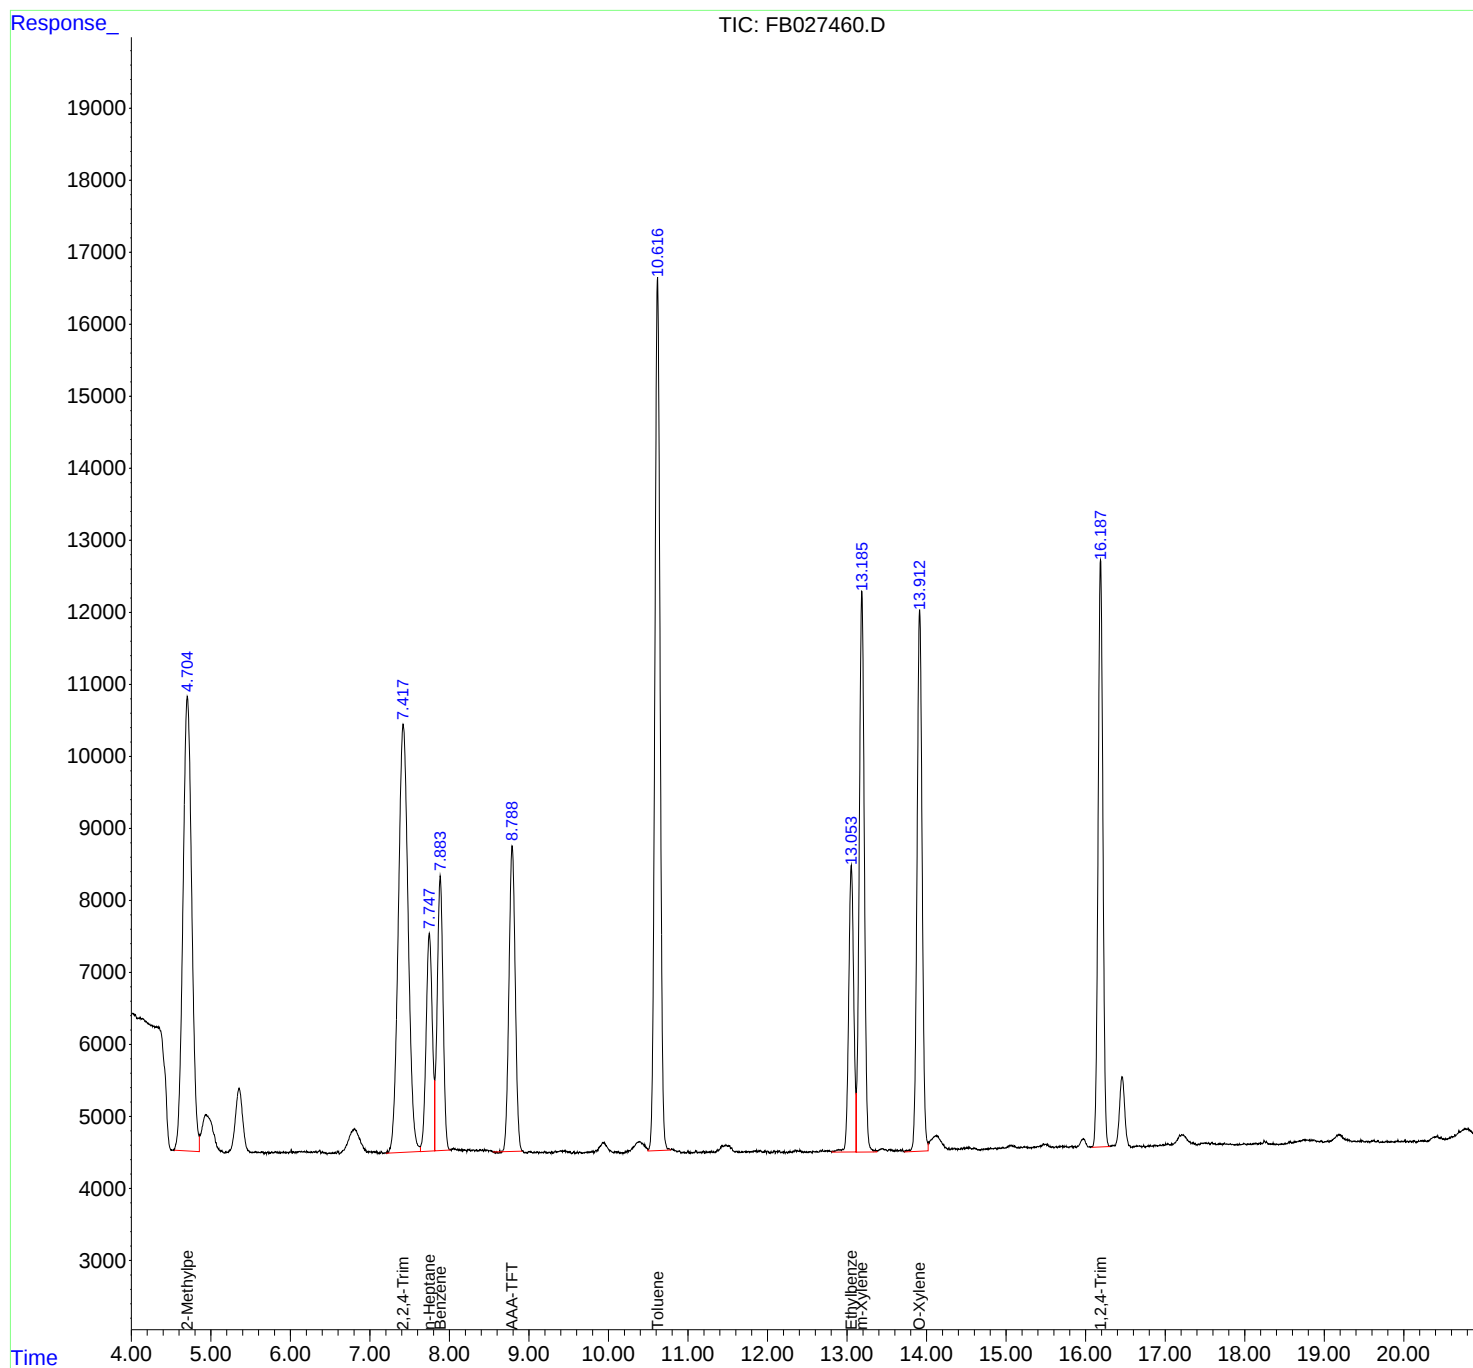


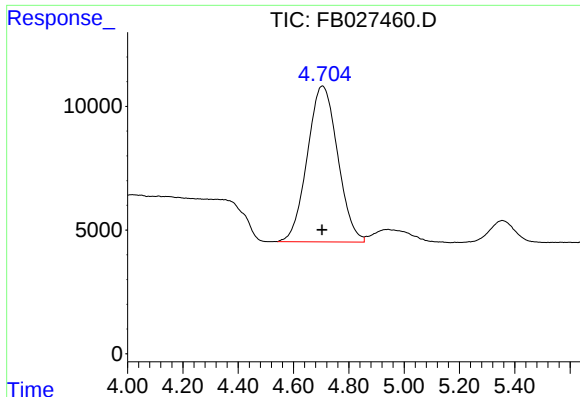

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.001 min
Response: 481963
Conc: 28.61 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0620S1

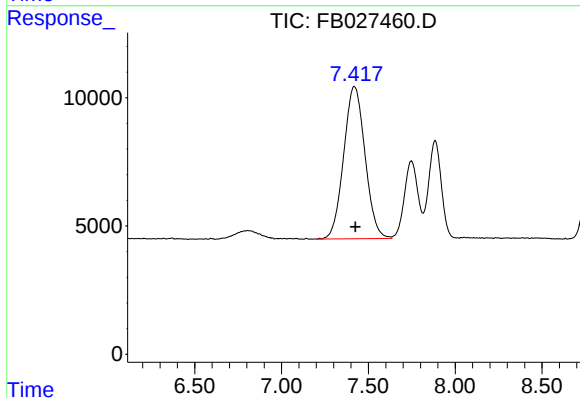


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.008 min
Response: 508075
Conc: 28.94 ng/ml

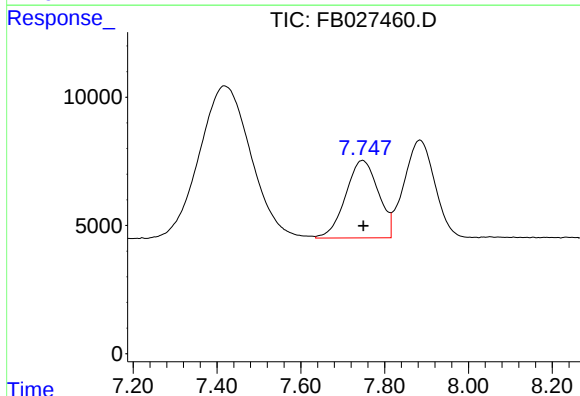


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.001 min
Response: 164035
Conc: 9.36 ng/ml

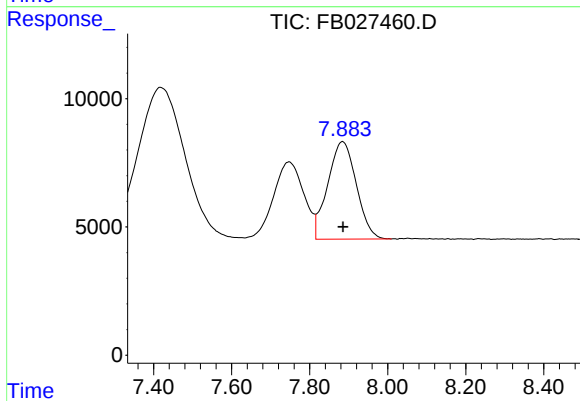

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 193624
Conc: 9.49 ng/ml

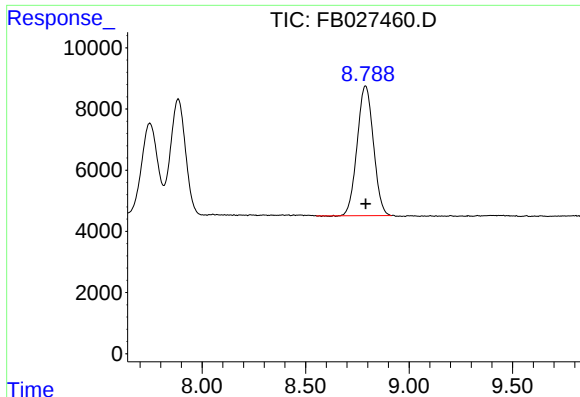

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.001 min
Response: 231284
Conc: 20.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0620S1

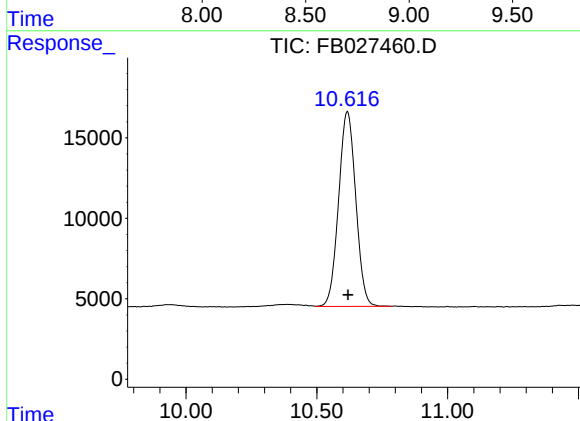


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.002 min
Response: 551573
Conc: 28.49 ng/ml

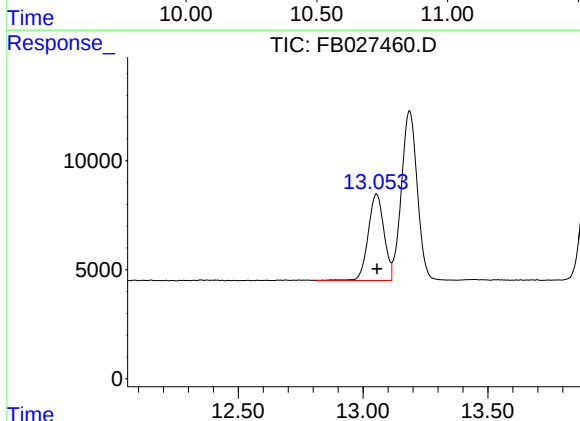


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.002 min
Response: 175016
Conc: 9.66 ng/ml

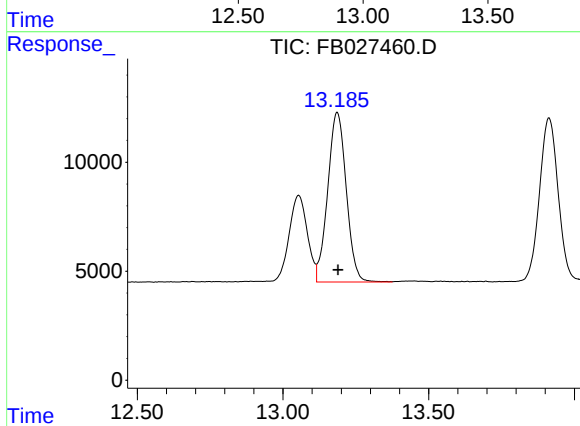

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.003 min
Response: 344307
Conc: 19.31 ng/ml

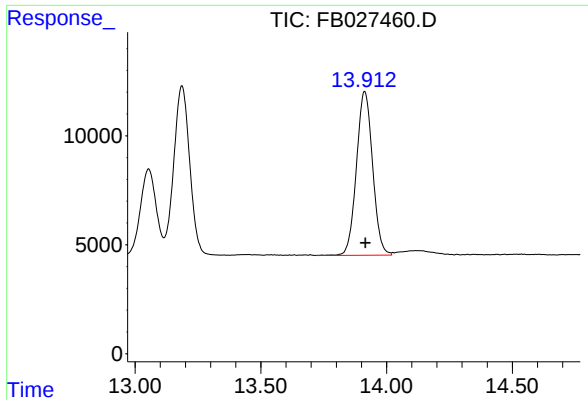

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.003 min
Response: 335243
Conc: 19.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0620S1

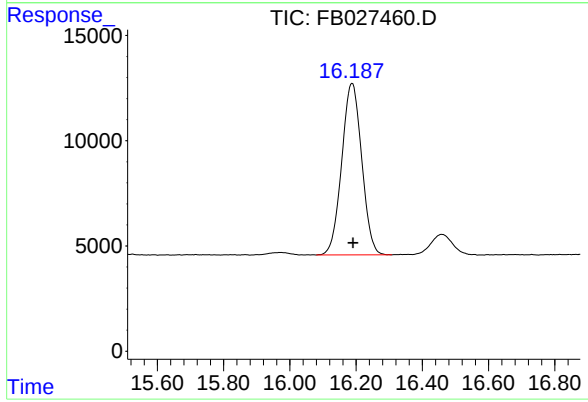

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.003 min
Response: 341378
Conc: 19.87 ng/ml